



**PRODUCT PERFORMANCE TESTING LABORATORY**  
100 Clemson Research Blvd., Anderson, SC 29625  
**Phone** 864.646.8453 **Fax** 864.646.2821  
**Email** [testing@tcnatile.com](mailto:testing@tcnatile.com) **Web** [www.TCNAtile.com](http://www.TCNAtile.com)

---

June 8, 2017

Regan Scientific Instruments  
Attn: Peter Ermish  
901 S. Kimball Ave.  
Southlake, TX 76092

Dear Mr. Ermish,

Tile Council of North America has tested the device you submitted. Test report TCNA-892-16 is enclosed. If you have any questions or concerns, please contact us.

Best Regards,

TILE COUNCIL OF NORTH AMERICA, INC.

Katelyn Simpson  
Laboratory Manager  
Enclosures



**TCNA TEST REPORT NUMBER:**

**TCNA-892-16**

**PAGE: 1 OF 5**

**TEST REQUESTED BY:**

**Regan Scientific Instruments**

**ASTM F2508-16 "Standard Practice for Validation, Calibration, and Certification of Walkway Tribometers Using Reference Surfaces" – Walkway Tribometer Validation**

Informal Test Method Description: This practice provides a procedure and suite of reference surfaces to validate a walkway tribometer by properly ranking and differentiating the surfaces.

This summary is provided for the reader's convenience and is not a complete description of the method. See ASTM F2508 for all method details and information.

**TRIBOMETER TESTED:** Model Name: BOT 3000E

Tribometer Serial #: VS901265800358

Calibration Due Date: 11/03/2017

Test Foot: Sensor #03298, SBR rubber, approximately 1"x1", manufactured: 12/21/2015

**TEST DATE:**

1/24/2017

**TEST PROCEDURE NOTES:**

- The reference surfaces RS A, RS B, RS C, and RS D were obtained from ASTM in February 2011. The surfaces have been maintained in a temperature and humidity controlled environment and are in acceptable condition for testing.
- The tiles were cleaned according to section 8.2.1 of ASTM F2508 prior to testing.
- The SBR sensor was resurfaced according to the sensor resurfacing procedure found in ANSI A137.1, section 9.6.1.3. Throughout testing, the sensor was resurfaced every four measurements as specified in ANSI A137.1.
- Testing was conducted in a temperature and humidity controlled laboratory maintained at 70°F - 77°F and 50% ± 5% relative humidity.
- Each reference surface was tested according to the procedure in ASTM F2508.
  - RS A was tested in the wet condition with 0.04% by volume solution of Triton X-100, and the other three reference surfaces were tested in the wet condition with de-ionized water.
  - 24 measurements were made on each surface, 6 measurements in each of 4 orthogonal directions.

**TEST RESULTS:**

Reference Surface Results (based on 24 measurements)				
	RS A	RS B	RS C	RS D
Mean	0.22	0.26	0.40	0.79
SD	0.03	0.02	0.02	0.01
SE	0.007	0.005	0.004	0.002
CI -	0.20	0.25	0.39	0.79
CI +	0.23	0.27	0.40	0.80

Differences Between Adjacent Ranked Surfaces (based on 24 pairs)			
	RS A - RS B	RS B - RS C	RS C - RS D
Mean Difference	-0.04	-0.14	-0.40
SD	0.025	0.034	0.021
t	7.727	20.143	91.890

Note: All descriptions of calculations can be found in ASTM F2508. SD: Standard Deviation, SE: Standard Error of the Mean, CI +/-: 95<sup>th</sup> percentile confidence intervals, t: paired t-test value

TCNA TEST REPORT NUMBER:

TCNA-892-16

PAGE: 2 OF 5

## CONCLUSIONS:

*Rank Order:* ASTM F2508, section 9.2.1 states that the rank order of the mean walkway tribometer results shall be RS A < RS B < RS C < RS D.

The BOT 3000E (Serial #: VS901265800358) ranked the reference surfaces in the following order, RS A (0.22) < RS B (0.26) < RS C (0.40) < RS D (0.79)

*Differentiation:* ASTM F2508, section 9.2.2 states that using the mean and standard deviation, paired *t*-tests shall produce significantly different results for all adjacently ranked reference surfaces, that is between RS A and RS B, RS B and RS C, and RS C and RS D. As stated in Annex A2 of ASTM F2508, the *t* critical value is 1.714 which assumes one-tailed *t* test (used when there is an expectation of a significant difference between groups), 23 degrees of freedom (number of pairs -1), and 0.05 level of significance. A calculated *t* value greater than or equal to 1.714 indicates a statistically significant difference exists between reference surfaces.

The calculated paired *t*-test results for the measurements with the BOT 3000E (Serial #: VS901265800358) were as follows:

RS A – RS B, *t*=7.727

RS B – RS C, *t*=20.143

RS C – RS D, *t*=91.890

Based on the results above, the BOT 3000E (Serial #: VS901265800358) met the requirements established in ASTM F2508 for walkway tribometer validation.

## IMAGES:



Image 1: BOT 3000E (Serial #: VS901265800358)

TCNA TEST REPORT NUMBER:

TCNA-892-16

PAGE: 3 OF 5

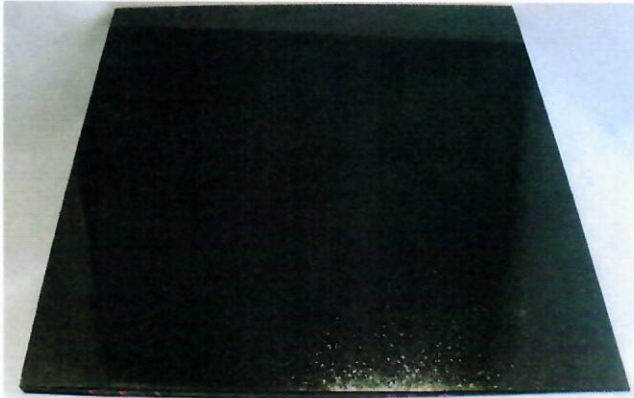


Image 2: Reference Surface A



Image 3: Reference Surface B



Image 4: Reference Surface C



Image 5: Reference Surface D



**TCNA TEST REPORT NUMBER:**

**TCNA-892-16**

**PAGE: 4 OF 5**

**RAW DATA:**

	RSA	RSB	RSC	RSD
1	0.28	0.28	0.41	0.77
2	0.26	0.24	0.43	0.81
3	0.21	0.25	0.38	0.77
4	0.21	0.24	0.41	0.80
5	0.26	0.24	0.39	0.80
6	0.21	0.26	0.44	0.81
7	0.18	0.23	0.39	0.80
8	0.19	0.23	0.40	0.80
9	0.25	0.29	0.42	0.79
10	0.23	0.26	0.42	0.80
11	0.18	0.25	0.38	0.78
12	0.19	0.25	0.41	0.80
13	0.25	0.29	0.36	0.78
14	0.25	0.29	0.41	0.79
15	0.20	0.23	0.37	0.79
16	0.20	0.23	0.39	0.78
17	0.24	0.28	0.37	0.78
18	0.20	0.24	0.40	0.79
19	0.19	0.26	0.39	0.80
20	0.18	0.25	0.42	0.77
21	0.27	0.31	0.36	0.80
22	0.20	0.28	0.39	0.79
23	0.18	0.22	0.38	0.80
24	0.18	0.23	0.39	0.79

**DISCLAIMER AND LIMITATION OF LIABILITY**

This report is provided for the sole use of the client and no one else. It is intended for professional use by a knowledgeable professional. If published by the client, it must be published in full, including this disclaimer and limitation of liability.

This report is not an endorsement, recommendation, approval, certification, or criticism by TCNA of any particular product or its application. TCNA recommends that anyone considering the use or installation of a particular product consult with the manufacturer or an industry professional for advice specific to the person's needs and consider any applicable laws, statutes, codes, or regulations relevant to the particular product. TCNA does not know all the different manners and applications in which a client's particular product might be used, and, therefore, it disclaims any and all duty to provide warnings or to further investigate the suitability of the use of a particular product in a particular situation.

**PRODUCT PERFORMANCE TESTING LABORATORY**

100 Clemson Research Blvd., Anderson, SC 29625

Phone 864.646.8453 Fax 864.646.2821

Email [testing@tcnatile.com](mailto:testing@tcnatile.com) Web [www.TCNAtile.com](http://www.TCNAtile.com)**TCNA TEST REPORT NUMBER:****TCNA-892-16****PAGE: 5 OF 5**

Unless otherwise expressly stated, TCNA tested the specific test subject material provided by the client and identified in the lab report, as indicated by the client. TCNA does not independently verify the information provided by the client, and it makes no representation that similar results would be achieved with other, untested materials, even if such other materials purportedly have the same product name, are purportedly of the same or similar type of tile or product made by the client, or are purportedly from the same batch of tile or product. Nor does TCNA state that the date in this report is representative of production occurring at the same time or at any other time. Only the manufacturer may make that claim, based on sampling and quality control parameters beyond the knowledge and control of TCNA. TCNA does not provide any supervision, review, management, or quality control of any manufacturer's production.

TCNA makes no representation that the client's products are uniform or identical to the test subject material, that the test subject material is suitable for any particular use, application, or installation, or that it will exhibit the same properties when installed or used in a particular manner. The data provided in this report results from standardized laboratory testing performed under laboratory conditions. As such it does not represent all conditions under which the products may be used or subjected. For testing on actual materials being used or considered for a job site, contact TCNA for sampling provisions and possible testing.

This report is intended solely to provide the results of the test procedure stated above as performed on the test subject material provided by the client, and may not be relied on for any other purpose. TCNA MAKES NO OTHER REPRESENTATIONS OR WARRANTIES OF ANY KIND, WHETHER EXPRESS OR IMPLIED. ALL IMPLIED WARRANTIES, INCLUDING, WITHOUT LIMITATION, IMPLIED WARRANTIES OF MERCHANTABILITY, OR FITNESS FOR A PARTICULAR PURPOSE, ARE HEREBY EXPRESSLY DISCLAIMED. IN THE EVENT OF A DISPUTE CONCERNING THIS REPORT, THE EXCLUSIVE REMEDY FOR CLIENT SHALL BE FOR TCNA TO REPEAT THE TEST REQUESTED, BUT IN NO EVENT SHALL TCNA BE LIABLE FOR AN AMOUNT GREATER THAN THE AMOUNT IT RECEIVED FROM CLIENT FOR THE TEST. UNDER NO CIRCUMSTANCES WILL TCNA BE LIABLE TO CLIENT FOR ANY OTHER DAMAGES (NOR SHALL IT BE LIABLE TO ANY OTHER PERSON OR BUSINESS ENTITY FOR ANY DAMAGES), INCLUDING WITHOUT LIMITATION ANY AND ALL DIRECT, INDIRECT, SPECIAL, INCIDENTAL, CONSEQUENTIAL, OR EXEMPLARY DAMAGES, RESULTING, IN WHOLE OR IN PART, FROM ANY USE OF, REFERENCE TO, OR RELIANCE UPON THE REPORT, EVEN IF ADVISED OF THE POSSIBILITY OF SUCH DAMAGES. TCNA DISCLAIMS ALL LIABILITY TO ANY THIRD PARTY CONCERNING THIS REPORT. THE FOREGOING LIMITATION OF LIABILITY IS A FUNDAMENTAL ELEMENT OF TCNA'S AGREEMENT TO CONDUCT AND PROVIDE THE REPORT.

6/8/2017

Katelyn Simpson  
Laboratory Manager