


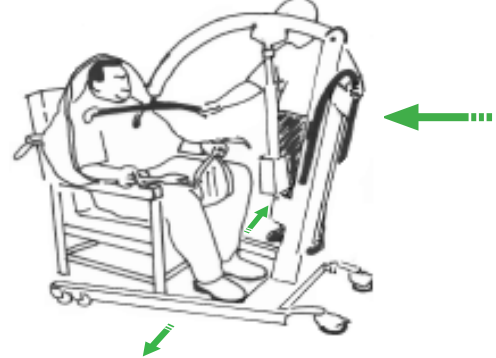
## From chair to chair

**1**




Place sling around patient.  
Place leg straps on the inside of thighs.  
Make sure sling is not folded or twisted.

**2**




Position lift in front of patient. If needed, place patient's legs on or over the chassis.  
Adjust spreader bar to shoulder height.

**3**

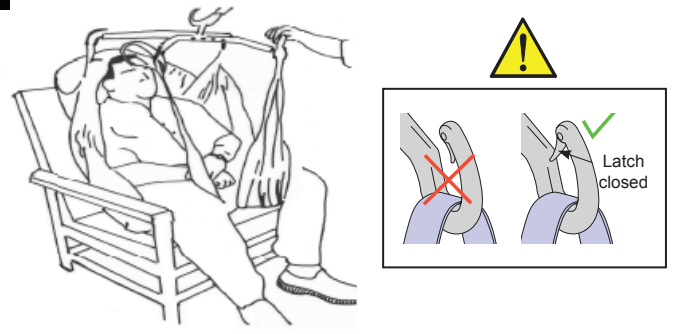


Attach sling loops to spreader bar correctly.  
Make sure sling is secured in the hooks before lifting patient.

**4**

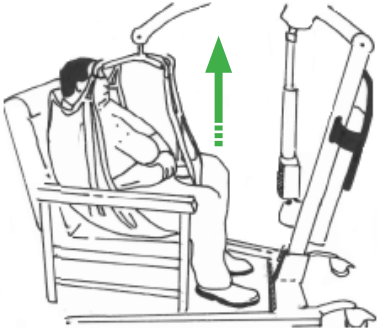


Lift patient.

**5**

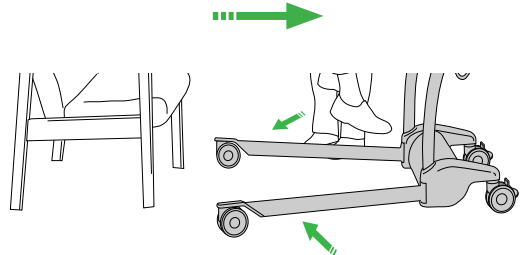

Move lift away from chair.  
If applicable, close chassis legs.  
Transfer patient.

**6**

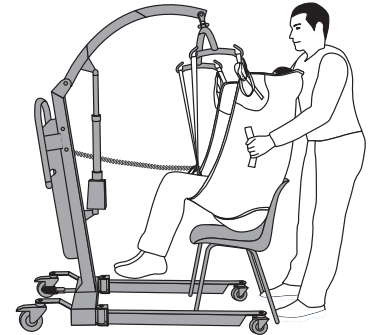

Position patient over chair. Carefully lower to sitting position.  
Detach sling from lift. Move lift away from patient.  
Remove sling from patient.