



Dr. pen X5

USER MANUAL

PLEASE READ THE MANUAL BEFORE USE



Parts Name





How to operate

Wireless Model: Dr pen X5-W

The instrument used with both built-in battery or AC power

Wired Model: Dr pen X5-C

The instrument used with AC power only

1. Plug in DC adaptor to the jack
2. Plug in DC adaptor to AC outlet
3. To charge the battery: Plug the adapter into an outlet and connect it to the power interface



Charging Status


- The power indicator stays red while charging
- The power indicator turns green after charging completed



How to operate

Preparation

1. Take out needles cartridges from the sterilized package
2. Pushing the needle cartridge horizontally into the round slot of pen
3. Assemble the needles cartridges by counterclockwise rotation. Take apart the needles cartridges by clockwise rotation
4. Adjustment of needle length should be done after turning on the machine



5. Start the Dr.pen X5

Press the power button for 2-3 seconds to start or shut down the device

Attention

In order to protect the instrument well, do not invert the instrument to prevent the liquid backflow




How to operate

Adjustment of needle length

Adjust the depth of needle by turning the scale adjustment ring

Turn it clockwise, needle depth will be shorter

Turn it counterclockwise, needle depth will be longer

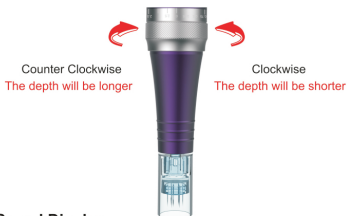

Speed Display




5 Speeds Adjustment

The pen starts from low to high speed

The speed changes once each time you press the button



Needle cartridge introduction





Specification

Product name:

Auto-stamp Motorized Meso Machine

Model name: Dr pen X5

Adapter: 5V-1000mA

Package Weight: 315g

Package Size: 169*123*56mm

Packing List

Item	Quantity
Hand Piece	1 pc
Adapter	1 pc
Manual	1 pc
Power Cable	1 pc
Needle Cartridge	2 pcs



Precaution

	Please be sure to read instructions before use and follow as described.
	Do not apply it to the man as follow: 1. Who has acute disease or bloody disease over 38℃ 2. Who has allergy and hemophilia 3. Who has melanosis of the face 4. Who has high internal heat 5. Who regularly visits hospital 6. Who takes medicines 7. Who is under 12 years old
	Do not use it on the power other than AC 220V. It may cause fires or malfunction
	Do not use it near the place with high temperature, dust or humidity (Near the humidifier). It may cause malfunction.
	Do not repair, disassemble or alter the controller and the body. It may cause malfunction.
	Do not touch the device or detach the power cords with wet hands. It may cause electric shock.
	Do not use the stripped cord or propped cord. It may cause fires(Be sure to replace it with another).
	Do not use the propped cord which has crack or scares. It may cause scares on the skin.
	When you don't use it for a long time, unplug it from the outlet.
	Be sure to have an inspection for test. If any troubles are found, get it repaired.
	No one other than the operator can touch it. It may cause accidents or malfunction.

	Alternating current		Serial No
	Direct current		EU Representative
	Class I equipment		CE mark
	Attention, consult accompanying documents		Manufacturer
	Date of manufacture		Floating applied part



Warranty

The warranty period of Dr pen X5 is 6 months. We offer repair to our products from the day they are purchased. If any of our products has damages or natural trouble. We offer repair or replacements

General maintenance

Make sure to inspect the device and adapter before use

Keep it with its power off. Wipe its surface out with a dry cloth

Keep it away from direct sunlight or high temperature and humidity

Do not leave the measurement, repair or alter of the device to non-professional staff

When you use the device which has not been used for a long time, make sure to check if it works properly with safety

Dr.pen X5
USER MANUAL