

1 CLINICIAN REQUIRED

Account Location

PO Number

Clinician

Clinician Email



Tel: 1-877-767-3338
 Fax: 1-866-919-9268
 www.kevinrootmedical.com
 hello@kevinrootmedical.com



A250 Overlap Free Motion AFO

ORDER FORM PAGE 1 OF 1

Contact me to review Order Form Date: MM/DD/YYYY Rush order due date: MM/DD/YYYY

2 PATIENT REQUIRED

Patient's Email

First Name

Last Name

DOB MM/DD/YYYY Sex: M F Weight Height



A250 Overlap Free Motion AFO

- Overlap free motion joints
- 4mm Polypropylene frame
- Rearfoot intrinsic post
- 3mm 30 Shore A EVA top cover
- 2 anterior/1 poster straps
- Medial & lateral upper lining
- Mid fibula height
- Foot frame to metatarsals

3 SIDE

Use separate Rx for each side

Right

Left

IMPRESSION

- Plaster
- STS Casting Socks
- 3D Foot Scanner
- Fiberglass Casting Tape

FITTING

Shoe size:

Fit AFO to submitted:


Tracing

Shoes

4 MODEL HEIGHT & COVER LENGTH REQUIRED

Height:

- A109 - Standard (mid fibula)
- A105 - Short (above malleoli)
- A112 - Tall (to fibula head)

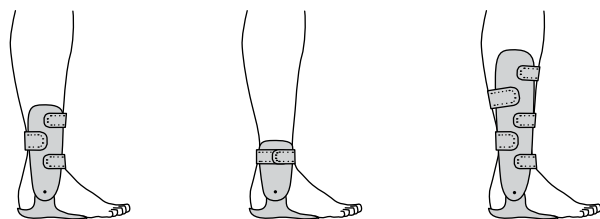

Length of 3mm EVA Cover:

- To Mets
- To Sulcus
- To Toes

A MEASUREMENTS OPTIONAL

Height: Fibula Head Proximal Trim

Circumference: Proximal Trim Above Ankle Ankle Mid-Foot

Forefoot

B PRONATION CORRECTIONS OPTIONAL

	Varus Forefoot Posts	Balance FF to RF	8° <input type="checkbox"/> 6° <input type="checkbox"/> 4° <input type="checkbox"/> 2° <input type="checkbox"/> 90° <input type="checkbox"/>	
		VR Extrinsic (Bar)	6° <input type="checkbox"/> 4° <input type="checkbox"/> 2° <input type="checkbox"/> 0° <input type="checkbox"/>	
		VR Met Wedge	6° <input type="checkbox"/> 4° <input type="checkbox"/> 2° <input type="checkbox"/>	
	Midfoot	Raise Med Arch	6 <input type="checkbox"/> 4.5 <input type="checkbox"/> 3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)	
		Scaphoid Pad	6 <input type="checkbox"/> 4.5 <input type="checkbox"/> 3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)	
		VR Cuboid Pad	6 <input type="checkbox"/> 4.5 <input type="checkbox"/> 3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)	
	Varus Rearfoot Posts	Medial Flange	High <input type="checkbox"/> Medium <input checked="" type="checkbox"/> Low <input type="checkbox"/>	
		VR Intrinsic	6° <input type="checkbox"/> 4° <input type="checkbox"/> 2° <input type="checkbox"/> 0° <input checked="" type="checkbox"/>	
		VR Extrinsic	6° <input type="checkbox"/> 4° <input type="checkbox"/> 2° <input type="checkbox"/> 0° <input type="checkbox"/>	
		Heel Skive	6 <input type="checkbox"/> 4 <input type="checkbox"/> 2 <input type="checkbox"/> (mm)	

C SUPINATION CORRECTIONS OPTIONAL

	Valgus Forefoot Posts	Balance FF to RF	8° <input type="checkbox"/> 6° <input type="checkbox"/> 4° <input type="checkbox"/> 2° <input type="checkbox"/> 90° <input type="checkbox"/>	
		VG Extrinsic (Bar)	6° <input type="checkbox"/> 4° <input type="checkbox"/> 2° <input type="checkbox"/> 0° <input type="checkbox"/>	
		VG Met Wedge	6° <input type="checkbox"/> 4° <input type="checkbox"/> 2° <input type="checkbox"/>	
	Midfoot	Lower Med Arch	6 <input type="checkbox"/> 4.5 <input type="checkbox"/> 3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)	
		Lateral Flange	High <input type="checkbox"/> Medium <input type="checkbox"/> Low <input type="checkbox"/>	
		VG Frame Filler	6° <input type="checkbox"/> 4° <input type="checkbox"/> 2° <input type="checkbox"/> 0° <input type="checkbox"/>	
	Valgus Rearfoot Posts	VG Cuboid Pad	6 <input type="checkbox"/> 4.5 <input type="checkbox"/> 3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)	
		VG Intrinsic	6° <input type="checkbox"/> 4° <input type="checkbox"/> 2° <input type="checkbox"/> 0° <input type="checkbox"/>	
		VG Extrinsic	6° <input type="checkbox"/> 4° <input type="checkbox"/> 2° <input type="checkbox"/> 0° <input type="checkbox"/>	

D EXTENSIONS OPTIONAL

	Toe Length	Toe Extension	Myolite 4.5 <input type="checkbox"/> 3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)	
		Morton's Ext.	U.skiv <input type="checkbox"/> 4.5 <input type="checkbox"/> 3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)	
		Rev. Morton's	U.skiv <input type="checkbox"/> 4.5 <input type="checkbox"/> 3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)	
		Dynamic Wedge	3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)	
	Sulcus Length	Sulcus Extension	Myolite 4.5 <input type="checkbox"/> 3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)	
		Morton's Ext.	U.skiv <input type="checkbox"/> 4.5 <input type="checkbox"/> 3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)	
		Rev. Morton's	U.skiv <input type="checkbox"/> 4.5 <input type="checkbox"/> 3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)	
		Foot Cookie Ext.	Myolite 4.5 <input type="checkbox"/> 3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)	
Partial Foot Toe Filler	Toe Filler <input checked="" type="checkbox"/>	5 th <input type="checkbox"/> 4 th <input type="checkbox"/> 3 rd <input type="checkbox"/> 2 nd <input type="checkbox"/> 1 st <input type="checkbox"/>		

E OFFLOADING PADS & CUSHIONS OPTIONAL

	Forefoot	Met Balance <input checked="" type="checkbox"/>	5 th <input type="checkbox"/> 4 th <input type="checkbox"/> 3 rd <input type="checkbox"/> 2 nd <input type="checkbox"/> 1 st <input type="checkbox"/>	
		Met Punch <input checked="" type="checkbox"/>	5 th <input type="checkbox"/> 4 th <input type="checkbox"/> 3 rd <input type="checkbox"/> 2 nd <input type="checkbox"/> 1 st <input type="checkbox"/>	
		Met Pad 2-4	4.5 <input type="checkbox"/> 3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)	
		Met Bar 1-5	4.5 <input type="checkbox"/> 3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)	
		Dancer's Pad	4.5 <input type="checkbox"/> 3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)	
	Midfoot	Cuboid Offload	6 <input type="checkbox"/> 4.5 <input type="checkbox"/> 3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)	
		Rearfoot	Heel Cushion	6 <input type="checkbox"/> 4.5 <input type="checkbox"/> 3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)
		Heel Spur Pad	6 <input type="checkbox"/> 4.5 <input type="checkbox"/> 3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)	
	Device Length	Myolite Layer	4.5 <input type="checkbox"/> 3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)	
		Cushion	Plastazote Layer	6 <input type="checkbox"/> 4.5 <input type="checkbox"/> 3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)

F FRAME MODIFICATIONS OPTIONAL

	Forefoot	1 st Ray Cut Out	Full <input type="checkbox"/> 65° <input type="checkbox"/> 45° <input type="checkbox"/>	
		5 th Ray Cut Out	65° <input type="checkbox"/> 45° <input type="checkbox"/>	
	Midfoot	Navicular B. Out	6 <input type="checkbox"/> 4.5 <input type="checkbox"/> 3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)	
		5 th Button Out	6 <input type="checkbox"/> 4.5 <input type="checkbox"/> 3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)	
	Rearfoot	Heel Lift	6 <input type="checkbox"/> 4.5 <input type="checkbox"/> 3 <input type="checkbox"/> 1.5 <input type="checkbox"/> (mm)	
		Heel Lift Tapered	26 <input type="checkbox"/> 22 <input type="checkbox"/> 18 <input type="checkbox"/> 14 <input type="checkbox"/> 10 <input type="checkbox"/> (mm)	
		Heel Cup Depth	30 <input type="checkbox"/> 24 <input type="checkbox"/> 18 <input type="checkbox"/> 12 <input type="checkbox"/> 6 <input type="checkbox"/> (mm)	

Special Instructions:

