















Green light: normal temp

32°C-37.5°C

Yellow light: low fever warning

37.6°C-38.1°C

Red light: High fever alarm

38.2°C-42.9°C





## SWITCH MODE CELSIUS/FAHRENHEIT BY ONE BUTTON

Suitable for the habit around the world



## PRODUCT DETAILS



Product size:128MM\*70MM\*300MM

Product material :ABS+PC

Max power:3W

Power supply:4AA battery or DC5V 2.1A

Temperature taking mode: infrared induction

Temperature measuring distance: 1-5M

Temperature measurement:  $(32^{\circ}\text{C} \sim 42.9^{\circ}\text{C}, 89.6^{\circ}\text{F} \sim 109.2^{\circ}\text{F})$ 

Temperature measuring time:2 second

Error: ±0.2°C

Bottle capacity:300ML


Types of liquid:hand sanitizer;


Liquid way: infrared induction

Working environment:  $1^{\circ}$  ~35  $^{\circ}$  (33.8  $^{\circ}$  F ~95  $^{\circ}$ F); humidity < 85%

Storage environment:-20  $^{\circ}$ C ~55  $^{\circ}$ C (-4  $^{\circ}$ F ~131  $^{\circ}$ F);humidity < 85%

Temperature unit: Celsius (°C)/Fahrenheit (°F)

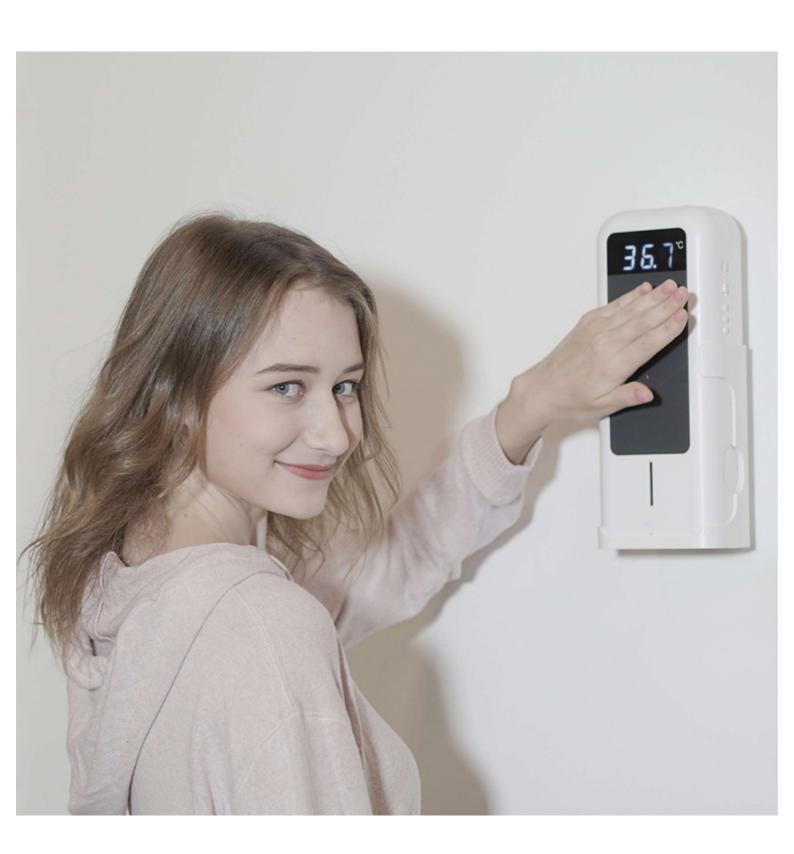

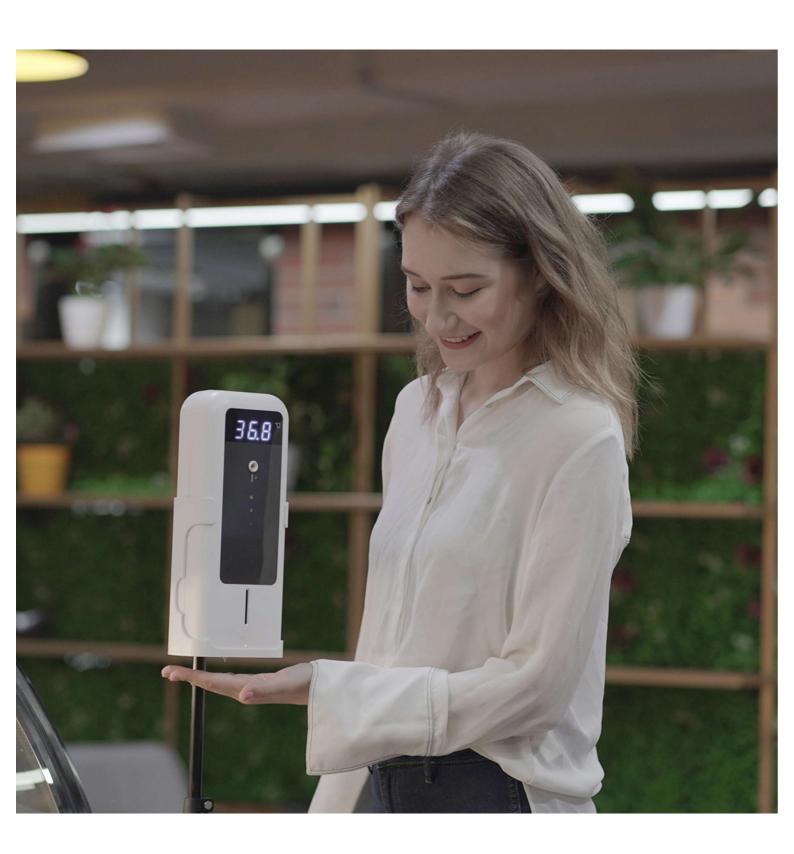

## Disinfectant replacement step

• 0 •



Remove the device and open the back cover






Align the bottle with the interface after liquid adding is complete



Press down the bottle and put on the back cover, replace complete


## Hanging installation

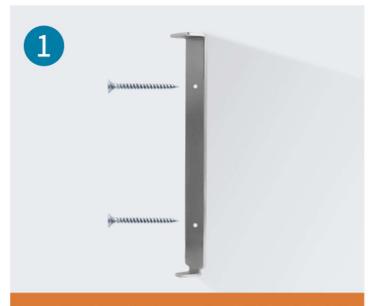

Fix the wall hanging bracket to the wall with screws



Put on the housing

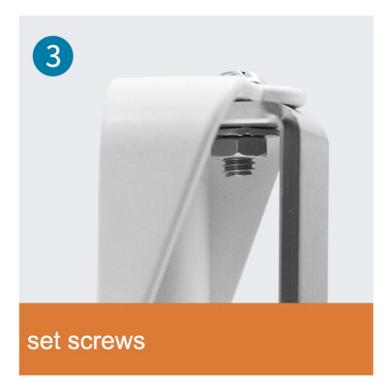



housing and the start work