



TECHNICAL SPECIFICATIONS

| | |
|--------------------------------|--|
| Instrument Type | 12-lead resting electrocardiograph |
| Input Channels | Simultaneous acquisition of all 12 leads |
| Standard Leads Acquired | I, II, III, aVR, aVL, aVF, V1, V2, V3, V4, V5, V6 |
| Frequency Response | 0.05 Hz - 300 Hz |
| Gain | 2.5, 5, 10, 20 mm/mV |
| Filters | AC filter: None, 50 Hz, 60 Hz Low-pass filters: 40 Hz, 150 Hz, 300 Hz |
| Digital Sampling Rate | 40,000 samples/sec/channel used for pacemaker spike detection 1,000 samples/sec/channel used for recording and analysis |
| Report Formats | Standard or Cabrera; 3+1, 3+3, 6, 6+6, or 12 channel |
| Acquisition Device | Welch Allyn Wireless Acquisition Module or Welch Allyn AM™12 Acquisition Module |
| Storage Capacity | Unlimited with external archive |

MINIMUM STANDALONE/CLIENT SPECIFICATIONS

| | | |
|--|--|------------------------|
| Operating Systems | Microsoft® Windows® 7 Professional (32-bit* or 64-bit) Microsoft Windows 10 Professional (64-bit) Note: If installing ELI™ Link with Diagnostic Cardiology Suite, system requires 64-bit OS to operate both. | |
| Compatible Viewing Resolutions and Font Scaling | Resolutions | Font scaling |
| | 1024×768, 1366×768, 1280×800 | 100% |
| | 1680×1050, 1920×1080, 1920×1200 | 100%, 125%, 150% |
| | 2736×1824 | 100%, 125%, 150%, 200% |
| Processor | Performance equivalent or better than an Intel® Core™ i3 | |
| RAM | Minimum 4 GB | |
| Hard Drive Capacity | Minimum 250 GB (If client: minimum 160 GB) | |
| Archive | Network or external USB drive | |
| Software Installation | DVD | |
| Network | 100 Mbps connection or better | |
| USB Ports | Requires at least two USB 2.0 ports (WAM/AM12 modules, external USB drive) | |
| Input Devices | Standard keyboard, mouse, ECG acquisition input device (e.g. WAM, AM12 modules) | |
| Printing Device | HP M501dn Windows Printer with HPUPD PCL5 driver or equivalent | |

MINIMUM SERVER REQUIREMENTS

| | |
|-------------------------|---|
| Instrument Type | Performance equivalent to an Intel Xeon® class, quad-core with hyperthreading |
| Resolution | 1024x768 or better |
| RAM | Minimum 4 GB |
| Operating System | Microsoft Windows 2012 R2 (64-bit) Microsoft Windows Server 2016 |
| System Disk | 100 GB for OS and product installation (RAID recommended for data redundancy) |
| Data Disks | 550 GB hard drive space available HD controller with 128 MB read/write cache (RAID recommended for data redundancy) |

MINIMUM CITRIX® XENAPP® REQUIREMENTS

| | |
|---|---|
| Client Machines That Run Citrix XenApp | Microsoft Windows 7 Professional (64-bit and 32-bit) Microsoft Windows 10 Professional (64-bit) Citrix Receiver Any internet browser supported by Citrix |
| Citrix Desktop Delivery Controller | Citrix XenApp version 7.13 Any operating system supported by Citrix |
| Citrix App Servers | Microsoft Windows 2012 R2 (64-bit) Microsoft Windows 2016 Server R2 (64-bit) Citrix Virtual Delivery Agent 7.13 |

MINIMUM WINDOWS RDP REQUIREMENTS


| | |
|--|--|
| Thin Clients Using Windows RDP | Microsoft Windows 7 Professional (64-bit and 32-bit) Microsoft Windows 10 Professional (64-bit) |
| Operating Systems for Servers Running Windows RDP | Microsoft Windows 2016 Server R2 (64-bit) Microsoft Windows 2012 R2 (64-bit) |

To order, or for more information, please contact:

docStock
com.au

Ph: (02) 8850 7177 Fax: (02) 8850 7988
email: info@docstock.com.au
www.docstock.com.au [...medical products online]

For more information, please contact your local distributor or Hillrom sales representative at 1-800-535-6663.

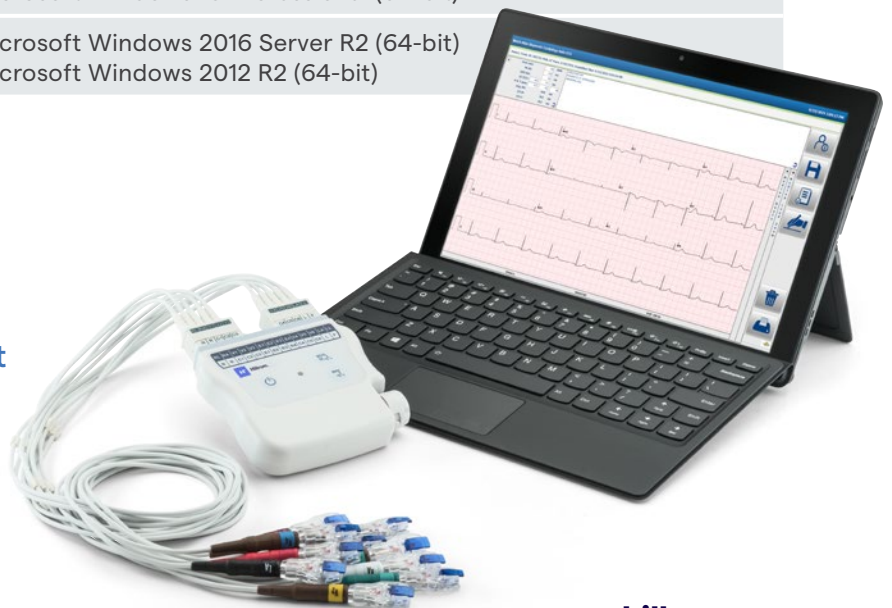

hillrom.com

*If using EMR interface, font scaling may vary. If installing ELI Link with Diagnostic Cardiology Suite, system requires 64-bit OS to operate both. Specifications are subject to change without notice.