


## Certificate of Anaysis and Conformity Syringe Filters

## PES 0.45 µm 25 mmØ. Lot. 275008

Test	Specification	Result
Visual inspection	Absence of external visual defects	Pass
Luer-lock	Enhanced Luer-Lock (ISO 594-1)	Pass
Filter integrity	Sample clarification by filtration test	Pass
Bubble point	>280 kPa	333
Ext. Dimensions	31.9±0.5 mmØ x 25.7±0.5 mm (height)	Pass
Water Flow Rate	>15 ml/min.cm2 (at 25°C 0.7bar)	44,8
UV extractable	According conditions specified below. Absorbance at:	Water
	214 < 0.04 AU	0,0150
	254 < 0.04 AU	0,0004
	280 < 0.04 AU	0.0001

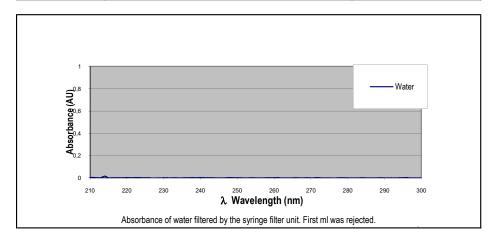

This product complies all procedures, manufacturing specifications and quality controls for release.

Signed Quality Manager June 3, 2021

Product manufactured in compliance with ISO 9001 and technical procedures. Inspection document 2.2 according EN 10204:2004



Essex Scientific Laboratory Supplies Limited 356-358 Prince Avenue, Westcliff-on-Sea, Essex,SSO ONF, United Kingdom