



中国认可  
国际互认  
检测  
TESTING  
CNAS L0608

# 天纺标检测认证股份有限公司

TianFangBiao Standardization Certification & Testing Co.,Ltd.

国家服装质量监督检验中心 (天津)

National Clothing Quality Inspection & Supervision Center(Tianjin)

国家针织产品质量质量监督检验中心

National Knitted Product Quality Inspection & Supervision Center


# 检验检测报告

Test Report



T T T S - W F 2 1 0 0 2 5 9 5 - 0 1

Information Provided by Client	Applicant	ZHEJIANG DIANFENG INDUSTRIAL CO., LTD.		Contact	/
		NO. 602 CUIWEI ROAD, CAOZHAI TOWN, JINDONG DISTRICT, JINHUA CITY, ZHEJIANG CHINA		Tel.	/
	Manufacturer	ZHEJIANG DIANFENG INDUSTRIAL CO., LTD.			
		NO. 602 CUIWEI ROAD, CAOZHAI TOWN, JINDONG DISTRICT, JINHUA CITY, ZHEJIANG CHINA			
	Information of Submitted Sample	Sample Name	KN95 Protective Mask	Trademark	SUMMIT PERSON
Sample Count		100 Piece(s)			
Size or Specification		/	Colour	/	
Quality Grade		/	Safety Category	/	
	Style No. or Order No.	M9502			
Test Standards	GB 2626-2019 Respiratory protection-Non-powered air-purifying particle respirator				
Test Part Description	1# Mask				
Test Type	Commission Test	Date of Submission	2021-05-19	Date of Checking	2021-05-26
Test Date	2021-05-19		To	2021-05-24	
Test Standards	See next page(s)				
Conclusion	As we have tested the sample(s) received, the test items can confirm to the standard GB 2626-2019, please refer to next page(s).				
Remarks	/				

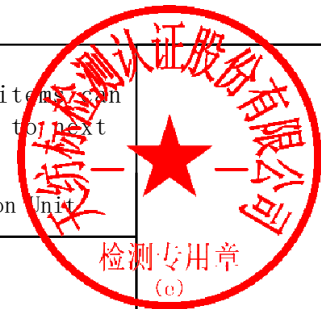

Approver

方倩

Checker

于洋

Editor

岳玉婷



中国认可  
国际互认  
检测  
TESTING  
CNAS L0608

**天纺标检测认证股份有限公司**  
TianFangBiao Standardization Certification & Testing Co.,Ltd.

**国家服装质量监督检验中心 (天津)**

National Clothing Quality Inspection & Supervision Center(Tianjin)

**国家针织产品质量质量监督检验中心**

National Knitted Product Quality Inspection & Supervision Center

**检验检测报告**  
Test Report

TTS-WF21002595-01

Page 2 of 5

Test Items	Description	Unit	Standard Requirement	Results	Conclusions	Test Method/Remarks
1# Mask						
Respiratory Resistance	Expiratory Resistance	Pa	≤210	Samples Without Pretreatment: 1: 97 2: 98 Samples With Pretreatment: 1: 89 2: 87	Pass	GB 2626-2019
	Inspiratory Resistance	Pa	≤210	Samples Without Pretreatment: 1: 105 2: 106 Samples With Pretreatment: 1: 99 2: 95		
Flammability	Afterflame Time	s	≤5	0	Pass	GB 2626-2019
Dead Space	---	%	≤1	0.9	Pass	GB 2626-2019
Filtration Efficiency (KN95)	NaCl Particle	%	≥95.0	Samples Without Pretreatment: 1: 99.86 2: 99.83 3: 99.78 4: 99.74 5: 99.81 6: 99.75 7: 99.80 8: 99.69 9: 99.84 10: 99.76 11: 99.67 12: 99.70 13: 99.85 14: 99.82 15: 99.68 Samples With Pretreatment: 1: 99.56 2: 99.49 3: 99.60 4: 99.42 5: 99.57	Pass	GB 2626-2019



中国认可  
国际互认  
检测  
TESTING  
CNAS L0608

**天纺标检测认证股份有限公司**  
TianFangBiao Standardization Certification & Testing Co.,Ltd.

**国家服装质量监督检验中心 (天津)**

National Clothing Quality Inspection & Supervision Center(Tianjin)

**国家针织产品质量质量监督检验中心**

National Knitted Product Quality Inspection & Supervision Center

**检验检测报告**  
Test Report

TTTS-WF21002595-01

Page 3 of 5

Test Items	Description	Unit	Standard Requirement	Results							Conclusions	Test Method/Remarks	
1#	Mask												
Leakage (KN95)	/	/	Based on the evaluation of TIL for each action, at least 46 of the 50 actions, the TIL is less than 11%. Based on the evaluation of the TIL for total person, at least 8 of the 10 person being tested, the total TIL is less than 8%.	Tester	D1 (%)	D2 (%)	D3 (%)	D4 (%)	D5 (%)	TIL (%)	Pass	GB 2626-2019	
				Without Pretreatment	1	6.8	7.2	7.0	7.7	7.4			7.2
					2	7.0	7.3	7.2	8.2	7.1			7.4
					3	5.5	6.5	6.2	7.3	6.8			6.5
					4	5.7	6.3	7.1	8.5	7.0			6.9
					5	7.1	7.3	8.2	9.0	7.6			7.8
				With Pretreatment	6	6.1	6.8	6.5	8.4	6.5			6.9
					7	7.5	7.8	7.6	8.0	7.7			7.7
					8	6.1	7.1	7.0	7.7	6.3			6.8
					9	7.1	7.0	7.6	7.7	6.3			7.1
10	6.3	6.9	6.6		8.2	8.1	7.2						

Blank Part Below



中国认可  
国际互认  
检测  
TESTING  
CNAS L0608

**天纺标检测认证股份有限公司**  
TianFangBiao Standardization Certification & Testing Co.,Ltd.

**国家服装质量监督检验中心 (天津)**  
National Clothing Quality Inspection & Supervision Center(Tianjin)  
**国家针织产品质量质量监督检验中心**  
National Knitted Product Quality Inspection & Supervision Center

# 检验检测报告

Test Report

TTTS-WF21002595-01

Page 4 of 5

## Sample





中国认可  
国际互认  
检测  
TESTING  
CNAS L0608

**天纺标检测认证股份有限公司**  
TianFangBiao Standardization Certification & Testing Co.,Ltd.

**国家服装质量监督检验中心 (天津)**

National Clothing Quality Inspection & Supervision Center(Tianjin)

**国家针织产品质量质量监督检验中心**

National Knitted Product Quality Inspection & Supervision Center

# 检验检测报告

Test Report

TTTS-WF21002595-01

Page 5 of 5

## Sample

