



# LDSBus EC Sensor Adapter Datasheet



## 1 Introduction

The LDSBus Electrical Conductivity (EC) Sensor Adapter is designed to work with EC probes to form a complete EC sensor. The adapter consists of built-in BNC connector used to attach EC probes.

The adapter and probe are calibrated using a two-point calibration procedure and the resulting sensor supports EC measurements ranging from 0.001mS/cm to 150mS/cm with a 0.001 mS/cm resolution.

The sensor is suitable for use in measuring salts, nutrients, and impurities in water in hydroponics, aquaponics and aquaculture and freshwater systems. Monitoring, alerting, and controlling the system can be done in real-time.

### 1.1 Features

- Supports Probe Cell Constant  $K=0.1$ ,  $K=1.0$  and  $K=10$  probes with BNC connectors
- Measures EC range of 0.001mS/cm to 150mS/cm with linearized output and 0.001mS/cm resolution
- 2 Point step-by-step guided calibration
- BRTSys's LDSBus protocol. Wired data/power transmission through LDSBus HVT-Junction
- High report rate of 1 report every 5 seconds
- Low power consumption 5V-91mW
- Operating temperature range: 0°C to +70°C
- Flush Mount and DIN Rail Mount options
- Supported platform applications: BRTSys's IoTPortal and LDSBus Python SDK. Visit <https://brtsys.com/resources> for more information.



Neither the whole nor any part of the information contained in, or the product described in this manual, may be adapted, or Reproduced in any material or electronic form without the prior written consent of the copyright holder. This product and its documentation are supplied on an as-is basis and no warranty as to their suitability for any particular purpose is either made or implied. BRT Systems Pte Ltd will not accept any claim for damages howsoever arising as a result of use or failure of this product. Your statutory rights are not affected. This product or any variant of it is not intended for use in any medical appliance, device, or System in which the failure of the product might reasonably be expected to result in personal injury. This document provides preliminary information that may be subject to change without notice. No freedom to use patents or other intellectual property rights is implied by the publication of this document. BRT Systems Pte Ltd, 178 Paya Lebar Road, #07-03, Singapore 409030. Singapore Registered Company Number: 202220043R

## 2 Part Numbers

Part#	Naming
LS050101A	LDSBus EC Sensor Adapter
LA120101A	LDSBus DIN Rail Mount Set

## Table of Contents


<b>1</b>	<b>Introduction .....</b>	<b>1</b>
<b>2</b>	<b>Part Numbers .....</b>	<b>2</b>
<b>3</b>	<b>Product Specifications.....</b>	<b>4</b>
<b>4</b>	<b>Hardware Features.....</b>	<b>5</b>
<b>5</b>	<b>Sensor Configuration and Installation .....</b>	<b>6</b>
5.1	Connection Diagram.....	6
<b>6</b>	<b>Mounting Options .....</b>	<b>7</b>
6.1	Flush Mount .....	7
6.2	DIN Rail Mount.....	7
<b>7</b>	<b>System Status LED Indicators .....</b>	<b>8</b>
<b>8</b>	<b>Probe Selection .....</b>	<b>9</b>
<b>9</b>	<b>Mechanical Dimension.....</b>	<b>10</b>
<b>10</b>	<b>Contact Information.....</b>	<b>11</b>
<b>Appendix A – References .....</b>		<b>12</b>
	Document References .....	12
	Acronyms and Abbreviations .....	12
<b>Appendix B – List of Figures and Tables.....</b>		<b>13</b>
	List of Figures .....	13
	List of Tables .....	13
<b>Appendix C – Revision History .....</b>		<b>14</b>

### 3 Product Specifications

<b>Features</b>	Interface	BNC – EC probe connector RS485 – LDSBus communication
	LED Indicator (RGB)	System Status Indicator (Please refer to <a href="#">LED section</a> )
	Mounting	Flush Mount
DIN Rail Mount		
<b>Power</b>	Input Voltage	5V DC Bus Power
	Typical Power	5V, 91mW
	Max. Power	266mW
<b>EC Sensor input module</b>	Detection Range	0.001 – 150mS/cm
	Resolution	0.001mS/cm
	Response Time	<1Minute
	Calibration	2 Point Calibration
<b>Physical Characteristics</b>	Color	White
	Housing	Polycarbonate
	Dimensions	L117.6mm x W42.9mm x H29.7mm
<b>Environmental Limits</b>	Operating Temperature	0 to 70°C
	Storage Temperature	-20 to 85°C
	Ambient Relative Humidity	5 to 95% (non-condensing)
<b>Package Contents</b>	Device	1x LDSBus EC Sensor Adapter
	Installation (Optional)	1x DIN Rail Bracket set
	Wire Assembly	1X 5m RJ11 Cable

**Table 1 - LDSBus EC Sensor Adapter Specifications**

## 4 Hardware Features

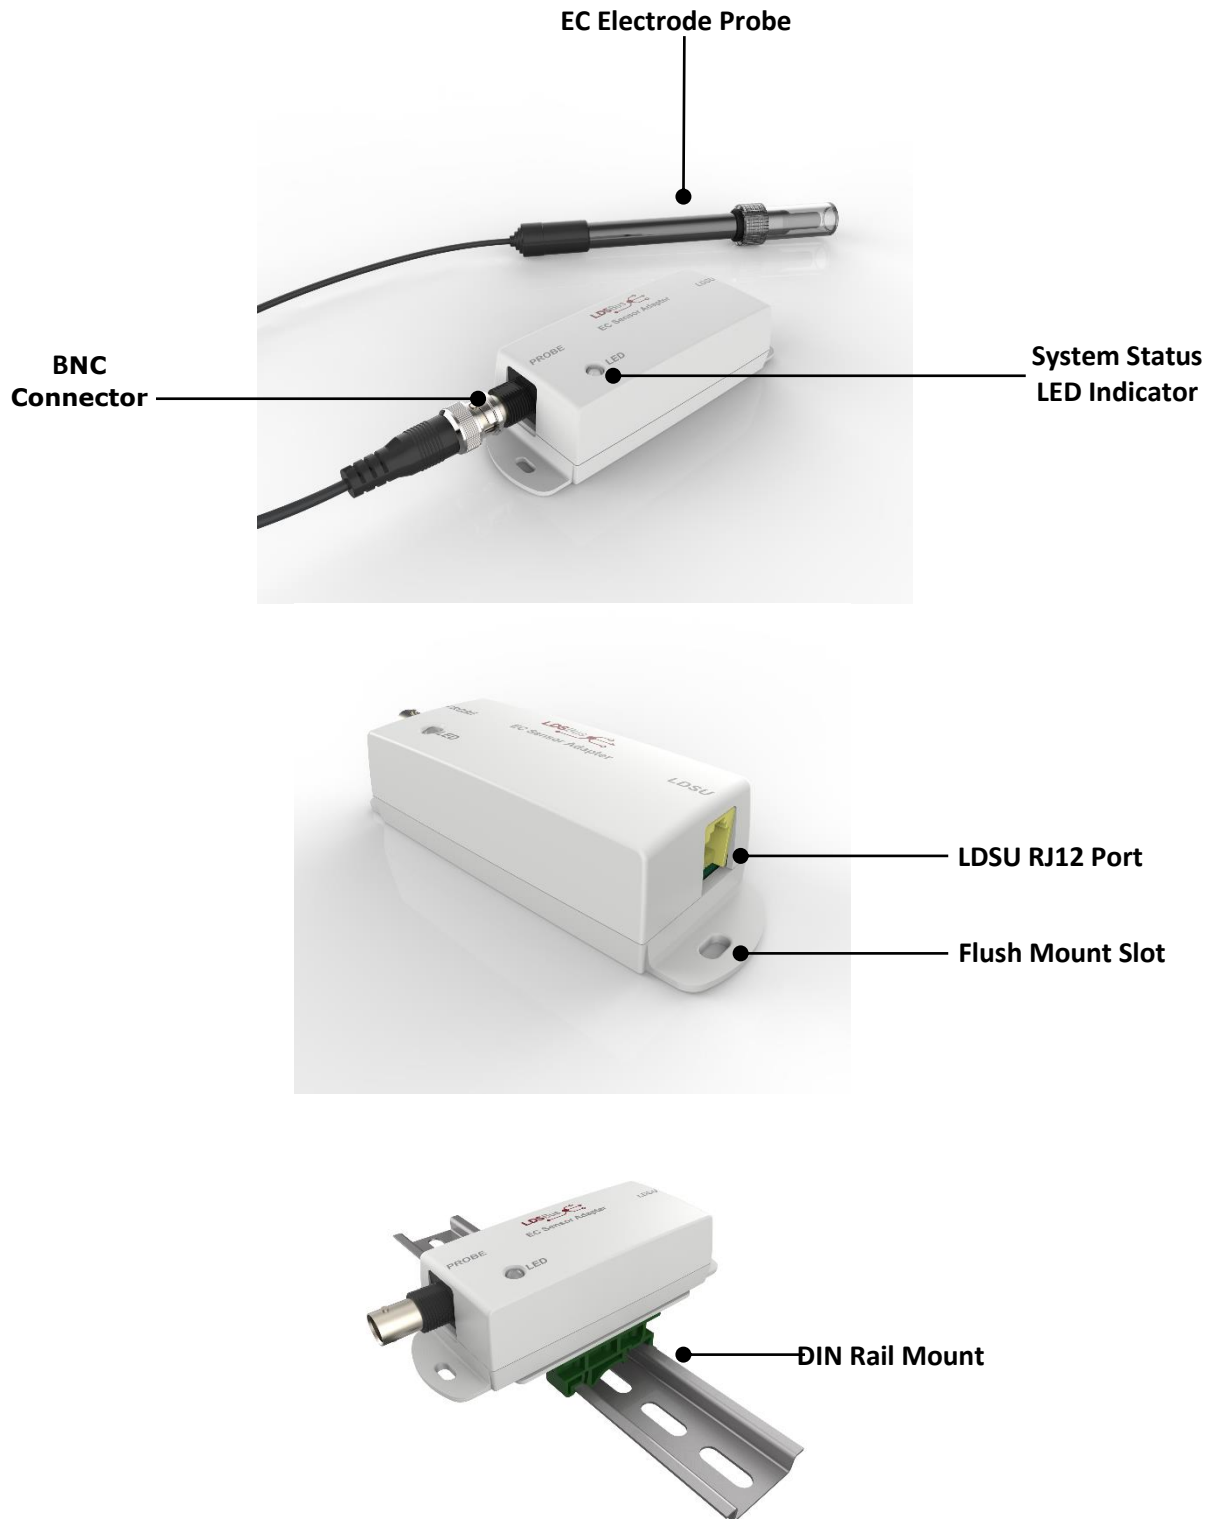


**Figure 1 - LDSBus EC Sensor Adapter Hardware Features**

## 5 Sensor Configuration and Installation

Please visit <https://brtsys.com/resources> to access the LDSBus Configuration Utility Guide on how to configure the device name, address, and termination settings before using it for your application.

### 5.1 Connection Diagram

Figure 2 illustrates the connection of the LDSBus EC Sensor Adapter (LDSBus Device) to the LDSBus. Please visit <https://brtsys.com/resources> to view the full device application, setup, and installation guides.

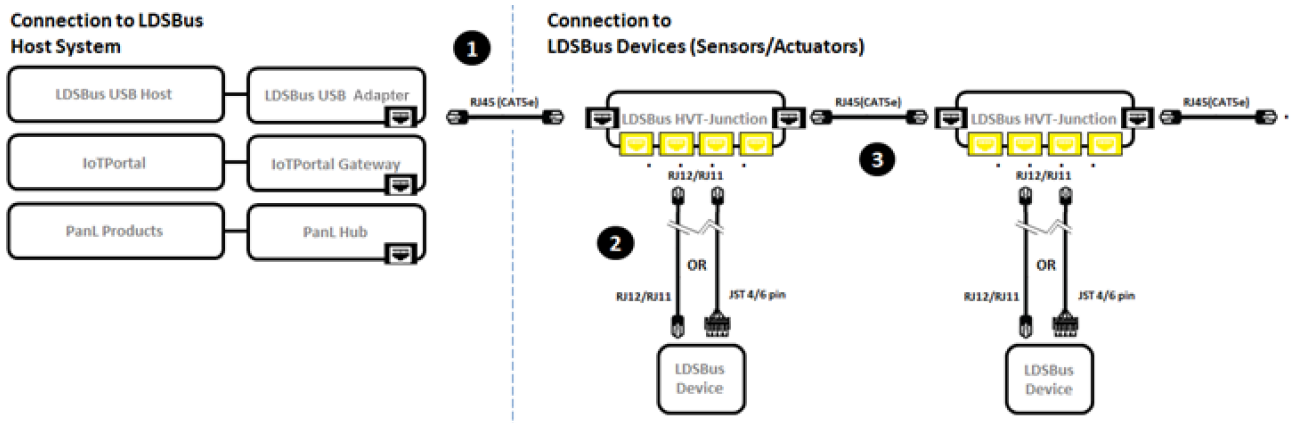

**Figure 2 - LDSBus EC Sensor Adapter to LDSBus - Connection Diagram**


#### **Setup Instructions:**

1. Connect the first LDSBus HVT-Junction to any of the LDSBus Host Systems using the RJ45 (CAT5e) cable.
2. Connect the configured LDSBus EC Sensor to the LDSBus HVT-Junction as shown in Figure 2.
3. If there is more than one LDSBus HVT-Junction, chain them together as shown in Figure 2.

## 6 Mounting Options

### 6.1 Flush Mount


The LDSBus EC Sensor Adapter can be flush mounted directly on a wall or any flat surface using 2 M3.5\*16mm (thread) screws.

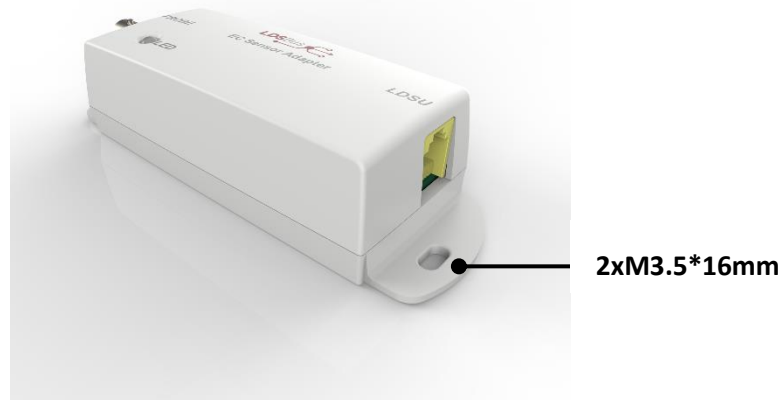

**Figure 3 - LDSBus EC Sensor Adapter Flush Mount**

### 6.2 DIN Rail Mount

The DIN Rail Mount can be fixed using a DIN Rail bracket that has two mounting holes. The package includes mounting screws and a backplate. (The DIN Rail Bracket is not included in the package).

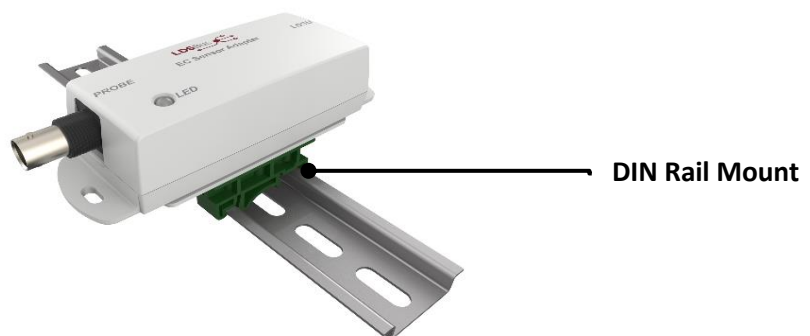










**Figure 4 - LDSBus EC Sensor Adapter DIN Rail Mount**

## 7 System Status LED Indicators

LDSU devices come with an RGB LED (4 status colors) as mentioned in the table below.

Status display colors

1. RED - Device in error condition
2. YELLOW - Un-configured device
3. GREEN - Device in normal state (Device termination is OFF)
4. BLUE - Device in normal state (Device termination is ON)

Device Status	LED Color	Flashing Frequency	Description
Un-configured device	YELLOW 	LED flashing @1Hz	Un-configured device with factory default address (126)
Configured device	GREEN 	Steady-Non-flashing	Configured device (Device ID 1-125) and device is idle.
	BLUE 		
Addressed device	GREEN 	LED flashing @5Hz	Device is busy communicating.
	BLUE 		
Identified device	GREEN 	LED flashing @1Hz	Device in identify state.
	BLUE 		
Device error	RED 	Steady - Non-flashing	Device error has occurred.
Firmware update	YELLOW 	Steady - Non-flashing	Device firmware update.

**Table 2 – LDSBus EC Sensor Adapter – System Status LED Indicator**




## 8 Probe Selection

The following specifications are recommended for selecting a Probe -

Detection Range	:	0.001mS/cm to 1.5mS/cm
Cell Constant	:	K=0.1
Detection Range	:	0.05mS/cm to 15mS/cm
Cell Constant	:	K=1.0
Detection Range	:	0.5mS/cm to 150mS/cm
Cell Constant	:	K=10
Connector	:	BNC

For more information on calibration, please refer to  
[BRTSYS AN 001 LDSBus Configuration Utility Guide](#)


## 9 Mechanical Dimension

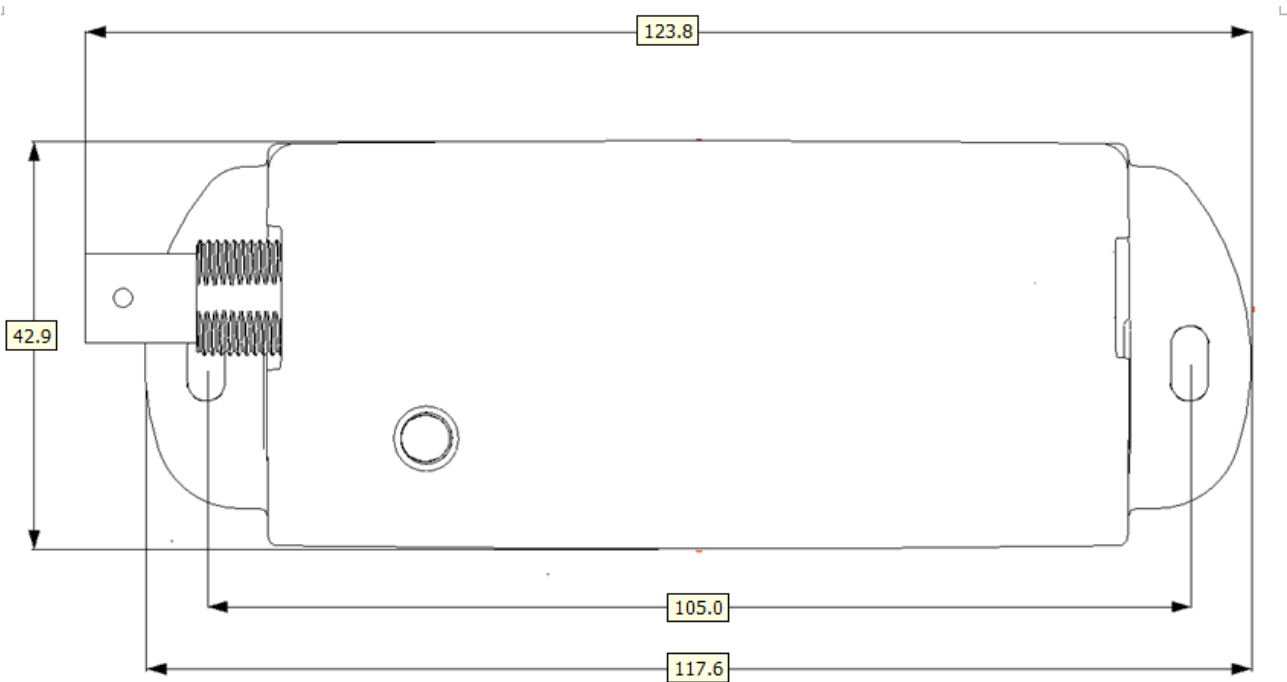

**Figure 5 – LDSBus EC Sensor Adapter Dimension – Top View**



**Figure 6 – LDSBus EC Sensor Adapter Dimension – Side View**

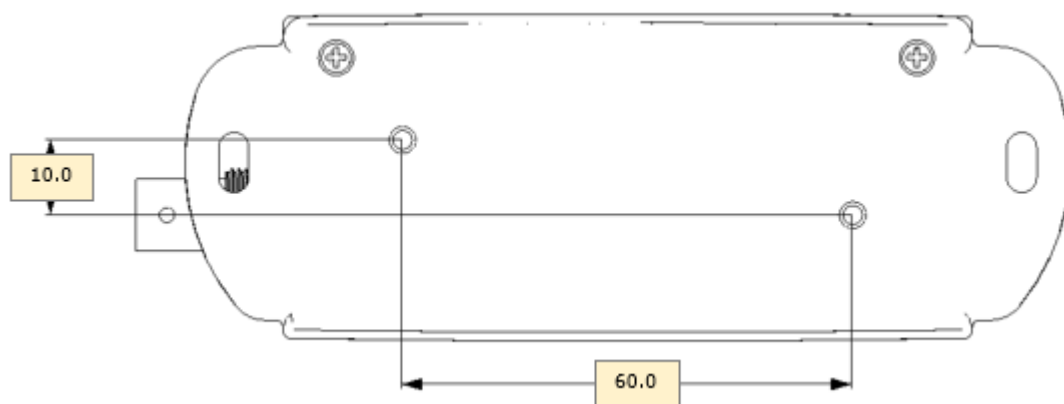

**Figure 7 – LDSBus EC Sensor Adapter Dimension – Bottom View**

**Note:** All dimensions are in millimetres.

## 10 Contact Information

### Head Quarters – Singapore

BRT Systems Pte Ltd  
178 Paya Lebar Road, #07-03  
Singapore 409030  
Tel: +65 6547 4827  
Fax: +65 6841 6071

E-mail (Sales) [sales@brtsys.com](mailto:sales@brtsys.com)  
E-mail (Support) [support@brtsys.com](mailto:support@brtsys.com)

### Web Site

<http://brtsys.com/>

### Distributor and Sales Representatives

Please visit the Sales Network page of the [BRT Systems Web Site](#) for the contact details of our distributor(s) and sales representative(s) in your country.

System and equipment manufacturers and designers are responsible to ensure that their systems, and any BRT Systems Pte Ltd (BRTSys) devices incorporated in their systems, meet all applicable safety, regulatory and system-level performance requirements. All application-related information in this document (including application descriptions, suggested BRTSys devices and other materials) is provided for reference only. While BRTSys has taken care to assure it is accurate, this information is subject to customer confirmation, and BRTSys disclaims all liability for system designs and for any applications assistance provided by BRTSys. Use of BRTSys devices in life support and/or safety applications is entirely at the user's risk, and the user agrees to defend, indemnify, and hold harmless BRTSys from any and all damages, claims, suits, or expense resulting from such use. This document is subject to change without notice. No freedom to use patents or other intellectual property rights is implied by the publication of this document. Neither the whole nor any part of the information contained in, or the product described in this document, may be adapted, or reproduced in any material or electronic form without the prior written consent of the copyright holder. BRT Systems Pte Ltd, 178 Paya Lebar Road, #07-03, Singapore 409030. Singapore Registered Company Number: 202220043R.

## Appendix A – References

### Document References

[BRTSYS AN 001 LDSBus Configuration Utility Guide](#)

### Acronyms and Abbreviations

Terms	Description
DC	Direct Current
EC	Electrical Conductivity
LDSBus	Long Distance Sensor Bus
LED	Light Emitting Diode

## **Appendix B – List of Figures and Tables**

### **List of Figures**

Figure 1 - LDSBus EC Sensor Adapter Hardware Features.....	5
Figure 2 - LDSBus EC Sensor Adapter to LDSBus - Connection Diagram .....	6
Figure 3 - LDSBus EC Sensor Adapter Flush Mount .....	7
Figure 4 - LDSBus EC Sensor Adapter DIN Rail Mount.....	7
Figure 5 - LDSBus EC Sensor Adapter Dimension – Top View.....	10
Figure 6 - LDSBus EC Sensor Adapter Dimension – Side View.....	10
Figure 7 - LDSBus EC Sensor Adapter Dimension – Bottom View.....	10

### **List of Tables**

Table 1 - LDSBus EC Sensor Adapter Specifications .....	4
Table 2 - LDSBus EC Sensor Adapter – System Status LED Indicator.....	8

## Appendix C – Revision History

Document Title: LDSBus EC Sensor Adapter Datasheet  
Document Reference No.: BRTSYS\_000011  
Clearance No.: BRTSYS#011  
Product Page: <https://brtsys.com/ldsbus/>  
Document Feedback: [Send Feedback](#)

Revision	Changes	Date
Version 1.0	Initial Release	04-03-2022
Version 1.1	Updated release under BRT Systems	15-09-2022
Version 1.2	Corrected BRTSYS to BRTSys	24-03-2023