


**RoHS COMPLIANT**

CUSTOMER:	P/N:	MD115-AL	REV.	APPROVALED BY:	REVISIONS	
					DESCRIPTION	DATE
					A	2021.09.13
					B	Change the wire printing, change the plug into an integrated terminal frame
						2022.08.12

NOTES:  
1. RoHS shown on the carton

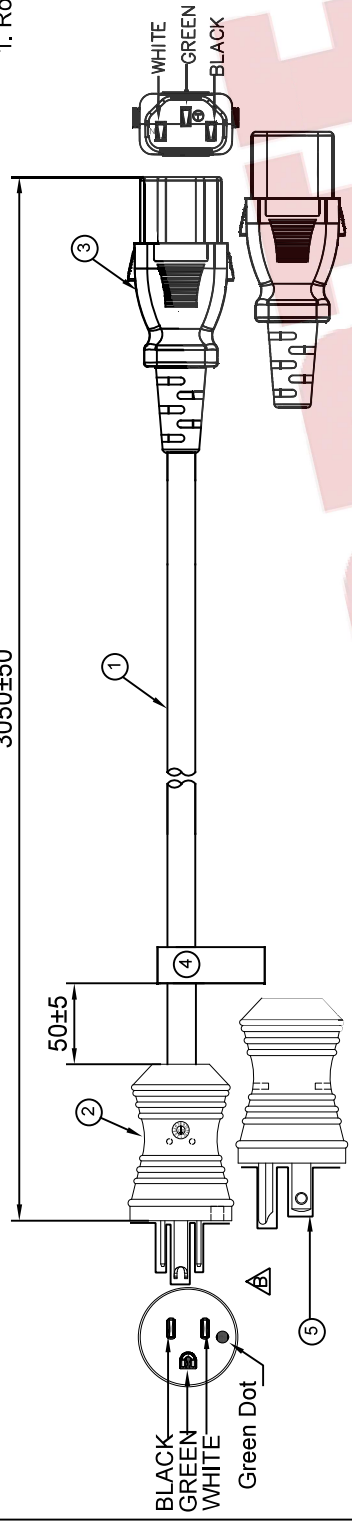

**MARKING:**

WELL SHIN®  
WS-002A-4  
E115330  
10A 125V~1312


IEC-60320-C13  
AUTO-LOCK  
CLEAR

WELL SHIN®  
WS-001H  
10A 125V~  
E115330  
HOSPITAL GRADE  
UL

2023.03.20  
Chen Tony

**CORDTEC POWER CORPORATION**  
**CONFIRMED**

④ Hosp. Grade label

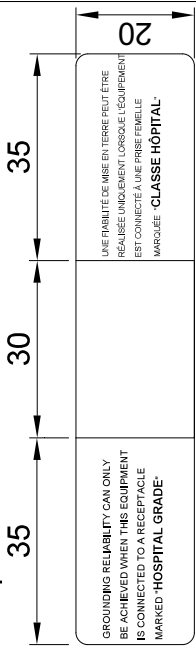

GROUNDING RELIABILITY CAN ONLY BE ACHIEVED WHEN THIS EQUIPMENT IS CONNECTED TO A RECEPTACLE MARKED "HOSPITAL GRADE"

UNE FACILITE DE MISE EN TERRE PEUT ÊTRE RÉALISÉE INDICÉMENT. L'ÉQUIPEMENT EST CONNECTÉ À UNE PRISE FEMELLE MARQUÉE "CLASSE HÔPITAL"

⑥	Cable tie	WHITE	1PCS
⑤	Protective case	WHITE	1PCS
④	Wire label 100mm*20mm		1PCS
③	WS-002A-4 10A 125V APPROVAL: UL,CUL	CLEAR	1PCS
②	WS-001H(5-15P) 10(A) 125(V) APPROVAL: UL,CUL CUL/US E90165-K SJTW 3x0.824mm²(18AWG) with thread 105°C 300V VW-1 WELL SHIN/UL	CLEAR	1PCS
①		GRAY	1PCS
NO.	DESCRIPTION	COLOR	QTY

SIGNATURE	
ENGINEER BY:	
MANAGER BY:	
CHECKED BY:	
DRAWN BY:	

**CORDTEC**  
POWER CORPORATION

**AC Connectors of Cordtec Power Corp**  
Main: 1-414-434-2220 Fax: 1-414-323-8386  
Text: 1-414-323-3240  
Email: Info@CordtecPower.com  
Website: CordtecPower.com/ ACWORKS.com