
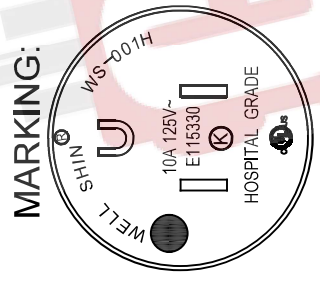


RoHS COMPLIANT

REV.	DESCRIPTION	DATE
A		2021.11.09
A	Change the wire specification	2022.07.16

CUSTOMER: P/N: MD117 REV. APPROVED BY:

NOTES:
 1. The outer box must have the RoHS mark (RoHS shown on the carton)
 2. The rear WS-002 uses a transparent inner sleeve

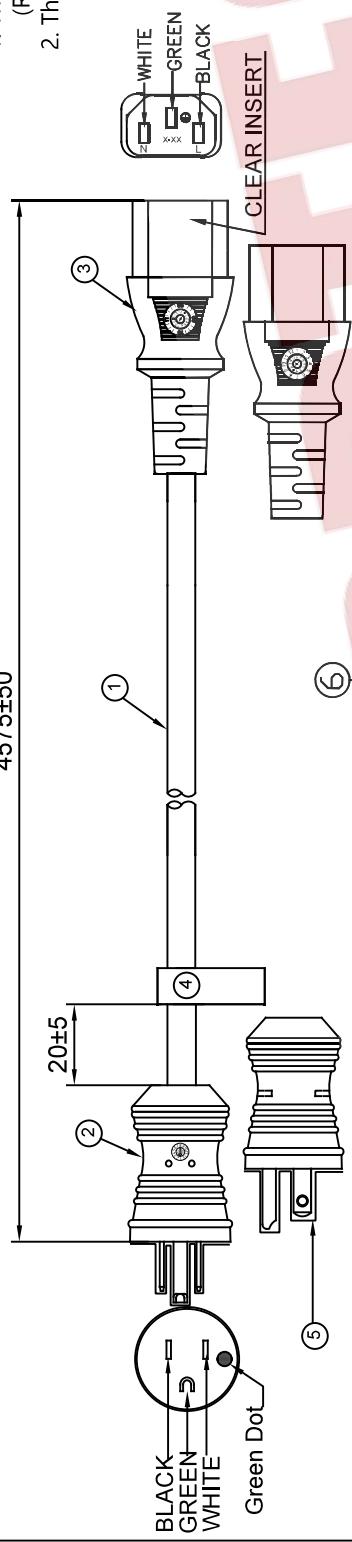


**NEMA 5-15P
HOSPITAL GRADE
CLEAR**



**IEC-60320-C13
CLEAR**



④ Hosp. Grade label

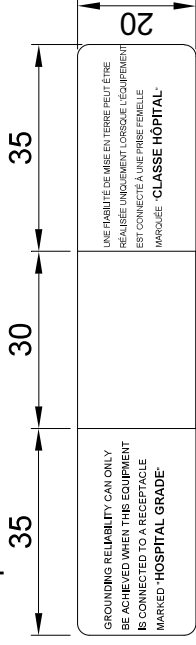

NO.	DESCRIPTION	COLOR	QTY
⑥	Cable tie	WHITE	2PCS
⑤	Protective case	WHITE	1PCS
④	Wire label 100mm*20mm	CLEAR	1PCS
③	WS-002 10A 125V APPROVAL: UL,CUL	CLEAR	1PCS
②	WS-001H(5-15P) 10(A) 125(V) APPROVAL: UL,CUL	CLEAR	1PCS
①	CUL(U.S. E90165-K SJTW 3x0.824mm²(18AWG) with thread 105°C 300V VW-1 WELLSHIN A)	GRAY	1PCS
NO.	DESCRIPTION	COLOR	QTY

SIGNATURE	ENGINEER BY:	MANAGER BY:	CHECKED BY:	DRAWN BY:

CORDTEC POWER CORPORATION
AC Connectors of Cordtec Power Corp
 Main: 1-414-434-2220 Fax: 1-414-323-8386
 Text: 1-414-323-3240
 Email: Info@CordtecPower.com
 Website: CordtecPower.com/ ACWORKS.com