

RoHS COMPLIANT

REV.	DESCRIPTION	DATE
A	Change the plug to the terminal frame type	2021.12.08
A		2022.10.11

CUSTOMER:


P/N: MD231

REV.


APPROVALED BY:

NOTES:

- The outer box must have the RoHS mark (RoHS shown on the carton)
- The tail WS-002 uses a transparent inner sleeve

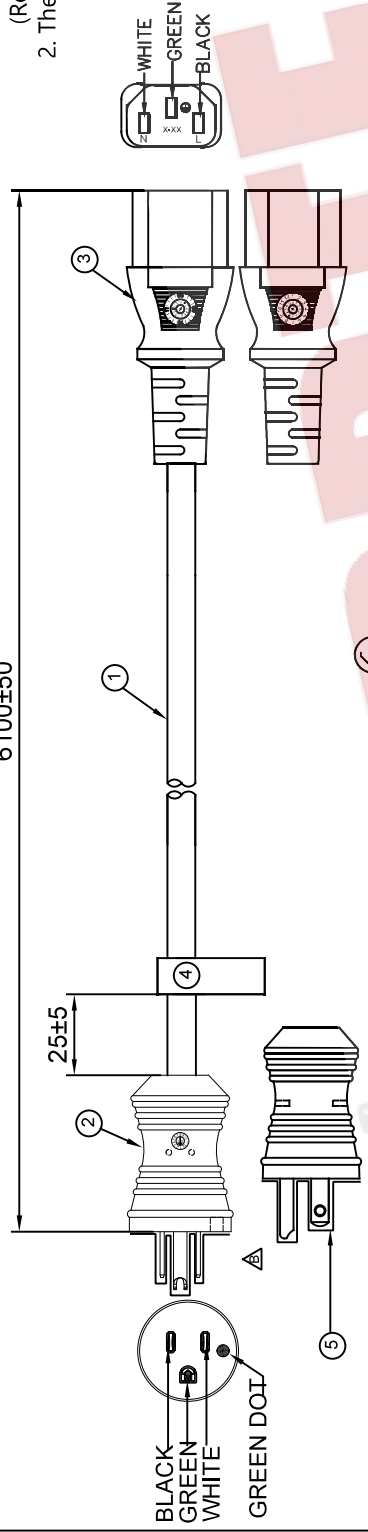

MARKING:



NEMA 5-15P
HOSPITAL GRADE
CLEAR


MARKING:



CORDTEC POWER CORPORATION
CONFIRMED

2023.03.20
Chen Tony

Hosp. Grade label

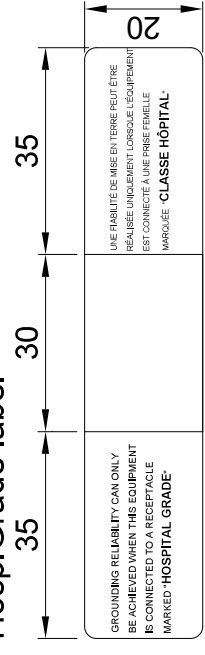

NO.	DESCRIPTION	COLOR	QTY
⑥	Cable tie	WHITE	1PCS
⑤	Protective case	WHITE	1PCS
④	Wire label 100mm*20mm		1PCS
③	WS-002 15A 125V APPROVAL: UL,CUL	CLEAR	1PCS
②	WS-001H(5-15P) 15(A) 125(V) APPROVAL: UL,CUL	CLEAR	1PCS
①	CUL/US E90165-K SJT 3*2.08mm ² (14AWG) 105°C 300V VW-1 WELL SHIN	GRAY	1PCS
NO.	DESCRIPTION	COLOR	QTY

SIGNATURE
ENGINEER BY:
MANAGER BY:
CHECKED BY:
DRAWN BY:



AC Connectors of Cordtec Power Corp
Main: 1-414-434-2220 Fax: 1-414-323-8386
Text: 1-414-323-3240
Email: Info@CordtecPower.com
Website: CordtecPower.com/ ACWORKS.com