


RoHS (2011/65/EU) COMPLIANT

REVISIONS	
REV.	DESCRIPTION
1	Correct the end of security print and marking, update Notes 1
2	
3	
4	
5	

CUSTOMER: P/N: MD261-AL REV. APPROVED BY:

4572±50

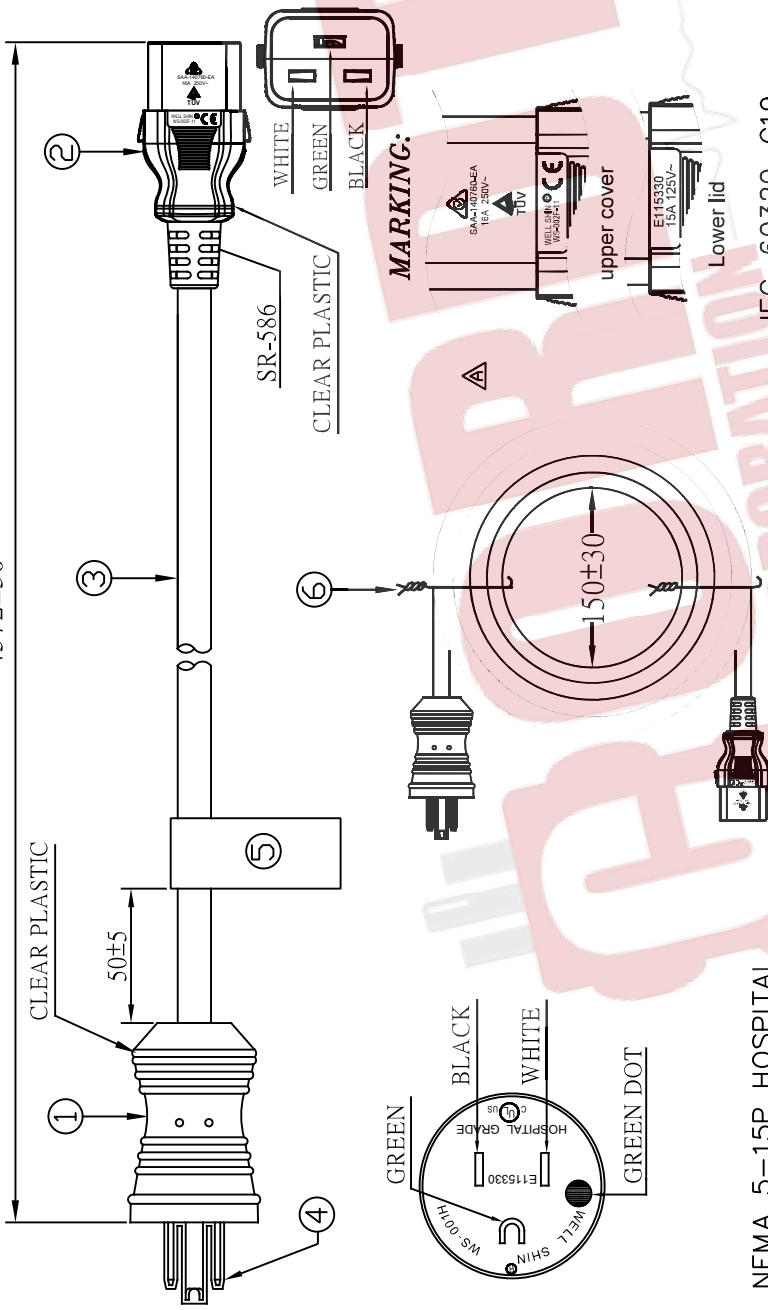


NOTES: 1. RoHS shown on the carton



NEMA 5-15P HOSPITAL GRADE CLEAR
IEC-60320-C19
AUTO-LOCK CLEAR

5 Hosp. Grade label

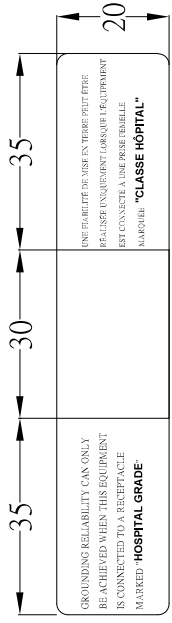

ITEM	DESCRIPTION	QTY	COLOR
6	Cable tie	2	WHITE
5	Hosp. Grade label	1	---
4	Plastic cap	1	WHITE
3	SJTW 14AWG*3C 105°C APPROVAL : UL,CSA	1	(GY-H) PANTONE Cool Grey 9C
2	WS-002F-11 15 (A) 125 (V) APPROVAL : UL,CUL,SAA,TUV,CE	1	CLEAR
1	WS-001H(5-15P) 15 (A) 125 (V) APPROVAL : UL,CUL	1	CLEAR

SIGNATURE	
ENGINEER BY:	
MANAGER BY:	
CHECKED BY:	
DRAWN BY:	



AC Connectors of Cordtec Power Corp
Main: 1-414-434-2220 Fax: 1-414-323-8386 Text: 1-414-323-3240
Email: Info@CordtecPower.com
Website: CordtecPower.com/ ACWORKS.com

