




E-FLEX RT

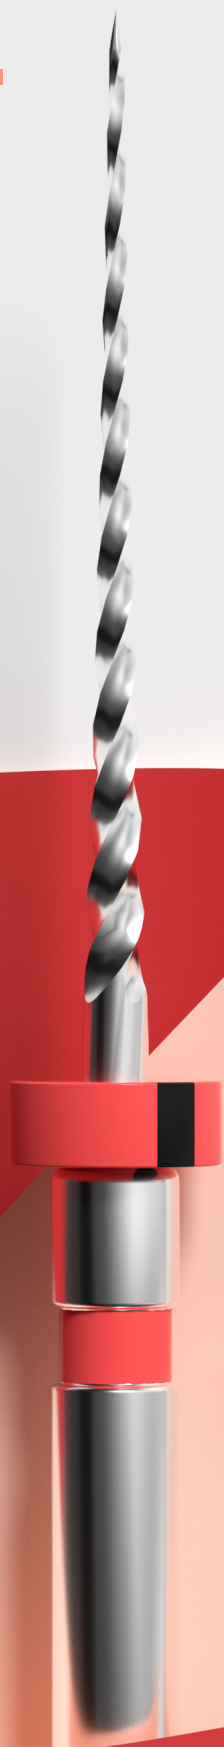

Safe and effective removal of obturation materials Reducing the need for solvents

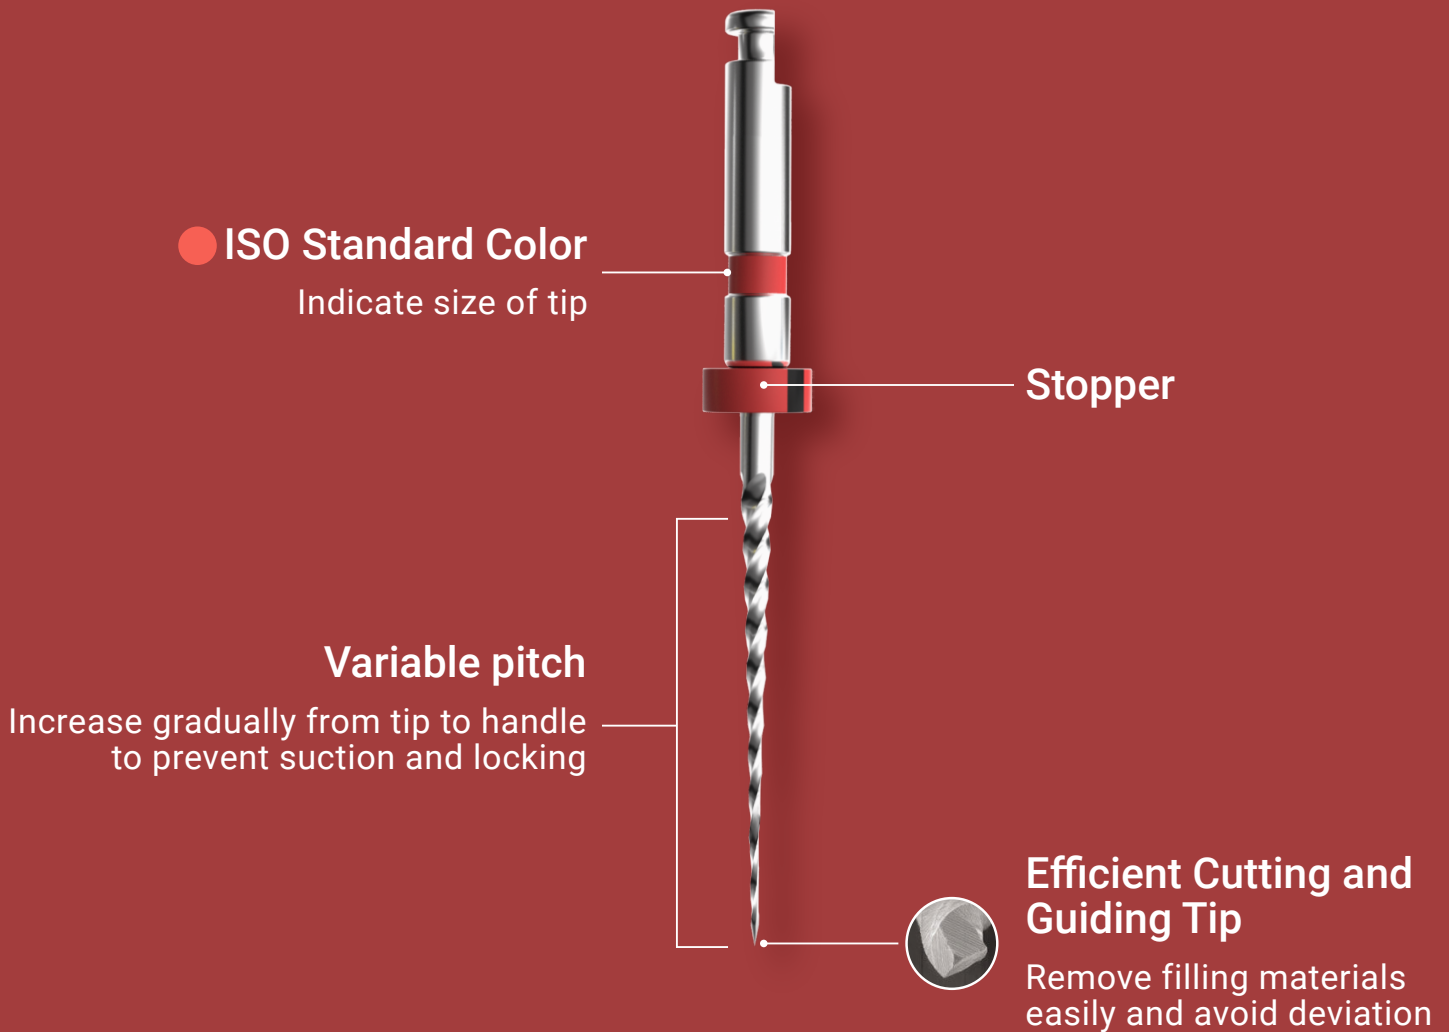

• Usage Protocol

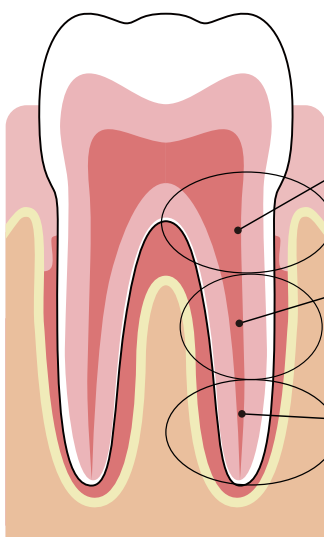

09/30

For Coronal 1/3



08/25


For Middle 1/3



07/20

For Apical 1/3

Retreatment File

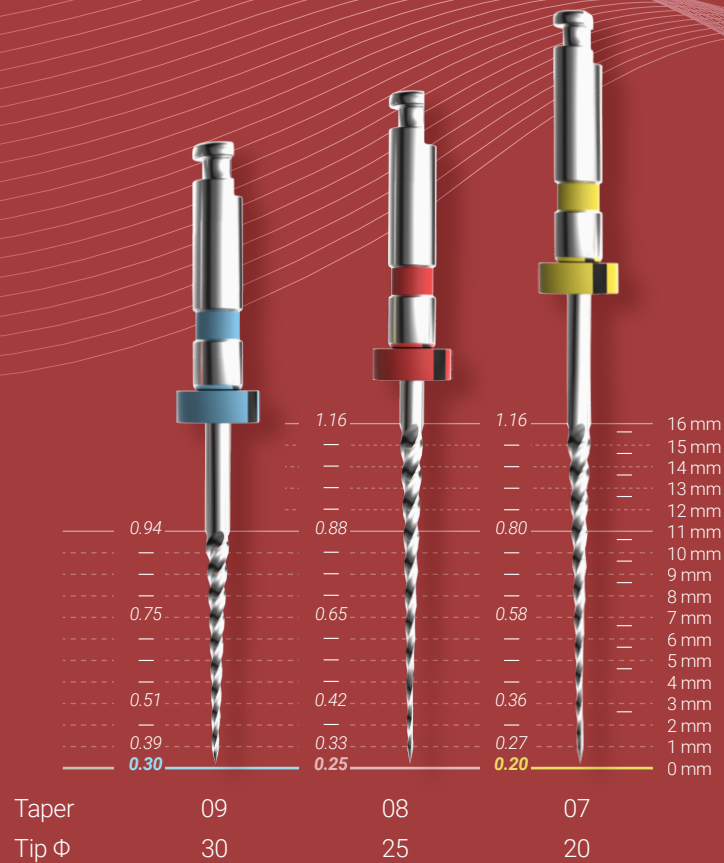

	Color	Tip Size	Taper (%)	Cross-Section	Length (mm)	Suggested Speed/Torque
E-FLEX RT	●	30	9		16	350 rpm 2 N·cm
	●	25	8		18	
	●	20	7		22	