

QUALITY. SERVICE. VALUE.

WP Series Waterproof Portables

WP-90 User Manual



Waterproof



User Friendly



GLP Compliant



USB Download



Data logging



Multiple Power Options

Congratulations !

You have purchased the latest in Handheld Specific Ion-pH-ORP-Temperature instrumentation. We trust that your new **WP-90** will give you many years of reliable service.

The **WP-90** is a breeze to operate. This manual has been designed to help you get started, and also contains some handy application tips. If at any stage you require assistance, please contact either your local TPS representative or the TPS factory in Brisbane.

The manual is divided into the following sections:

1. Table of Contents

Each major section of the handbook is clearly listed. Sub-sections have also been included to enable you to find the information you need at a glance.

2. Introduction

The introduction has a diagram and explanation of the display and controls of the **WP-90**. It also contains a full listing of all of the items that you should have received with your **WP-90**. Please take the time to read this section, as it explains some of items that are mentioned in subsequent sections.

3. Main Section

The main section of the handbook provides complete details of the **WP-90**, including operating modes, calibration, troubleshooting, specifications, and warranty terms.

4. Appendices

Appendices containing background information and application notes are provided at the back of this manual.



TPS Pty Ltd

Phone : (07) 3205 8027

Email : sales@tps.com.au

Web : www.tps.com.au

**Model WP-90
Specific Ion, pH,
ORP & Temp. Meter**

Version: 2.1

Date: 16/06/2021


Contents

1. Introduction	5
1.1 WP-90 Display and Controls	5
1.2 Unpacking Information	7
1.3 Specifications	8
2. WP-90 Menu Structure	9
3. Specific Ion Mode	11
3.1 Selecting ppM or ppK Mode	11
3.2 Selecting Exponential Mode (e.g. Molar)	13
4. Specific Ion Calibration	15
4.1 Calibration Procedure	15
4.2 Calibration Notes	16
4.3 Calibration Messages	17
5. pH Calibration	18
5.1 Calibration Procedure	18
5.2 Calibration Notes	19
5.3 Calibration Messages	19
6. mV/ORP Calibration	20
7. Relative mV/ORP Calibration	20
7.1 Notes	20
8. Temperature Calibration	21
8.1 Calibration Procedure	21
8.2 Calibration Notes	22
8.3 Calibration Messages	22
8.4 Manual Temperature Setting	22
9. Good Laboratory Practices (GLP)	23
9.1 To recall GLP information on the display	23
9.2 Failed Calibration	24
9.3 Printing GLP Information to the RS232 Port	24
9.4 Instrument Serial Number	25
9.5 Additional GLP Features	25
10. Notepad Function	26
10.1 Recording Readings into the Notepad	26
10.2 Recalling Records from the Notepad	26
10.3 Erasing Records from the Notepad	27
10.4 Printing Records from the Notepad to the RS232 Port	27
11. Automatic Data logging	28

12.	RS232 Port	30
12.1	Setting the Baud Rate	30
12.2	Sending Readings to the RS232 Port	30
12.3	RS232 Configuration	30
12.4	Communication and Statistical Software	30
12.5	Commands	31
12.6	Data Format	32
12.7	GLP Data Format	33
13.	Battery Saver Function	34
14.	Recharging the Battery	35
15.	Clock Function	36
15.1	Setting the Clock	36
15.2	Displaying or Hiding the Clock	36
16.	Selecting Buffers for Auto Buffer Recognition	37
17.	Initialising the WP-90	38
18.	Instrument firmware version number.	38
19.	Troubleshooting	39
19.1	General Errors	39
19.2	Specific Ion, pH and mV/ORP Troubleshooting	40
19.3	Temperature Troubleshooting	42
20.	Appendices: pH Sensor Theory	43
20.1	Asymmetry of a pH Sensor	43
20.2	Slope of a pH Sensor	44
20.3	pH Temperature Compensation	45

1. Introduction

1.1 WP-90 Display and Controls

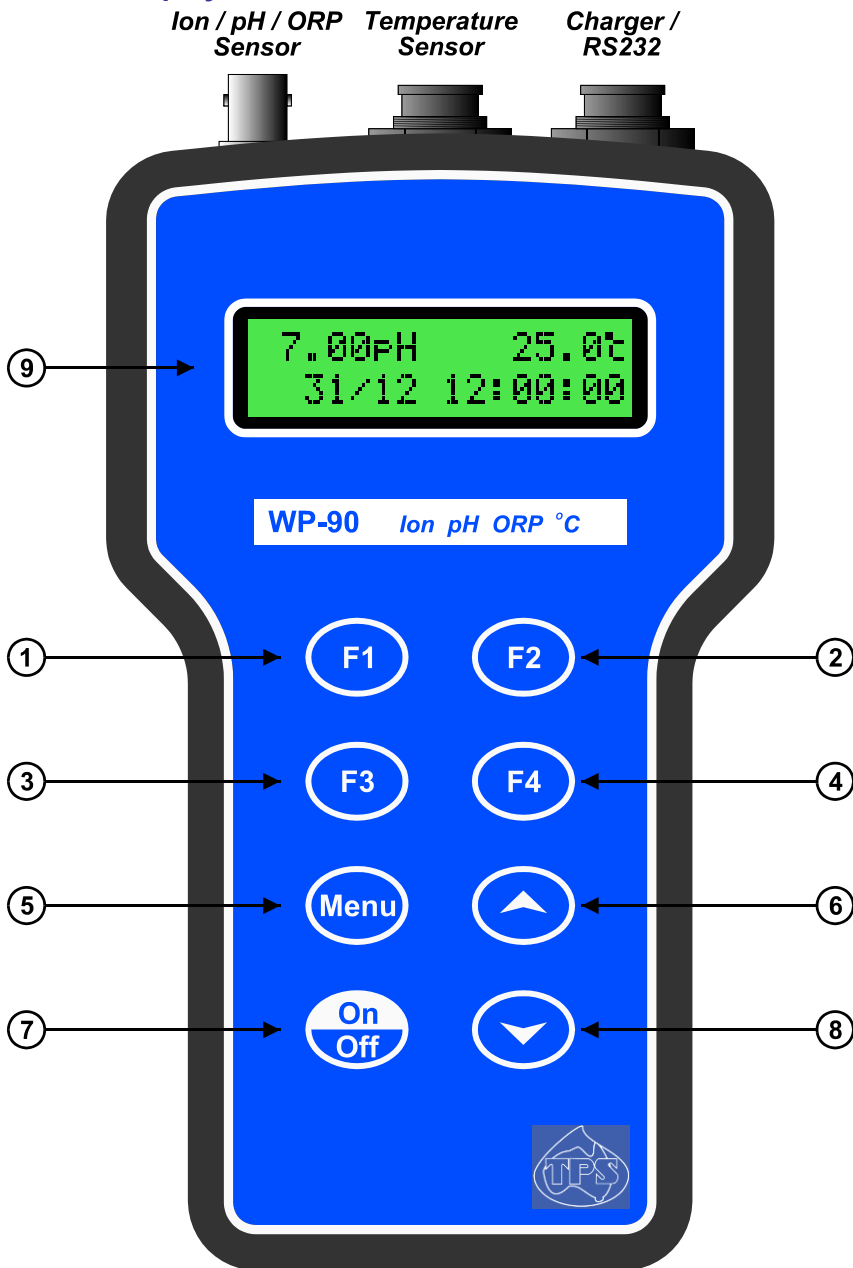



Press to record readings into memory. See section 10.1.

Also used at turn-on to select pH7.00 or pH6.86 as the primary pH buffer (section 16).



Press to show or hide the date and time. See section 15.2.



Press to start or stop automatic logging. See section 11.

Alternatively, press to transmit current reading plus date and time to the RS232 port. See section 12.2.






Press to zero Relative mV/ORP, when Relative mV/ORP mode is selected (section 7).



Press to access the user-friendly menu system which makes the **WP-90** easy to operate.



The  and  keys are used for calibrating temperature readout (section 8.1), setting the clock (section 15.1), setting the automatic logging period (section 11), and displaying GLP information (section 9.1).

The  key is also used to initialise the **WP-90** at turn-on. See section 17.



Switches the **WP-90** on and off.

⑨ Display 32 character alpha-numeric display with user-friendly menu and prompting system. Shows Specific Ion/pH/ORP and Temperature simultaneously. Date and time can also be displayed.

1.2 Unpacking Information

Before using your new **WP-90**, please check that the following accessories have been included:

	Part No
1. WP-90 Specific Ion-pH-ORP-Temp Instrument	121191
2. Temperature/ATC Sensor	121247
3. Battery charger	130037
4. Manual	

*Options that may have been ordered with your **WP-90**:*

1. Your choice of a complete range of Ion Selective, Reference, pH and ORP sensors. (*see cable label for part No*)
2. Extended cable 130040
3. RS232 Serial Interface Cable 130041
4. Communication software for Windows 95 and later 130086
5. USB to Serial Adaptor (requires 130041 also) 130087
6. Hard Carry Case 130059
7. Battery charger lead for 12V cigarette lighter socket 130046
8. Battery charger lead for 12V DC, with battery clips 130052
9. Solar Panel 130012

1.3 Specifications

Specific Ions

Range Auto-ranging, in units of ppM, ppK and
Exponential Notation

Resolution 3 significant digits

Accuracy \pm least significant digit

pH

Range 0 to 14.00 pH

Resolution 0.01 pH

Accuracy ± 0.01 pH

mV/ORP

Range 0 to ± 500.0 and 0 to ± 1500 mV (auto-
ranging)

Resolution 0.15 and 1 mV

Accuracy ± 0.3 and ± 1 mV

Temperature

Range -10.0 to +120.0 °C

Resolution 0.1 °C

Accuracy ± 0.2 °C

General Specifications

Temperature Compensation:

pH & Ion (only, not for mV/ORP). Automatic 0 to 100 °C
Manual 0 to 100 °C

Calibration:

pH Auto Standard Recognition in pH4.01,
pH6.86, pH7.00, pH9.18 or pH10.01
buffers.

pH Sensor Asymmetry Range -1.00 to +1.00 pH

pH Sensor Slope Range 85.0 to 105%

Input Impedance $>3 \times 10^{12} \Omega$

Specific Ion Calibration in user-definable standards.

mV/ORP Sensor calibration not available.

Temperature Use a reference thermometer.

Temperature Sensor Offset . -10.0°C to +10.0°C

Memory 3600 readings including date and time

Automatic Logging User-set for one reading every 1 to 90 seconds, 1 to 90 minutes, or 1 to 24 hours.

RS232 Output 300, 1200, 9600 & 19200 baud. 8 bits, no parity, 1 stop bit, XON/XOFF Protocol.

Clock Calendar clock displays date, month, hours, minutes & seconds.
Year is recorded in memory and transmitted to RS232 port, but is not displayed.

Battery Saver On : Auto switch-off after 5 minutes
Off : Continuous use
Bar Graph display of battery charge level.
Readout of battery voltage available for troubleshooting.

Good Laboratory Practices Date, Time and Value of last Specific Ion, pH and Temperature calibration are stored, and can be recalled or sent to the RS232 port at any time.

Power 6V NiMH Rechargeable Battery for approx 50 hours operation.

Dimensions 195 x 110 x 55 mm


Mass Instrument only : Approx 520g

Full Kit : Approx 2.5kg

Environment..... Temperature : 0 to 45 °C
Humidity : 0 to 95 % R.H.

2. WP-90 Menu Structure

A detailed breakdown of the menu system of the **WP-90** is shown below. This diagram provides a quick reference for the **WP-90** menu functions.

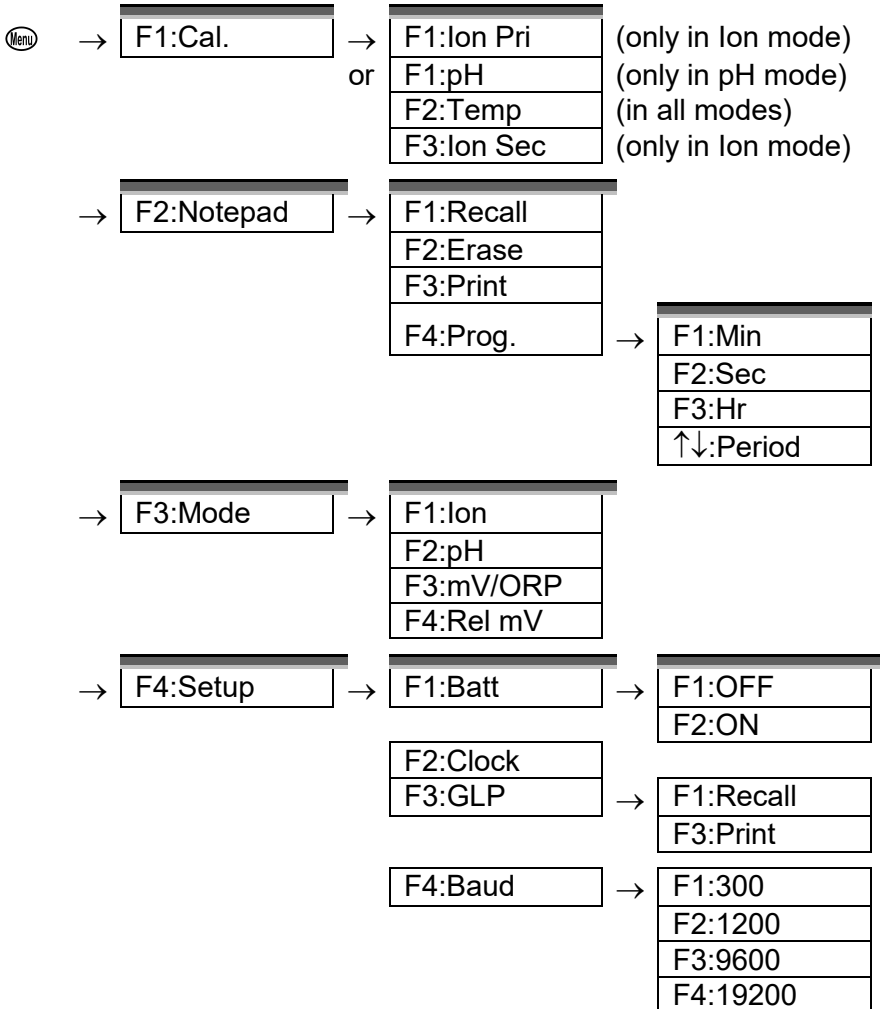

3. Specific Ion Mode

Before taking Specific Ion measurements, it is necessary to set up this mode for the Specific Ion to be measured. To set up the Specific Ion mode, follow these simple steps...

3.1 Selecting ppM or ppK Mode

1. Select Specific Ion mode (Menu → **F3:Mode** → **F1:Ion**).
2. Select ppM/ppK as the unit of measurement.

Select Ion Mode F1:ppM/ppK F2:Exp

Press **F1** to select readout in ppM (parts per million) and ppK (parts per thousand). The **WP-90** will automatically select the range that provides the best resolution for the sample being measured.

3. Select the type of Specific Ion to be measured.

F1:+Mono F2:-Mono F3:++Di F4:--Di
--


Press **F1** for Monovalent Cation (e.g. Na⁺).

Press **F2** for Monovalent Anion (e.g. F⁻).

Press **F3** for Divalent Cation (e.g. Cu²⁺).

Press **F4** for Divalent Anion (e.g. S²⁻).

4. Enter the value of the Primary Standard to be used for calibration.



1.000ppM Pri Std
F1:← F2:→ ↑↓:Set

Use the \uparrow and \downarrow keys to set the first digit. The numbers scroll from 0 to 9 plus the decimal point.


Press $F2$ to move to the next digit, then use the \uparrow and \downarrow keys to set it. Continue moving from digit to digit until the value of the Primary Standard has been correctly set. Up to 4 digits plus a decimal point can be entered.

After the last digit has been entered, $F2$ will move the cursor to the units.

Use the \uparrow and \downarrow keys to select ppM or ppK.

Press $F2$ to save the Primary Standard.

5. Enter the value of the Secondary Standard to be used for calibration. The Secondary Standard must be at least 2 to 100 times higher or lower than the Primary Standard.



10.00ppM Sec Std
F1:← F2:→ ↑↓:Set

Use the \uparrow and \downarrow keys to set the first digit. The numbers scroll from 0 to 9 plus the decimal point.

Press $F2$ to move to the next digit, then use the \uparrow and \downarrow keys to set it. Continue moving from digit to digit until the value of the Secondary Standard has been correctly set.

Up to 4 digits plus a decimal point can be entered.

After the last digit has been entered, $F2$ will move the cursor to the units.

Use the \uparrow and \downarrow keys to select ppM or ppK.

Press $F2$ to save the Secondary Standard.

6. The **WP-90** will now return to normal measurement mode.
7. A “ * ” will be shown in place of the decimal point if the Specific Ion mode is not calibrated, or if calibration has failed.

3.2 Selecting Exponential Mode (e.g. Molar)

1. Select Specific Ion mode (Menu) → **F3:Mode** → **F1:Ion**).
2. Select Exponential mode as the unit of measurement. This mode is designed specifically for units such as Molar.

Select Ion Mode
F1:ppM/ppK F2:Exp

Press (F2) to select Exponential readout (e.g. Molar). The **WP-90** will automatically select the range that provides the best resolution for the sample being measured.

3. Select the type of Specific Ion to be measured.

F1:+Mono F2:-Mono
F3:++Di F4:--Di

Press (F1) for Monovalent Cation (e.g. Na⁺).

Press (F2) for Monovalent Anion (e.g. F⁻).

Press (F3) for Divalent Cation (e.g. Cu²⁺).

Press (F4) for Divalent Anion (e.g. S²⁻).

4. Enter the value of the Primary Standard to be used for calibration.

1.0010⁺⁰⁰ Pri Std
F1:← F2:→ ↑↓:Set

Use the (▲) and (▼) keys to set the first digit. The numbers scroll from 0 to 9.

Press (F2) to move to the next 2 digits, then use the (▲) and (▼) keys to set each in turn (the decimal point is fixed in the second position).

Press (F2) to move the 10⁺, then use the (▲) and (▼) keys to set it as 10⁺ or 10⁻.

Press (F2) to move to the next 2 digits, then use the (▲) and (▼) keys to set each in turn.


For example...

1.0010⁺⁰¹ is 1.00×10^1 in units of the operator's choice (e.g. Molar).

1.0010⁻⁰¹ is 1.00×10^{-1} in units of the operator's choice (e.g. Molar).

Press **F2** to save the Primary Standard.

5. Enter the value of the Secondary Standard to be used for calibration.
The Secondary Standard must be at least 2 to 100 times higher or lower than the Primary Standard.



1.0010⁺⁰⁰ Sec Std
F1:← F2:→ ↑↓:Set

Use the **▲** and **▼** keys to set the first digit. The numbers scroll from 0 to 9.

Press **F2** to move to the next 2 digits, then use the **▲** and **▼** keys to set each in turn (the decimal point is fixed in the second position).

Press **F2** to move the 10^+ , then use the **▲** and **▼** keys to set it as 10^+ or 10^- .

Press **F2** to move to the next 2 digits, then use the **▲** and **▼** keys to set each in turn.

For example...

1.0010⁺⁰¹ is 1.00×10^1 in units of the operator's choice (e.g. Molar).

1.0010⁻⁰¹ is 1.00×10^{-1} in units of the operator's choice (e.g. Molar).

Press **F2** to save the Secondary Standard.

6. The **WP-90** will now return to normal measurement mode.
7. A “ * ” will be shown in place of the decimal point if the Specific Ion mode is not calibrated, or if calibration has failed.

4. Specific Ion Calibration

4.1 Calibration Procedure

1. Plug the Ion Selective Electrode into the **Sensor** socket. If a separate Reference Electrode is being used, plug this into the separate 4mm Reference socket provided.
2. Switch the meter on.
3. Select and set up Ion mode, as detailed in section 3.

For the purposes of this handbook, the **WP-90** has been set up for 1.000ppM as the Primary Standard and 0.100ppM as the Secondary Standard.

4. Ensure that temperature has already been calibrated (see section 8.1).

NOTE: A “*” in place of the decimal point in the temperature readout indicates that temperature is not calibrated.

5. Rinse the Ion Selective Electrode, (Reference Electrode if using) and Temperature sensors in distilled water and blot dry.

Primary Calibration


6. Place the Ion Selective Electrode, (Reference Electrode if using) and Temperature sensors into the Primary Standard.

Ensure that any Ionic Strength Adjusting Buffer (ISAB) that may be required has been added (see the Ion Selective Electrode’s handbook). A magnetic stirrer providing constant, gentle stirring generally improves stability.

7. Select Primary Calibration ( → **F1:Ca1** → **F1:Ion Pri**).

The following message should be displayed. The current reading is displayed on the top left. A “*” in the reading indicates that the **WP-90** is currently not calibrated.

1*234ppM	25.0°C
F1:Ca1 at1.000ppM	

When the reading has stabilised, press  to perform a Primary Calibration. A “*” will not be removed from the display after a 1-point Asymmetry Calibration.

8. Rinse the Sensors in distilled water and blot dry.

Secondary Calibration


9. Place the Ion Selective Electrode, (Reference Electrode if using) and Temperature sensors into the Secondary Standard.

Ensure that any Ionic Strength Adjusting Buffer (ISAB) that may be required has been added (see the Ion Selective Electrode's handbook).


A magnetic stirrer providing constant, gentle stirring generally improves stability.

10. Select Secondary Calibration ( → **F1:Ca1** → **F3:Ion Sec**).

The following message should be displayed. The current reading is displayed on the top left. A "*" in the reading indicates that the **WP-90** is currently not calibrated.



0*123ppM 25.0°C
F1:Ca1 at 0.100ppM

When the reading has stabilised, press  to perform a Secondary Calibration.

A "*" in the display will be replaced by a decimal point after a successful 2-point Slope calibration.

11. The WP-90 is now calibrated ready for Specific Ion measurements.

4.2 Calibration Notes

1. A Primary Calibration should be performed at least weekly. In applications where the reference electrode junction can become blocked, such as dairy products, mining slurries etc, a Primary Calibration may have to be done daily.
2. A full Primary and Secondary Calibration should be performed at least monthly. Of course, more frequent calibration will result in greater confidence in results.
3. All calibration information is retained in memory when the **WP-90** is switched off, even when the battery is removed. This information can be recalled or printed later using the GLP function (see section 9).
4. The **WP-90** displays the value of the standard to which it will attempt to calibrate. Ensure that the standard value displayed corresponds to the standard that you are using. Alter the set-up if necessary (see section 3)

4.3 Calibration Messages

1. If a Primary Calibration has been successfully performed, the **WP-90** will display the following message, and the offset value of the sensor. For example...

```
Primary Cal. OK  
Offset=      1.0mV
```

2. If a Secondary Calibration has been successfully performed, the **WP-90** will display the following message, and the slope value of the sensor. For example...

```
Sec Cal. OK  
Slope= 99.0%
```

3. If a Secondary Calibration has failed, the **WP-90** will display the following message, and the failed span value of the sensor. For example...






```
Sec Cal. Failed  
Slope= 49.0%
```

Notes

1. The Offset range is unlimited, as long as the reading is not over-ranged. This is to allow for the large variety of Ion Selective Electrodes available.
2. The allowable Slope range is 50.0% to 110.0%. This range is ample to allow for correctly functioning Ion Selective Electrodes.

5. pH Calibration

5.1 Calibration Procedure

1. Plug the pH sensor into the **Sensor** socket.
2. Switch the meter on.
3. Ensure that you are using buffers which have been selected for automatic buffer recognition. See section 16 for a detailed explanation.
4. Select pH Mode ( → **F3:Mode** → **F2:pH**).
5. Ensure that temperature has already been calibrated, or manually set (see sections 8.1 and 8.4). NOTE: If the decimal point in the temperature reading is shown by a *, then the temperature readout is not calibrated.
6. Remove the wetting cap from the pH sensor.
7. Rinse the pH and Temperature sensors in distilled water and blot them dry.
8. Ensure that you are using the primary buffer for which the **WP-90** has been set (see section 16).
Place both sensors into a small sample of pH7.00 (or pH6.86) buffer, so that the bulb and reference junction are both covered.
DO NOT place the sensors directly into the buffer bottle.
9. Select pH Calibration ( → **F1:Ca1.** → **F1:pH**).
10. When the reading has stabilised, press the  key to calibrate. If a 1 point calibration has been performed, the * will not be removed until a full 2 point calibration has been performed.
11. Rinse the pH and Temperature sensors in distilled water and blot them dry.
12. Place both sensors into a small sample of pH4.01, pH9.18 or pH10.01 Buffer, so that the bulb and reference junction are both covered. **DO NOT** place the sensors directly into the buffer bottle.
pH9.18 and pH10.01 buffers are unstable once the bottles have been opened. Discard immediately after use.
13. Select pH Calibration ( → **F1:Ca1.** → **F1:pH**).
14. When the reading has stabilised, press the  key to calibrate. The * will now be replaced by a decimal point, if calibration was successful.
15. The **WP-90** is now calibrated for pH and is ready for use. Discard the used samples of buffer.

5.2 Calibration Notes

1. A 1-point calibration should be performed at least weekly. In applications where the electrode junction can become blocked, such as dairy products, mining slurries etc, a 1-point calibration may have to be done daily.
2. A full 2-point calibration should be performed at least monthly. More frequent calibration will result in greater confidence in results.
3. All calibration information is retained in memory when the **WP-90** is switched off, even when the battery is removed. This information can be recalled or printed later using the GLP function (see section 9).
4. The **WP-90** displays the value of the pH buffer to which it will attempt to calibrate. Ensure that the buffer value displayed corresponds to the buffer that you are using.

5.3 Calibration Messages

1. If a 1-point Calibration has been successfully performed, the **WP-90** will display the following message, and the asymmetry value of the sensor. For example...

```
1 Point Cal.OK
Asy=0.10pH
```

2. If a 1-Point Calibration has failed, the **WP-90** will display the following message and the failed asymmetry value of the sensor. For example...

```
1 Point Cal.Fail
Asy=1.50pH
```

3. If a 2-Point Calibration has been successfully performed, the **WP-90** will display the following message, and the asymmetry and slope values of the sensor. For example...

```
2 Point Cal.OK
Asy=0.10pH
```

then:

```
2 Point Cal.OK
Slope= 99.0%
```

4. If a Secondary Calibration has failed, the **WP-90** will display the following message, and the failed slope value of the sensor. For example...

```
2 Point Cal.Fail
Slope= 70.0%
```

or:

```
2 Point Cal.Fail
Slope=130.0%
```

Notes


1. The allowable Asymmetry range is -1.00pH to $+1.00\text{pH}$.
2. The allowable Slope range is 85.0% to 105.0% .

6. mV/ORP Calibration


The mV/ORP section is factory calibrated. There is no sensor calibration using a calibration standard for this mode.


7. Relative mV/ORP Calibration

Select Relative mV/ORP mode when measurements relative to a calibration standard are required. Calibration of the Relative mV/ORP mode is simply a matter of zeroing the reading when the sensor is in the calibration standard.


1. Plug the ORP sensor into the **Sensor** socket. Temperature compensation is not applied in Relative mV/ORP mode, so the temperature sensor does not need to be connected.
2. Switch the meter on.
3. Select Relative mV/ORP Mode ( → **F3:Mode** → **F4:Rel mV**).


The display should now be showing Relative mV on the top line with absolute mV or date and time on the bottom line. For example...




Press  to alternate between absolute mV/ORP or the clock on the bottom line.

4. Remove the wetting cap from the ORP sensor.
5. Rinse the sensor in distilled water and blot dry.
6. Place the ORP sensor into a sample of the calibration standard. Ensure that the platinum tip and reference junction are both covered.

When the reading has stabilised, press the  key to zero the Relative mV reading. The Relative mV reading will now be zero, and the absolute mV reading will remain unchanged. For example...



7. The **WP-90** Relative mV/ORP mode is now zeroed and is ready for use. The readout can be re-zeroed by pressing the  key whenever required.


7.1 Notes


1. The Relative mV offset is retained in memory when the **WP-90** is switched off, even when the battery is removed.
2. The Relative mV zero is reset when leaving Relative mV mode.

8. Temperature Calibration





The temperature readout must be calibrated or manually set before attempting Specific Ion or pH calibration. The decimal point is replaced by a "*" if the reading is not calibrated.

8.1 Calibration Procedure

1. Plug the Temperature sensor into the **Temperature** socket.
2. Switch the meter on.
3. Place the sensor into a beaker of room temperature water, alongside a good quality mercury thermometer. Stir the sensor and the thermometer gently to ensure an even temperature throughout the beaker.
4. Select Temperature Calibration ( → **F1:Ca1.** → **F2:Temp**).
5. The reading from the sensor is now displayed on the right of the display, and the value you are going to set is shown on the left. A "*" in the reading indicates that the **WP-90** is currently not calibrated. For example...



→ 25.0 ← 24*0°C
 ↑↓:Set F1:Ca1.


6. When the reading on the right has stabilised, press the  and  keys until the reading on the left shows the same temperature as the mercury thermometer.
7. Press the  key to calibrate the temperature readout.
 The * will now be replaced by a decimal point, if calibration was successful.
 Alternatively, press the  key to abort temperature calibration.
8. The **WP-90** is now calibrated for Temperature and is ready for use. The unit can now be calibrated for Specific Ions and pH.

8.2 Calibration Notes

1. Temperature calibration information is retained in memory when the **WP-90** is switched off, even when the battery is removed. This information can be recalled or printed later using the GLP function (see section 9).
2. Temperature does not need to be re-calibrated unless the sensor is replaced or the meter is initialised.


8.3 Calibration Messages

1. If a temperature calibration has been successfully performed, the **WP-90** will display the following message and the offset value of the sensor.



```
Calibrate OK
Offset= 1.0°C
```


2. If a temperature calibration has failed, the **WP-90** will display the following message, and the failed offset value of the sensor.



```
Calibrate Fail
Offset= 10.5°C
```





8.4 Manual Temperature Setting

If the temperature sensor is not connected, the temperature of the sample solution must be set manually for accurate Specific Ion and pH measurements. A separate thermometer will be required for this.

1. Switch the meter on.
2. Measure the temperature of the sample.
3. Select Temperature Calibration ( → **F1:Ca1.** → **F2:Temp**)
4. The current temperature setting is now displayed. For example...




```
25.0 ← Man Temp
↑↓:Set   F1:Save
```

5. Press the  and  keys until the display shows the temperature of the sample.
6. Press the  key to save the temperature value.
Alternatively, press the  key to quit and retain the current setting.




9. Good Laboratory Practices (GLP)

The **WP-90** keeps a record of the date and time of the last Specific Ion, pH and Temperature calibrations as part of GLP guidelines.

9.1 To recall GLP information on the display

1. Select the GLP menu. ( → **F4:Setup** → **F3:GLP**)
2. Select **F1:Recall**.
3. The instrument model, firmware version number, and instrument serial number are displayed, along with a prompt describing how to scroll through the GLP information.

```
WP90 V2.0 R1234
↓:More ↑:Back
```

4. Press the  key to sequentially scroll through the GLP information for all parameters. Press the  key to scroll back to previous data. The sequence of information displayed is shown over the page. Press  to abort at any time.

GLP Display sequence...


```
WP90 V2.0 R1234
↓:More ↑:Back
```




```
Ion Offs 10.0mv
@ 31/12/11 11:00
```



```
Ion Slope 99.0%
@ 31/12/11 11:10
```



```
pH Asy 0.10pH
@ 31/12/11 11:20
```



```
pH Slope 99.0%
@ 31/12/11 11:30
```



```
Temp Offset 1.0°C
@ 31/12/11 11:40
```



```
Exit
```


9.2 Failed Calibration

If calibration has failed, the GLP function will reset the date and time to zero. The **WP-90** still shows the results of the last successful calibration. These calibration values are still used if further measurements are taken without re-calibrating. For example...

```
Ion Offs  10.0mv
@ 00/00/00 00:00
```

```
Ion Slope 99.0%
@ 00/00/00 00:00
```

```
pH Asy   0.10pH
@ 00/00/00 00:00
```

```
pH Slope 99.0%
@ 00/00/00 00:00
```


```
Temp Offset 1.0°C
@ 00/00/00 00:00
```

9.3 Printing GLP Information to the RS232 Port

The GLP information stored in the instrument's memory can be sent to a printer or PC via the RS232 port.

Switch the meter on.

Ensure that the **WP-90** RS232 cable is connected to the instrument and to the printer or PC.

Select the GLP menu. ( → **F4:Setup** → **F3:GLP**)

Select **F3:Print**.

The GLP information is sent to the RS232 port in formatted ASCII text.


For example...

```
WP90 V2.0 R1234 @ 31/12/11 12:00
Ion      Offset= 10.0mV @ 31/12/11 11:00
Ion      Slope=  99.0% @ 31/12/11 11:10
pH       Asy=   0.10pH @ 31/12/11 11:20
pH       Slope= 99.0% @ 31/12/11 11:30
Temperature Offset= 1.0oC @ 31/12/11 11:40
ENDS
```

9.4 Instrument Serial Number

In case the barcode serial number that is fitted to the rear of the **WP-90** is removed or becomes illegible, it is also available on the **WP-90** display.

- The serial number is displayed at turn-on...



WP90 V2.0 R1234
Ion pH ORP °C

where **R1234** is the serial number.

- The serial number is displayed when recalling the GLP information (section 9.1).
- The serial number is included on the printout of GLP information (section 9.3).

9.5 Additional GLP Features


Another GLP requirement is to record the date and time of every reading. The **WP-90** does this for you when readings are recorded either with the Notepad function (section 10.1) or the Automatic Logging function (section 11).

10. Notepad Function

10.1 Recording Readings into the Notepad

To record readings into the Notepad memory:

1. Press **F1** in normal display mode. The display should now look like this...




100.0ppM 25.0°C
F1: 1 12:00:00

2. Press **F1**, to record the current Specific Ion/pH/mV/ORP, Temperature, Date and Time into the notepad, and labelled as reading number 1.
3. Repeat steps 1 & 2 as often as required. The maximum number of readings that can be stored in the Notepad is 3600.

10.2 Recalling Records from the Notepad


To recall records from the Notepad onto the **WP-90** display...

1. Select the Notepad menu (**Menu** → **F2:Notepad**)
2. Select **F1:Recall** from the menu.
3. Record number 1 is now displayed. For example...



100.0ppM 25.0°C
1 F2:C1k

4. Press **F2** to alternate between the data and the date and time for this record. For example...





100.0ppM 25.0°C ← **F2** → 31/12 12:00:00
1 F2:C1k # 1 F2:Dat

5. Press **▲** to move forward through the records.
Press **▼** to move backward through the records.
Press and hold the **▲** or **▼** keys to roll rapidly through the readings.



10.3 Erasing Records from the Notepad

To erase all records from the Notepad...

1. Select the Notepad menu ( → **F2:Notepad**)
2. Select **F2:Erase** from the menu.
3. The **WP-90** now asks if you are sure that you wish to erase all records.



Erase, You Sure?
F1:Yes F2:No


4. Press  to erase all records from the Notepad.
Press  to quit without erasing the records from the Notepad.


10.4 Printing Records from the Notepad to the RS232 Port

1. Connect one end of the RS232 cable to the **Charger/RS232** socket of the **WP-90**. The charger, optional solar panel, or optional car battery lead can be connected into the spare socket on the cable for long term use, if required.
2. Connect the other end of the RS232 cable to an RS232 Printer, or to COM1 or COM2 of a PC.
3. Ensure that the baud rate for the printer or PC and the **WP-90** are the same.

If necessary, alter the baud rate of the **WP-90** (see section 12.1).


The **WP-90** uses XON/XOFF protocol. Ensure that the printer is set accordingly.

4. Select the Notepad menu ( → **F2:Notepad**).
5. Select **F3:Print** from the menu.


Printing starts as soon as  is pressed. The display shows the word “**Printing**” until printing is completed.

11. Automatic Data logging



The **WP-90** can automatically log readings. First the logging period must be programmed, then automatic logging can be started and stopped as required.


1. Select the Notepad menu ( → **F2:Notepad**).
2. Select **F4:Prog.** from the menu.


The display should now look like this...





The screenshot shows a green rectangular display area with the following text:
→00← F1:Min F2:Sec
↑↓:Period F3:Hr

3. Use the  and  keys to set the period at which the **WP-90** will automatically log records.
4. When the logging period has been correctly set, select whether this period is in minutes, seconds or hours.


Press  to save the period as minutes.

Press  to save the period as seconds.

Press  to save the period as hours.

For example, if the period is set to **05**, followed by  , then the **WP-90** will automatically log a record every 5 seconds.

5. The **WP-90** will ask if the records are to be logged into the Notepad, or sent directly to the RS232 port.

Press  to log records into the Notepad (maximum of 3600 readings).

Press  to send records directly to the RS232 port.

5. The automatic logging function is now programmed, and can be started and stopped as required.

6. To start automatic logging, press **F3** in normal display mode.

If the **WP-90** is logging into the Notepad, the display will look like this...

```
100.0ppM   25.0°C  
Log#  1 12:00:00
```

The log number will increment and the **WP-90** will beep each time a reading is recorded.

If the **WP-90** is sending records directly to the RS232 port, the display will look like this...

```
100.0ppM   25.0°C  
Sending 12:00:00
```

The **WP-90** will beep each time a record is sent to the RS232 port.


7. Press **F3** to stop automatic logging.


Notes:

1. The clock must be set before the **WP-90** will allow automatic logging to start. The message "**Clock Not Set**" is displayed if the clock is not set.
2. The Battery Saver function (section 13) is disabled while the meter is in Automatic Data logging mode, to stop the meter switching off while logging data. Even when the memory is full and the meter stops logging, the Battery Saver function is still disabled. This allows the data to be downloaded and the memory to be reset remotely.






12. RS232 Port

12.1 Setting the Baud Rate


1. Select the RS232 Set-up menu ( → **F4:Setup** → **F4:Baud**)
2. The available baud rates are listed on the display...



The arrow shows the current selection.

3. Press  to select 300 baud
Press  to select 1200 baud
Press  to select 9600 baud
Press  to select 19200 baud.
Press  to quit and retain the current setting.

12.2 Sending Readings to the RS232 Port

Press  to instantly send readings to the RS232 port whenever the **WP-90** is in normal display mode. This function is disabled if the automatic logging period is set to greater than zero (see section 11).

Records can be sent directly to the RS232 port rather than stored in memory during automatic data logging. See section 11 for details.

12.3 RS232 Configuration

The **WP-90** RS232 configuration is 8 bits, No Parity, 1 Stop Bit, XON/XOFF Protocol.

12.4 Communication and Statistical Software

Communication between the **WP-90** and a PC can be handled with any RS232 communication software. The diskette supplied by TPS contains a BASIC program for this purpose. A Windows[®] version is also optionally available.

Once the data is saved to disk, the next problem is how to use it. The data is formatted columns that can be imported by programs such as Microsoft[®] Excel[®] and Lotus 123[®].

Information on how to use the software is provided in the README files on the diskette.

12.5 Commands

The following commands can be sent from a PC to the **WP-90**. Note that <cr> denotes carriage return and <lf> denotes a line feed.

Action	Command	Notes
Request current data	?D<cr>	Returns the current Specific Ion/pH/mV/ORP, Temperature, date and time from the WP-90 . The log number returned is set to zero.
Request logged data	?R<cr>	Returns all logged records from the WP-90 memory. The data ends with the message ENDS<cr>
Erase logged data	?E<cr>	Erases all logged records from the WP-90 memory. Returns the message ERASED<cr> to confirm that the records have been erased.
Request status information	?S<cr>	Returns the model name, firmware version number, instrument serial number and number of logged readings in memory, eg: WP90♦V2.0♦R1234♦9999<cr> , where ♦ are spaces. Note that the number of logged readings is right-justified.
Request GLP information	?G<cr>	Returns all calibration GLP information, plus the instrument model and current date (see section 12.6 for data format and handshaking).

12.6 Data Format

Data is returned to the RS232 port by the **WP-90** in the following format...

LLLL♦DDDDDDDDUUU♦TTTTTTTTuuu♦dd/mm/yy♦hh:mm:ss

where...

LLLL is the Log Number. Maximum 4 characters, right justified.
The **WP-90** sends a Zero for instant readings (section 12.2)

♦ is one space.

DDDDDDDD is Specific Ion, pH, mV/ORP or Relative mV/ORP data, maximum 8 characters, right justified.

UUU is the unit description. Either “**ppM**”, “**ppK**”, “**pH♦**”, “**mV♦**”, “**mVR**”. “♦♦” is sent for Exponential readout of Specific Ions.

♦ is one space. (♦ are spaces.)

TTTTTTTT is the Temperature Data, maximum 8 characters, right justified.

uuu is the Temperature unit description. Either “**oC♦**” for real temperature data (where ♦ is 1 space), or “**oCm**” for manual temperature compensation data.

♦ is one space.

dd/mm/yy is the date, month and year data.

♦ is one space.

hh:mm:ss is the hours, minutes and seconds data.

When data is requested by a PC with the ?D or ?R commands (section 12.5), it is terminated with a carriage return.

When data is sent by the **WP-90** using the Print function (section 10.4) or the Instant Send function (section 12.2), the data ends with a carriage return and a line feed.

When the Temperature is not within the ATC limits for Specific Ion or pH measurement “ATCLIM” will be sent instead of the Data.

12.7 GLP Data Format

GLP information is returned as 7 lines terminated by a carriage return. When using the “?G” command (section 12.5), the computer must respond with a character after receiving each line.

For example...

```
WP90 V2.0 R1234 @ 31/12/11 12:00
Ion      Offset=    10.0mV @ 31/12/11 11:00
Ion      Slope=     99.0% @ 31/12/11 11:10
pH       Asy=       0.10pH @ 31/12/11 11:20
pH       Slope=     99.0% @ 31/12/11 11:30
Temperature Offset=  1.0oC @ 31/12/11 11:40
ENDS
```

13. Battery Saver Function

The **WP-90** is equipped with a battery saver function. If no button has been pressed for five minutes, the unit beeps and flashes the display for 20 seconds, and then shuts off. This function can be switched off for continuous use.

To enable or disable the battery saver function...


1. Switch the meter on.
2. Select Battery Saver Set-up ( → **F4:Setup** → **F1:Batt**)

The battery saver menu is now displayed...



The arrow indicates the current selection.


The bar graph and percentage indicate the approximate level of charge in the battery.

3. Press **F1** to disable the battery saver function for continuous use.
Press **F2** to enable the battery saver function. The meter will switch itself off if no key has been pressed for five minutes.
Press  to quit the battery saver menu and retain the current setting.


Notes:

1. For troubleshooting purposes, the battery volts can also be displayed in the battery saver menu. Press **F3** to display battery volts.
2. The Battery Saver function is disabled while the meter is in Automatic Data logging mode (section 11), to stop the meter switching off while logging data. Even when the memory is full and the meter stops logging, the Battery Saver function is still disabled. This allows the data to be downloaded and the memory reset remotely.

14. Recharging the Battery


The  symbol flashes when the battery drops below 5.60 volts. The battery should be recharged at this point. If the battery is not recharged, the **WP-90** will switch itself off when the battery drops below 5.00 volts.

To recharge the battery...


1. Plug the battery charger, solar panel, or car cigarette lighter adaptor into the **Charger/RS232** socket. **DO NOT** plug into the **Temperature** socket, as this will damage the **WP-90**.
2. Charge for approximately 8 hours for full capacity. The **WP-90** has special circuitry to prevent overcharging, so the charger can be used continuously.
3. To ensure optimum battery life and capacity, the **WP-90** should only be charged once the  symbol starts to flash.

15. Clock Function















15.1 Setting the Clock


1. Select the Clock Set-up menu ( → **F4:Setup** → **F2:Clock**).


The display now shows the current date and time. The cursor starts at the day.




```
31/12/11 12:00
F1:← F2:→ ↑↓:Set
```

2. Press the  and  keys until the day is correct.
3. Press  to move to the month. Press the  and  keys until the month is correct.
4. Press  to move to the year. Press the  and  keys until the year is correct.
5. Press  to move to the hour. Press the  and  keys until the hour is correct.
6. Press  to move the cursor to the minutes. Press the  and  keys until the minutes are correct.
7. Check that the date and time are correct.

If any changes are needed, press the  key to move left to the desired position.



8. Press  when the cursor is in the “minutes” position to save the settings.

Press  to quit without resetting the clock.

Note

The **WP-90** does not test for a valid day of the month when setting the clock (eg: attempting to enter 31/02/11 is not corrected).

15.2 Displaying or Hiding the Clock

Date and time are normally displayed along with the Specific Ion/pH/mV/ORP and Temperature readings. Press  in normal display mode to alternatively display or hide the clock. When Relative mV/ORP is selected, the  key alternatively displays the clock or absolute mV.

16. Selecting Buffers for Auto Buffer Recognition

The **WP-90** is factory set to automatically recognise pH4.01, pH7.00 and pH9.18 buffers. However, some users may prefer to use pH6.86 instead of pH7.00 and pH10.01 instead of pH9.18. The following procedure describes how to set which of these buffers are automatically recognised at calibration.

1. Switch the meter **OFF**.
2. Press and HOLD the **(F1)** key while switching the meter back on.

The buffer selection menu is now displayed.

```
Select →F1:7.00pH
Buffer  F2:6.86pH
```

The arrow indicates the current selection.

3. Press **(F1)** to select pH7.00 as the primary buffer.
Press **(F2)** to select pH6.86 as the primary buffer.
Press **(Menu)** to quit buffer selection and retain the current setting.
4. The display will now show the currently selected high pH buffer.

```
Select →F1:9.18pH
Buffer  F2:10.0pH
```


The arrow indicates the current selection.

5. Press **(F1)** to select pH9.18 as the high pH buffer.
Press **(F2)** to select pH10.01 as the high pH buffer (the display shows 10.0 for the latter, but this buffer is stored as pH10.01).
6. Press **(Menu)** to quit buffer selection and retain the current setting.
7. The setting is kept in memory when the meter is switched off, even if the battery is removed.

17. Initialising the WP-90

If the calibration settings of the **WP-90** exceed the allowable limits, the unit may need to be initialised to factory default values.

To initialise the **WP-90**...

8. Switch the **WP-90 OFF**.
9. Press and HOLD the  key while switching the **WP-90** back on.

The following messages should be displayed...

**Initialized
MUST ReCalibrate**

then:

**WP90s V2.0 R1234
Ion pH ORP °C**

(The “s” after **WP-90** is shown when the RS232 serial port option is fitted)

10. The meter then displays Specific Ion and Temperature. Note that the decimal points have been replaced with a *, to indicate that the unit requires re-calibration.


18. Instrument firmware version number.

If you need to phone or fax TPS for any further technical assistance, the version number of your **WP-90** firmware may of benefit to us. The version number is displayed by the **WP-90** at turn-on. In the example below, the firmware version number is **V2.0**.

**WP90s V2.0 R1234
Ion pH ORP °C**

19. Troubleshooting

19.1 General Errors

Error Message	Possible Causes	Remedy
Factory Cal. Failed	The EEPROM chip which contains the factory calibration information has failed.	The unit must be returned to TPS for service.
Memory Failed Calibration Lost then: Initialised MUST ReCalibrate	User calibration settings have been lost or corrupted.	Re-calibrate the instrument... <ul style="list-style-type: none"> • 2-point calibration for Specific Ion (section 4.1). • 2-point calibration for pH (section 5.1). • 1-point calibration for temperature (section 8.1).
Flashing  symbol.	Battery is below 5.60 volts.	Recharge the battery. Note that the unit will switch itself off when the battery falls below 5.00 volts.
Meter displays the word OFF , and switches off.	Battery is below 5.00 volts.	Recharge the battery. If this fails, check the charger. If charger OK, replace the battery.
Meter will not turn on.	<ol style="list-style-type: none"> 1. Battery is exhausted. 2. Faulty Instrument 	Recharge the battery. If this fails, check the charger. If charger OK, replace the battery. Return to factory for repair.
Battery does not charge up when charger is connected.	<ol style="list-style-type: none"> 1. Faulty battery charger or faulty battery. 2. Faulty instrument. 	Connect the charger and switch the power on. Display the battery volts in the battery saver menu (section 13). If the battery volts are increasing then the charger is OK. If the battery volts do not increase, then the charger is faulty. Replace the charger or the battery, as required. Return to factory for repair.

19.2 Specific Ion, pH and mV/ORP Troubleshooting

Symptom	Possible Causes	Remedy
Unit fails to calibrate, even with new sensor.	Calibration settings outside of allowable limits due to previous failed calibration.	Initialise the unit. See section 17.
1 Point calibration fails (Specific Ion offset causes over-range reading, or pH asymmetry is greater than ± 1.00 pH.)	<ol style="list-style-type: none"> Reference junction blocked. Reference electrolyte contaminated. 	<p>Clean reference junction, as per instructions supplied with the pH or reference sensor.</p> <p>Flush with distilled water and replace electrolyte.</p>
2 Point calibration fails (Specific Ion slope is less than 50% or pH Slope is less than 85%).	<ol style="list-style-type: none"> Incorrect primary Ion Standard or pH Buffer. Ion sensor surface or pH glass bulb not clean. Sensor is aged. Connector is damp. Ion Standard or pH Buffers are inaccurate. 	<p>Ensure that you are using the primary Ion Standard or pH Buffer for which the WP-90 has been set (sections 3 & 16).</p> <p>Clean Ion sensor or pH glass bulb as per instructions supplied with the sensor.</p> <p>Attempt rejuvenation, as per instructions supplied with the sensor. If not successful, replace sensor.</p> <p>Dry in a warm place.</p> <p>Replace standards or buffers.</p>

Continued next page...

Specific Ion, pH and mV/ORP Troubleshooting, continued...

Unstable readings.	<ol style="list-style-type: none"> 1. Reference electrolyte chamber needs to be refilled. 2. Reference junction blocked. 3. Ion sensor surface or pH glass bulb not clean. 4. Bubble in tip of Ion sensor or pH glass bulb. 5. Faulty connection to meter. 6. Reference junction not immersed. 7. KCl crystals around reference junction, inside the electrolyte chamber. 	<p>Refill electrolyte. See Ion sensor specifications for correct electrolyte. Use saturated KCl for pH sensor.</p> <p>Clean reference junction, as per instructions supplied with the sensor.</p> <p>Clean Ion sensor or pH glass bulb as per instructions supplied with the sensor.</p> <p>Flick the sensor to remove bubble.</p> <p>Check connectors. Replace if necessary.</p> <p>Ensure that the reference junction is fully immersed.</p> <p>Rinse electrolyte chamber with warm distilled water until dissolved. Replace electrolyte.</p>
Inaccurate readings, even when calibration is successful.	Reference junction blocked.	Clean reference junction, as per instructions supplied with the sensor.
Displays constant Specific Ion readings or pH7.00 for all solutions.	Electrical short in connector.	<ol style="list-style-type: none"> 1. Check connector. Replace if necessary. 2. Replace sensor.
Displays constant Specific Ion readings or pH4 to 6 for all solutions.	Ion sensor surface, pH glass bulb cracked, or internal damage.	Replace sensor.
Display flashes "ATC" and "LIMIT"	The Temperature is not within the ATC limits.	Cool/Heat solution before taking measurements.

19.3 Temperature Troubleshooting

Symptom	Possible Causes	Remedy
Displays "OVR°C" when Temperature sensor is plugged in.	<ol style="list-style-type: none"> 1. Faulty temperature sensor. 2. Faulty instrument. 	<p>Return sensor to factory for repair or replacement.</p> <p>Return to factory for repair.</p>
Temperature inaccurate and cannot be calibrated.	<ol style="list-style-type: none"> 1. Faulty connector. 2. Faulty Temperature sensor. 3. Faulty instrument. 	<p>Check the connector and replace if necessary.</p> <p>Return sensor to factory for repair or replacement.</p> <p>Return to factory for repair.</p>

20. pH Sensor Fundamentals

A combination pH Sensor is two sensors in one. The sensing membrane is the round or spear shaped bulb at the tip of the sensor. This produces a voltage that changes with the pH of the Solution. This voltage is measured with respect to the second part of the sensor, the reference section. The reference section makes contact with the sample solution using a salt bridge, which is referred to as the reference junction. A saturated solution of KCl is used to make contact with the sample. It is vital that the KCl solution has an adequate flow rate in order to obtain stable, accurate pH measurements.

20.1 Asymmetry of a pH Sensor

An "ideal" pH sensor produces 0 mV output at 7.00 pH. In practice, pH sensors, generally produce 0 mV output at slightly above or below 7.00 pH. The amount of variance from 7.00 pH is called the asymmetry. Figure 20-1 illustrates how asymmetry is expressed.

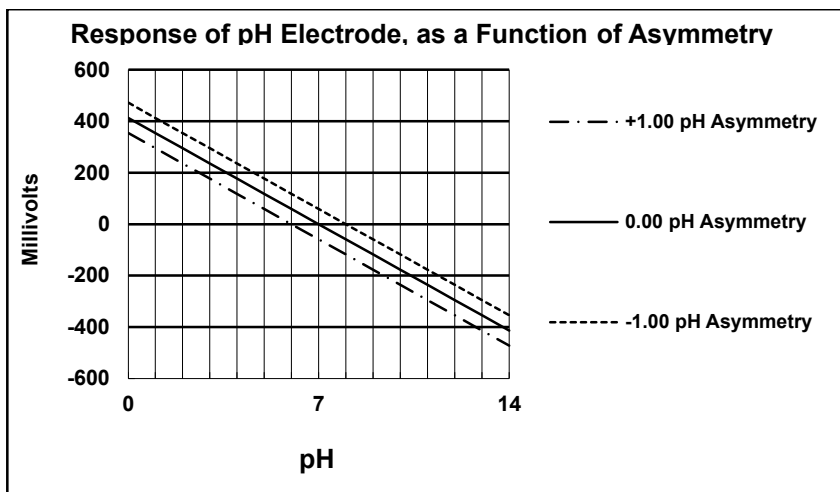


Figure 20-1

20.2 Slope of a pH Sensor

As mentioned above, a pH sensor produces 0 mV output at around 7.00 pH. As the pH goes up, an “ideal” pH sensor produces -59mV/pH unit at 25 °C. As the pH goes down, an ideal pH sensor produces +59mV/pH unit. In practice, pH sensors usually produce slightly less than this. The output of a pH sensor is expressed as a percentage of an ideal sensor. For example, an ideal sensor that produces 59mV/pH unit has “100% Slope”. An sensor that produces 50.15mV/pH unit has “85% Slope” (see Figure 20-2).

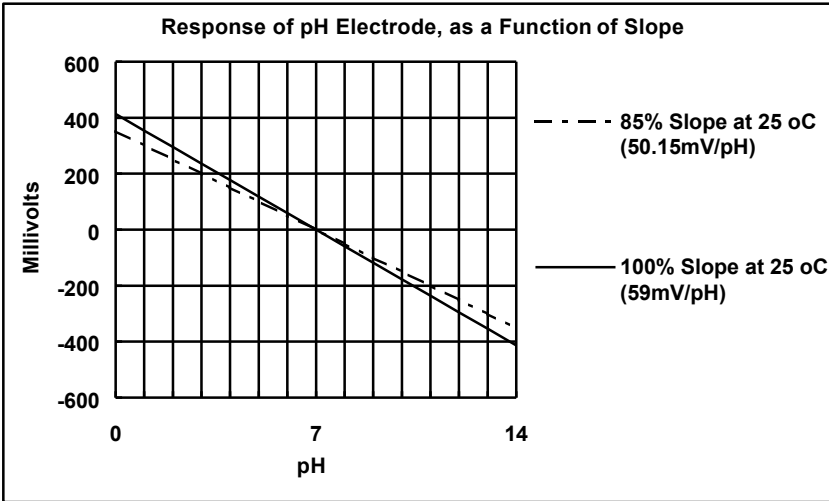


Figure 20-2

20.3 pH Temperature Compensation

The slope of a pH sensor (section 20.2) is affected by temperature. This effect is compensated for either by using an Automatic Temperature Compensation (ATC) sensor or by entering the sample temperature manually. Figure 20-3 shows the slope of a pH sensor at various temperatures.

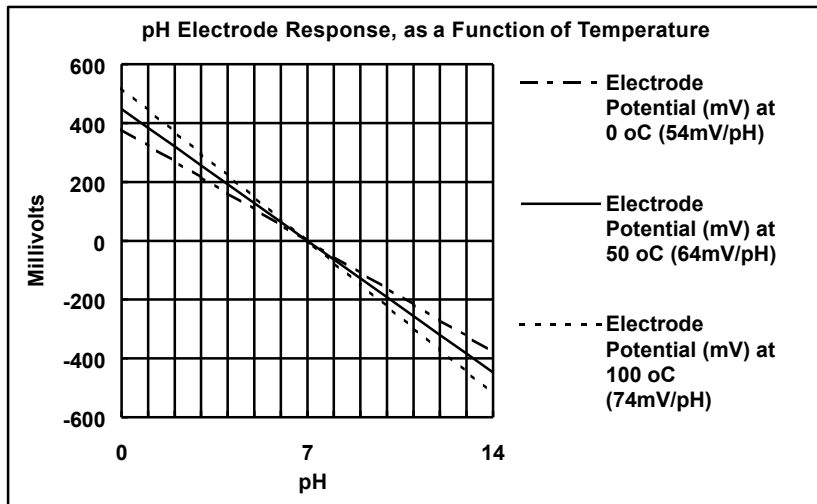


Figure 20-3