

Package Insert

EndoTrap[®] red

- Cat. No. LET0001 - EndoTrap[®] red 1/1
- Cat. No. LET0002 - EndoTrap[®] red 5/1
- Cat. No. LET0003 - EndoTrap[®] red 10
- Cat. No. LET0004 - EndoTrap[®] red 50
- Cat. No. LET0033 - EndoTrap[®] red 5
- Cat. No. LET0034 - EndoTrap[®] red Buffer Kit:
 - LET0005 - 5x EndoTrap[®] red Equilibration Buffer, 125 mL
 - LET0008 - 5x EndoTrap[®] red Regeneration Buffer, 125 mL

Distributed by:



Ilex Life Sciences LLC
1465 Sand Hill Rd, Ste 2018
Candler, NC 28715
United States
Tel: (828) 531-9949
Email: info@ilexlife.com
<https://ilexlife.com/>

For laboratory and research use only. Not for use in diagnostic procedures.

Store the kits at +2 to 8 °C

Table of Contents


1. General Information	3
1.1 Intended Use	3
1.2 Principle	3
1.3 EndoTrap® Kit Components.....	3
1.4 Specifications	4
1.5 Precautions.....	4
2. EndoTrap® Protocols	5
2.1 Protocol Column Mode	5
2.2 Protocol Batch Mode	6
2.3 How to work with a real flow through system.....	6
2.4 Optional Steps (Column / Batch Mode)	6
3. Additional Information	7
3.1 How to calculate the number of required cleaning steps	7
3.2 EndoTrap® HD.....	7
3.3 Custom Specific Buffers	8
3.4 EndoTrap® Equilibration Buffer Composition	8
3.5 Sample Applications for EndoTrap® blue and EndoTrap® red	9
3.6 Trouble Shooting Guide.....	10
4. Technical Support and Further Product Information	11
4.1 Inquiries and Technical Support	11
4.2 Legal Statements and Patent Information.....	11
4.3 Related Products by LIONEX	11

1. General Information

1.1 Intended Use


EndoTrap® is an affinity matrix intended for removal of lipopolysaccharide (LPS) from biological samples in aqueous solutions such as proteins, antibodies, cell extracts and nucleic acids. EndoTrap® can be employed in both batch and column mode.

1.2 Principle

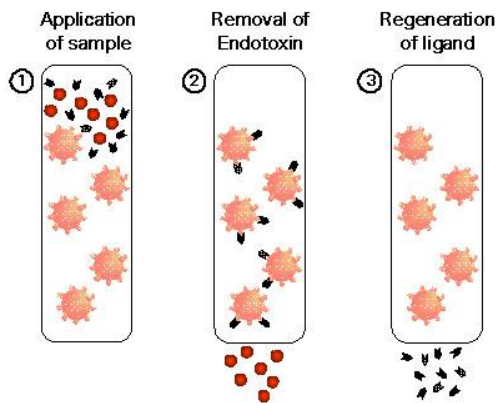

Principle of EndoTrap®:

1. Endotoxin-contaminated proteins and aqueous solutions are applied.
2. The endotoxin is specifically bound to the beads, elution of proteins.
3. Regeneration of ligand by addition of regeneration buffer.

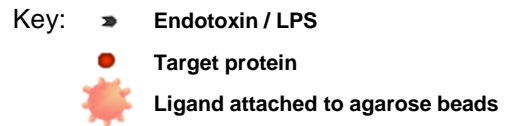

1.3 EndoTrap® Kit Components

Kit Components

EndoTrap® red 1/1	EndoTrap® red 5/1
1x1 ml column	5x1 ml column
25 ml 5x equilibration buffer	125 ml 5x equilibration buffer
25 ml 5x regeneration buffer	125 ml 5x regeneration buffer

Related products

EndoTrap® red 5	EndoTrap® red 10	EndoTrap® red 50
5 ml settled resin	10 ml settled resin	50 ml settled resin

EndoTrap® red Buffer Kit:

- 125 mL 5x EndoTrap® red Equilibration Buffer
- 125 mL 5x EndoTrap® red Regeneration Buffer

1.4 Specifications

EndoTrap® ligand	LPS-specific bacteriophage derived protein
Binding capacity	2 x 10 ⁶ EU/ml resin (1 EU = 100 pg LPS)
Dissociation constant	K _D = 5 x 10 ⁻⁸ M
Support matrix	Highly cross-linked 4% agarose , spherical beads
Void volume	0.3 to 0.5 ml
Mean particle size	90 µm
Max. flow rate	0.2 to 1 ml/min
Max. pressure	0.3 MPa (when using automated systems), 43 psi
Temperature stability	Between 4°C and room temperature
Storage	At 2 - 8°C in regeneration buffer supplemented with 0.02% sodium azide. Do not freeze!
Shelf life	EndoTrap® is stable until the stated expiry date when stored according to instructions.

1.5 Precautions

- EndoTrap® 5x buffers (Cat. No. LET0034 also contained in EndoTrap® red 1/1 and 5/1 (Cat. No. LET0001 and LET0002) have to be diluted 1:5 with endotoxin-free water prior to use.
- Buffers, resin and samples should have the same temperature (4 - 20°C) during the cleaning steps.
- Buffers must be prepared from endotoxin-free materials and endotoxin-free water.
- All materials used, such as containers, pipette tips and buffers, must be endotoxin-free. Glass ware is preferred, as endotoxins can be destroyed by heat treatment (200 °C, 4 h or 250 °C, 1 h). Endotoxin-free EndoGrade® Glass Test Tubes (capacity 5 ml) are supplied by LIONEX.
- Empty columns and funnels are available from LIONEX and supplied **not endotoxin-free**. In order to exclude any co-contamination with LPS, empty columns and funnels should be inserted in at least 1 M NaOH overnight (6 - 12 h), subsequently washed with endotoxin-free water and air dried. The protocol "Procedure for packing gel into a column" is available from LIONEX on request.
- EndoTrap® resins and pre-filled columns are supplied with ProClin® as a preservative. For safety information see the EndoTrap® Material Safety Data Sheet.
- For proteases see chapter 3.6 on page 10.
- The most important considerations for EndoTrap® red:

	EndoTrap® red
▪ pH (buffer)	pH 6-9
▪ Highest ionic strength possible	250 mM NaCl best results at < 100 mM NaCl
▪ Suitable with EDTA and other calcium chelators containing buffers	Yes
▪ Customer specific equilibration buffer has to be enriched with calcium	No
▪ PBS can be used as equilibration buffer <i>See 3.3 on page 8 for further details</i>	Yes, "half-concentrated" PBS should be used

2. EndoTrap® Protocols

Chromatography is commonly performed in two modes: continuous (column mode) chromatography and discontinuous (batch mode).

EndoTrap® can be used in both column and batch mode. Removal of high endotoxin levels is generally more convenient in the column mode. Batch mode may be used for small volumes or to increase contact time. Parameters such as pH, ionic strength, temperature and contact time should be optimized for each application to obtain maximum endotoxin removal with minimum product loss.

2.1 Protocol Column Mode

A. Preparation

- To use a **prepacked column** place the column in a suitable holder and first remove the **top cap**. This prevents air bubbles from emerging. Next, remove **bottom cap**. Allow the storage solution to drain from the column [~ 8 min]. The flow stops automatically when the solution reaches the upper disc. Make sure to **never** let the EndoTrap® resin dry out! **5x buffers must be diluted 1:5 with endotoxin-free water prior to use.**

B. Activation and Endotoxin Removal


- 1. Fill the column with 3 ml **regeneration buffer (RB)**¹ and let the column drain off completely. Repeat once [~12 min].
- 2. Fill the column with 3 ml **equilibration buffer (EB)**² or customer specific buffer and let the column drain off completely. Repeat once [~12 min].
- 3. Apply the **sample** (either in **equilibration buffer (EB)** or in customer specific buffer) onto the column and start collecting the fractions (depending on the applied sample volume) immediately. The applied sample elutes directly after the column void volume (0.3 to 0.5 ml). The column can be constantly filled up, until the whole sample (up to 50 ml) has been applied. Afterwards let the sample drain completely from column [flow rate: 0.2 to 1 ml/min].
- 4. In order to elute the entire sample, apply additional 1 ml **equilibration buffer (EB)** or customer specific buffer, let the column drain off and collect the flow through completely. [As substances pass through the column at different rates, it is important to test each fraction for the sample concentration. This can be done by for example measuring the optical density of the flow through fractions.]

C. Regeneration

Fill the column with 3 ml **regeneration buffer (RB)** or customer specific buffer and let the column drain off completely. Repeat once [~ 12 min]. **Continue with step B.2.**

D. Storage

Apply 1 ml regeneration buffer (RB), **supplement with ProClin® as preservative** and let the column drain off completely. Close the bottom cap of the column and apply 1 ml regeneration buffer (RB), **supplement with ProClin®** and store at 2 to 8°C (shelf life until the indicated expiry date). Alternatively 20% ethanol can be used as storage buffer; the storage time will then be reduced to 4 weeks.

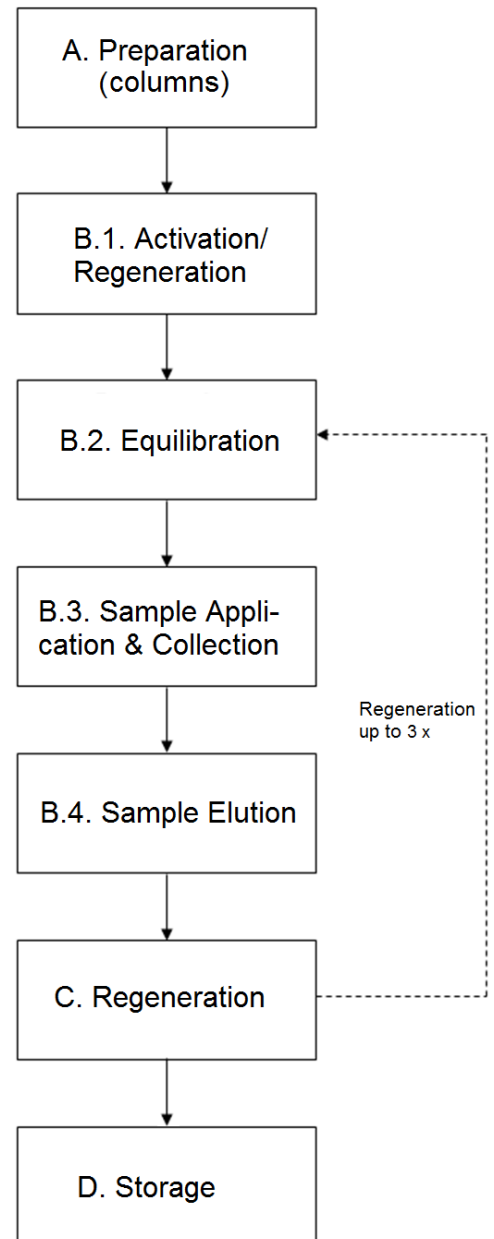

2.2 Protocol Batch Mode

A. Preparation

- A ratio of 2:1 to 10:1 between sample and resin volume is recommended (up to 50 ml sample per ml resin is possible). All centrifugation steps should be carried out at ~ 1200 x g for 5 min (bench top centrifuge)! Several contact times should be tested to determine the optimal contact time for endotoxin removal. Remove the storage buffer from the gel slurry by centrifugation and discard the supernatant. 10x buffers have to be diluted 1:10 with endotoxin-free water prior to use.

B. Activation and Endotoxin Removal

- 1. Add 2 gel volumes of **regeneration buffer (RB)**¹, mix by gently shaking the tube for 5 sec; centrifuge, and discard the supernatant. Repeat twice.
- 2. Add 2 gel volumes of **equilibration buffer (EB)**² or customer specific buffer, mix by gently shaking the tube for 5 sec; centrifuge and discard the supernatant. Repeat twice.
- 3. Add the sample (either in **equilibration buffer (EB)** or in customer specific buffer) and incubate for at least 5 min. Gently shake or rotate the tube while incubating.
- 4. Centrifuge at ~ 1200 x g for 2 min (bench top centrifuge) and transfer the supernatant (sample) to an endotoxin-free tube.

C. Regeneration

Resuspend the EndoTrap® gel pellet in 2 gel volumes of **regeneration buffer (RB)**, mix by gently shaking the tube for 5 sec; centrifuge and discard the supernatant. Repeat twice. Continue with **step B2**.


D. Storage

Resuspend the EndoTrap® gel pellet in 1 gel volume of regeneration buffer (RB), **supplemented with ProClin®** and store at 2 to 8°C (shelf life until the indicated expiry date). Alternatively 20% ethanol can be used as storage buffer; the storage time will then be reduced to 4 weeks.

¹ The regeneration substance is NOT (sodium) deoxycholate! DOC would have cytotoxic effects on cell culture and also influence the cell growth and the morphology of the cells. It is reported that DOC induces DNA damage.

²

5 x Equilibration buffer "red" (EB): provided in the kit (only LET0001, LET0002)

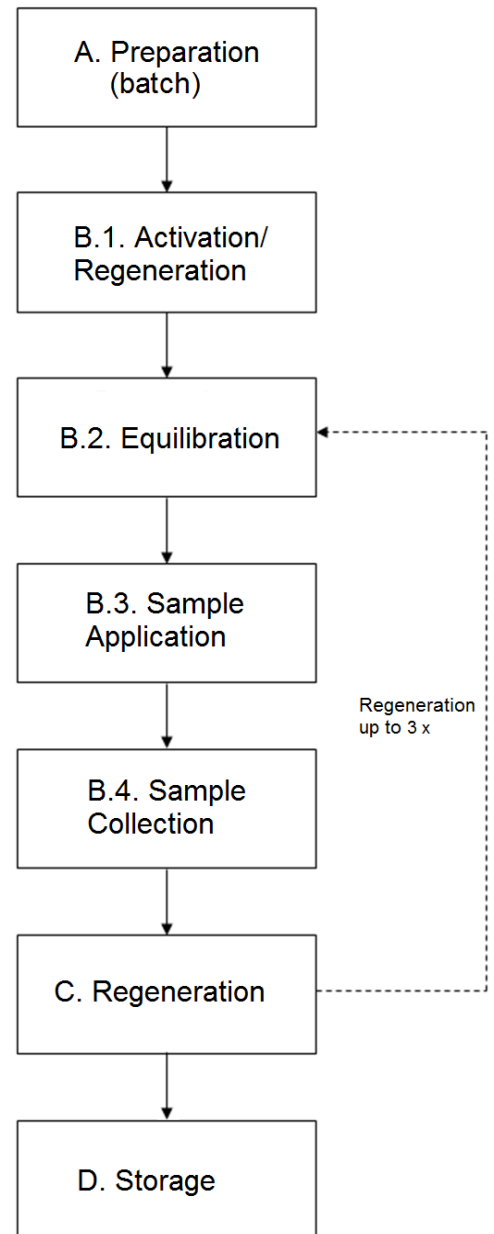

2.3 How to work with a real flow through system

EndoTrap® is a **real flow through system** ("ready-to-use" columns). Apply the sample (up to 50 ml) continuously to a 1 ml column – up to 3 ml at once. With an additional funnel, 20 to 25 ml can be filled at once.

2.4 Optional Steps (Column / Batch Mode)

Endotoxin / LPS detection:

- Check the LPS removal efficiency using an endotoxin detection assay. If the LPS contamination is still too high, perform a second LPS removal step.

Protein polishing / recovery:

- Combine the fractions and filtrate the solution over 0.2 µm membranes to ensure sterile conditions.
- Measure the protein concentration with appropriate methods or measure the absorption at 280 nm.

3. Additional Information

3.1 How to calculate the number of required cleaning steps

EndoTrap® red can be re-used at least three times (EndoTrap® HD at least 10 times) without any loss of endotoxin removal efficiency. If the initial endotoxin concentration is very high or if a very low concentration has to be reached, EndoTrap® can be applied several times in a consecutive manner. Each round of application theoretically yields a two log reduction of endotoxin.

Parameters such as pH, ionic strength, temperature, contact time, etc. can be optimized for each application to obtain maximum endotoxin removal with minimum loss of product.

Depending on the LPS starting concentration [EU] (1 EU = 100 pg LPS), perform a certain number of cleaning steps, in order to achieve the desired LPS end concentration [EU]. To achieve best results, total LPS units applied should not exceed 30 to 50% of the maximum resin capacity.

Starting LPS concentration (buffer) [EU]	After 1. cleaning step [EU]	regeneration step (kit includes regeneration buffer)	After 2. cleaning step [EU]	regeneration step (kit includes regeneration buffer)	After 3. cleaning step [EU]
100.000	1.000		10		3
10.000	100	1	0.3		
1.000	10	3	0.9		
100	1	0.3	0.09		
10	3	0.9	0.27		
1	0.3	0.09	0.027		
0.1	0.03	0.009	< 0.005		

LPS removal from buffers:

With repetitive use of EndoTrap®, concentrations lower than 0.005 EU/ml can be achieved.

LPS removal from proteins:

With repetitive use of EndoTrap®, concentrations lower than 0.1 EU/ml can be achieved. The efficiency of EndoTrap® slightly decreases at low endotoxin contamination levels (0.1 EU/ml), at this concentration the removal efficiency is approximately 70%.

Note that each cleaning step ends is followed by resin (ligand) regeneration.

Related products:

3.2 EndoTrap® HD

EndoTrap® HD offers best-in-class endotoxin binding capacity of **> 5,000,000 EU/ml** and can be **re-used more than 10 times**. Moreover, EndoTrap® HD has been especially optimized for application in biomanufacturing processes. It can be used in early or late bio-manufacturing process steps.

EndoTrap® HD is based on a hydrophilic, dimensionally stable affinity matrix with excellent pressure/flow characteristics. A Regulatory Support File can be provided on request.

EndoTrap® HD is available as pre-filled columns (1x 1 ml and 5x 1 ml, including all necessary buffers) and settled resins (10 ml, 50 ml, 250 ml and bulk).

3.3 Custom Specific Buffers

Custom specific buffers can be used for equilibration and endotoxin binding, the composition depends on which EndoTrap® system (blue or red) is used.

EndoTrap® red

Endotoxin removal with EndoTrap® red is efficient in the pH range of 6 - 9 and NaCl concentrations in the range of 50 - 250 mM (best results with < 100 mM NaCl).

Buffers such as HEPES, PBS, TRIS, MOPS, MES, PIPES and also Citrate, Acetate, Glycine and Carbonate buffers are recommended. EndoTrap® red **is suitable** with chelators of divalent cations (like **EDTA**).

Phosphate buffers with NaCl concentrations below 100 mM are recommended for EndoTrap® red.

Important:

With a “classical” **PBS buffer** (10 mM Na₂HPO₄, 1.8 mM KH₂PO₄, 137 mM NaCl, 2.7 mM KCl, pH 7.4), the LPS removal rate will be ~97% for each cleaning step. With a “half-concentrated” PBS buffer LPS removal rates of ~99% can be achieved.

Therefore, dilute the PBS buffer 1:2 with endotoxin free water (5 mM Na₂HPO₄, 0.9 mM KH₂PO₄, 68.5 mM NaCl, 1.35 mM KCl, pH 7.4).

3.4 EndoTrap® Equilibration Buffer is provided in the kit (LET0001/ LET0002).

EndoTrap® 5x buffers must be diluted 1:5 with endotoxin-free water prior to use.

3.5 Type of Samples which can be used with EndoTrap® red

	EndoTrap® red
Tested substances which can be applied onto the column	<ul style="list-style-type: none"> ▪ proteins ▪ peptides ▪ antibodies
Regeneration buffer (endotoxin concentration < 0.02 EU/ml)	Regeneration buffer "red" (based on "Phosphate buffer", pH7.4)
Equilibration buffer (endotoxin concentration < 0.02 EU/ml)	Equilibration buffer "red" ("Phosphate buffer", pH 7.4 with 80 mM NaCl)
Other suitable equilibration buffers	PBS, HEPES, Borate, TRIS, MOPS, MES, PIPES, Citrate, Acetate, Glycine and Carbonate buffers
pI of applied proteins	pI from 5 - 9
pH (buffer)	pH 6 - 9
Ionic strength	up to 250 mM NaCl < 100 mM NaCl is recommended
Recommended working concentration of applied substances	1 - 10 mg/ml
Recommended sample volume per ml resin	up to 50 ml
Tested substances which do not interfere with the performance of EndoTrap®*	DTT not tested max. 0.005% NaDOC 20% DMSO 20% Isopropanol 40% Methanol 20% Ethanol 20% Glycerol / Glycerin 1 M Urea 300 mM Imidazole
Tested substances which may interfere with the performance of EndoTrap® and therefore having an inhibitory effect on LPS binding	<ul style="list-style-type: none"> ▪ > 250 mM NaCl ▪ SDS, Tween20 and other detergents ▪ GdnHCl ▪ Ammoniumsulphate
Tested LPS-types (bacterial strain)	<ul style="list-style-type: none"> ▪ <i>Escherichia coli</i> K12 ▪ <i>Salmonella enterica</i> ▪ <i>Citrobacter freundii</i> ▪ <i>Pseudomonas aeruginosa</i>
	Use EndoTrap® red for: <ul style="list-style-type: none"> ▪ <i>Klebsiella pneumoniae</i> ▪ <i>Serratia marcescens</i>

3.6 Trouble Shooting Guide

Please consider the chemical characteristics of the used sample before choosing one improvement step.

Issue		EndoTrap® red
... low sample recovery rate ...		
- due to ionic interactions		EndoTrap® red is not suitable for high ionic strength – please use EndoTrap® blue.
- due to interactions with lipopolysaccharides	Hydrophobic interaction of samples with LPS may occur. As lipopolysaccharides form aggregates, it might also be possible that your sample arranges within these aggregates. It may help to disintegrate the aggregates or to reduce their size. For that purpose Triethylamine (combined with 15 min ultrasonic treatment) or detergents can be used. EndoTrap® is suitable for buffers containing 20% glycerol. Note: Detergents may interfere with endotoxin detection in the LAL assay. In this case.	
- due to negative charge of the sample		EndoTrap® red ligand could interact with negative charge – use EndoTrap® blue instead.
- due to interactions with calcium		EndoTrap® red does not need calcium ions
... low LPS removal rate ...		
- due to depletion of calcium		EndoTrap® red does not need calcium ions
- due to interference with buffer additives		Add up to 40% ethanol to the equilibration buffer or customer specific buffer.
- due to limiting contact time	1. Column mode: Use half of the sample or use a smaller column, alternatively close column bottom cap to achieve a longer contact time (max. overnight). 2. Batch mode: Increase the contact time or the resin to sample ratio.	
- due to limiting LPS binding capacity	To achieve best results, total LPS units applied should not exceed 30 to 50% of the maximum column capacity (2 x 10 ⁶ EU/ml resin).	
... slow flow through rate (<< 0.2 to 1 ml/min [gravity flow]) ...		
- due to viscous solutions	EndoTrap® red is not suitable for viscous solutions! For viscous solutions EndoTrap® HD (www.lionex.de) is recommended in batch mode.	
- due to bubbles	Remove bubbles by centrifuging the closed column (filled with buffer by a height of 1 - 2 cm) at ~ 1000 x g for 5 min. (using a "clinical-type" centrifuge, i.e. one with swinging baskets works best). For this procedure please place the column into a suitable 50 ml tube.	

How to deal with proteases when using EndoTrap®?

Proteases may destroy the EndoTrap® ligand during LPS removal. Please perform the cleaning steps at conditions where the protease is less active, e.g. 4°C, or change the buffer composition if possible.

Example: When using pepsin, work above pH 6 since pepsin is an acidic protease.

4. Technical Support and Further Product Information

4.1 Inquiries and Technical Support

Internet Visit EndoTrap® on LIONEX' website www.lionex.de for:
Technical resources including manuals, application notes, Certificates of Analysis, Material Safety Data Sheets (MSDS), FAQs, customer publications and reference customers
Complete technical service contact information

Contact us For more information or technical assistance, call, write, fax or e-mail.

Corporate Headquarters:
LIONEX GmbH
Salzdahlumer Strasse 196, D-38126 Braunschweig,
Germany
Tel: +49 (0) 531 260 12 66
Fax: +49 (0) 531 6180 654
E-mail: purchase@lionex.de or info@lionex.de

4.2 Legal Statements and Patent Information

Trademarks EndoTrap® and EndoGrade® are registered trademarks exclusively licensed to LIONEX GmbH
Tween20® is a registered trademark of ICI America, Inc.

Patent information Parts of EndoTrap® products are protected under the following patents:
EP1516188 and EP1695085

4.3 Related Products by LIONEX

EndoTrap® HD

- **EndoTrap® HD** Endotoxin removal system for High-Definition sample purification

EndoTrap® Leakage ELISA

- **EndoTrap® Leakage ELISA** for determination of EndoTrap® HD binding ligand

EndoGrade® Endotoxin-free Accessories

- **EndoGrade® Glass Test Tubes** - Endotoxin-free borosilicate glass test tubes with screw cap

EndoGrade® Endotoxin-free Reagents

- **EndoGrade® Ovalbumin** - Ultra-pure Ovalbumin for advanced immunology research
- Less than 0.1 EU/mg.

EndoTrap® patented technology has been developed and is exclusively licensed to LIONEX GmbH and is provided for research and biomanufacturing use only.

Copyright: All contents, graphics, forms and programmes are subject to copyright 2018 of LIONEX GmbH, unless stated otherwise. The reproduction, alteration, use or dissemination of the information published here without the written permission of LIONEX GmbH is prohibited.

Distributed by:



Ilex Life Sciences LLC
1465 Sand Hill Rd, Ste 2018
Candler, NC 28715
United States
Tel: (828) 531-9949
Email: info@ilexlife.com
<https://ilexlife.com/>