


KEY-1

PROTONRO D2O {D:\nmrdata\External\2023\19 JULY} nmr 12

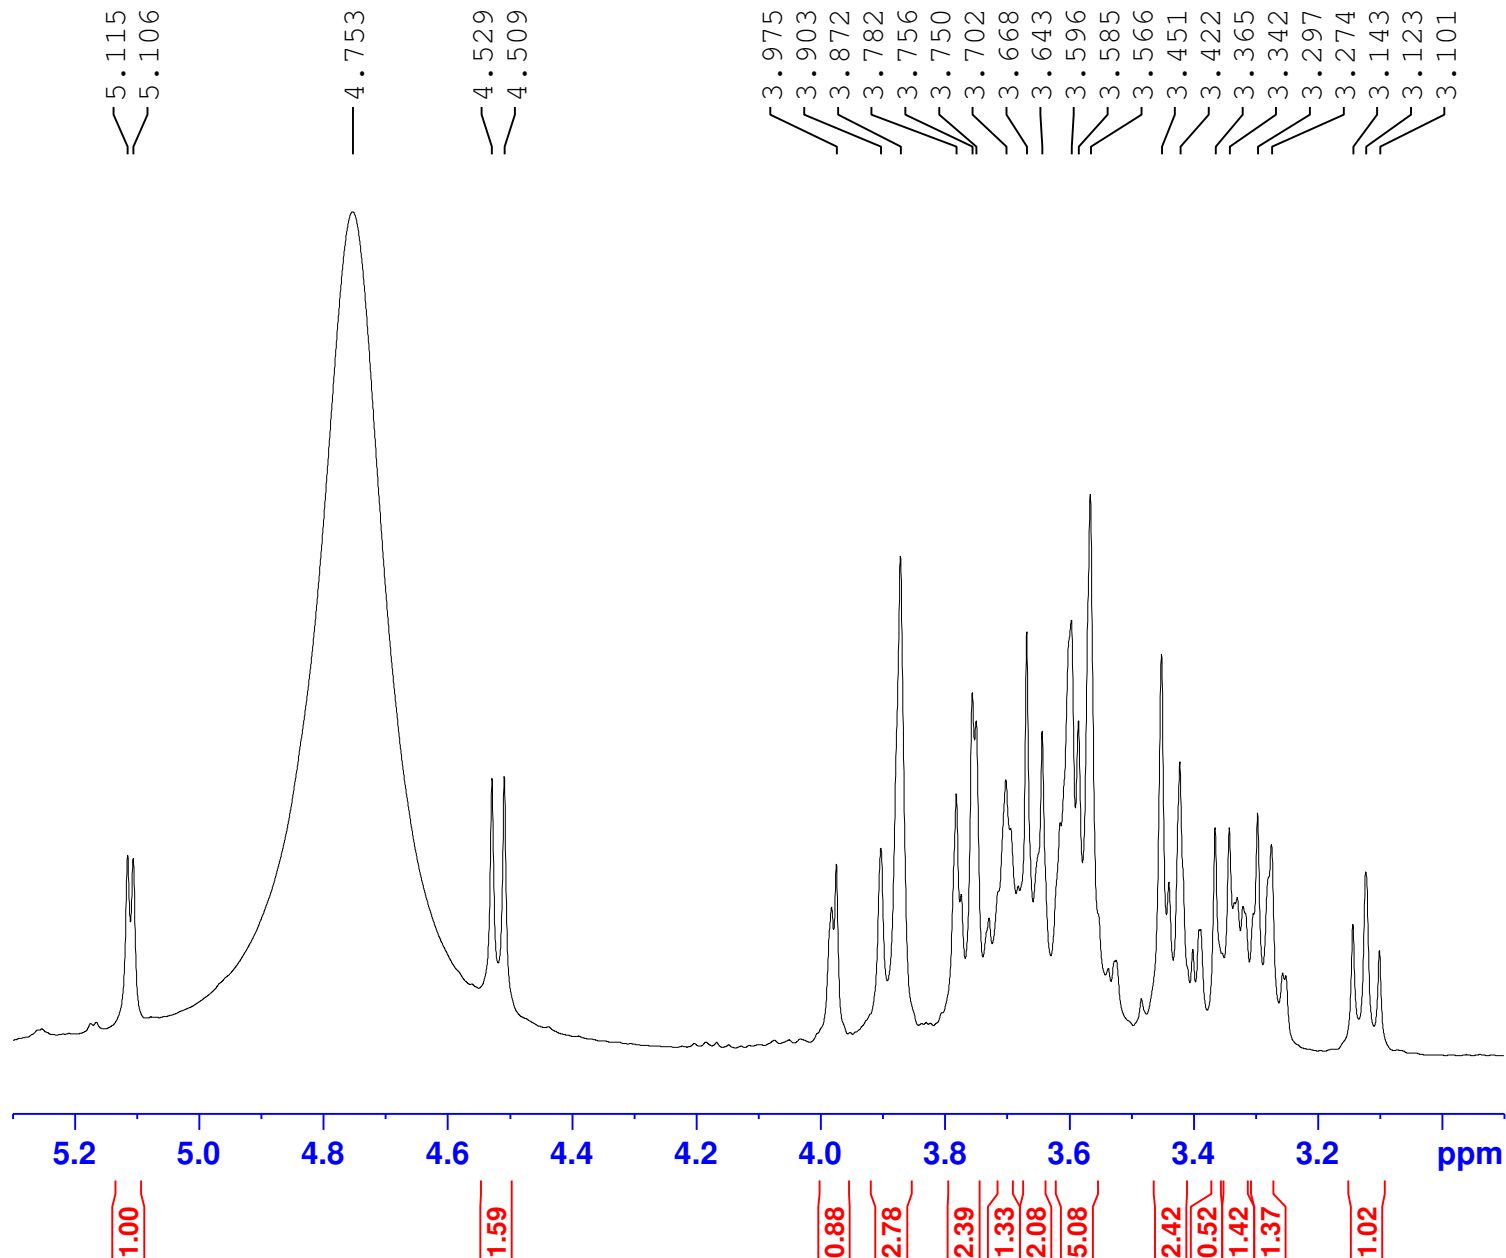

Current Data Parameters
NAME KEY-1
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20230719
Time 8.48 h
INSTRUM Avance Neo 400
PROBHD Z108618_1053 (
PULPROG zg30
TD 65536
SOLVENT D2O
NS 16
DS 2
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976959 sec
RG 12.5744
DW 61.000 usec
DE 12.86 usec
TE 298.1 K
D1 1.00000000 sec
TD0 1
SFO1 400.3024719 MHz
NUC1 1H
P0 4.67 usec
P1 14.00 usec
PLW1 15.77799988 W

F2 - Processing parameters
SI 65536
SF 400.3000000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00