



NATIONAL TYPE EVALUATION PROGRAM

Certificate of Conformance

for Weighing and Measuring Devices

For:

Weighing/Load Receiving Element
Bench/Counter/Platform
Model: TPB-4050 Series
 n_{max} : 5000
 e_{min} : 0.01 lb (See Below)
Capacity: 50 to 1250 lb (See Below)
Platform: 320 x 360 mm to 800 x 800 mm
Accuracy Class: III

Submitted By:

VisionTechShop.com
100 Temple Avenue
Hackensack, NJ 07601
Tel: 201-679-7793
Contact: Jong IL Kim
Email: kijpys@hotmail.com
Web site: www.visiontechshop.com

Standard Features and Options

Platform Size	Capacity (lb)	e_{min}	n_{max}
320 x 360 mm	50 /100/200	0.01/0.02/0.05 lb	5000
350 x 450mm	50 /100/200	0.01/0.02/0.05 lb	5000
400 x 400 mm	50 /100/200	0.01/0.02/0.05 lb	5000
400 x 500 mm	100/200/500	0.02/0.05/0.1 lb	5000
420 x 520 mm	100/200/500	0.02/0.05/0.1 lb	5000
600 x 600 mm	100/200/500/1000/1250	0.02/0.05/0.1/0.2/0.5 lb	5000
600 x 800 mm	500/1000/1250	0.1/0.2/0.5 lb	5000
800 x 800 mm	500/1000/1250	0.1/0.2/0.5 lb	5000

Platform Material:

- Mild Steel, Stainless Steel, Aluminum

Load Cell Used:


Models BT T2A non-NTEP, BT T4A non-NTEP, and BT T6B non-NTEP

Temperature Range: -10 °C to 40 °C (14 °F to 104 °F)

This device was evaluated under the National Type Evaluation Program and was found to comply with the applicable technical requirements of "NIST Handbook 44: Specifications, Tolerances and Other Technical Requirements for Weighing and Measuring Devices." Evaluation results and device characteristics necessary for inspection and use in commerce are on the following pages.



Craig VanBuren
Chairman, NCWM, Inc.

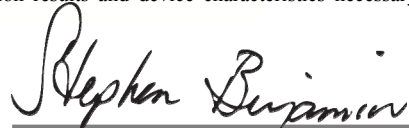

Stephen Benjamin
Committee Chair, NTEP Committee
Issued: December 9, 2019

1135 M Street, Suite 110 / Lincoln, Nebraska 68508

The National Conference on Weights and Measures (NCWM) does not approve, recommend or endorse any proprietary product or material, either as a single item or as a class or group. Results shall not be used in advertising or sales promotion to indicate explicit or implicit endorsement of the product or material by the NCWM.



VisionTechShop.com

Weighing/Load receiving Element / TPB-4050 Series

Application: For general purpose weighing applications when interfaced with a certified and compatible indicating element.

Identification: The G.S.1 information can be found on a self-destructive label on the load receiving element under the platform.

Sealing: This device has no physical means that require sealing. Calibrations are performed through the indicator. Seal the indicator as required in its NTEP Certificate of Conformance.

Test Conditions: This certificate is issued based upon the following tests and upon information provided by the manufacturer. The emphasis of this evaluation was on device design, performance, and compliance with influence factor requirements. Three TPB-4050s were submitted to the laboratory, 400 x 400 mm (50 x 0.01 lb) 600 x 600 mm (500 x 0.01 lb) 800 x 800 mm (1000 x 0.02 lb), Several increasing/decreasing and shift tests were performed. The devices were tested over a temperature range of -10°C to 40°C (14°F to 104°F). A load of approximately one-half capacity was applied over 100 000 times. The scales were tested periodically during this time.

Evaluated By: E. A. Payne, Jr (MD)

Type Evaluation Criteria Used: *NIST Handbook 44 Specifications, Tolerances, and Other Technical Requirements for Weighing and Measuring Devices*, 2012 Edition. *NCWM Publication 14 Measuring Devices*, 2012 Edition.

Conclusion: The results of the evaluation and information provided by the manufacturer indicate the device complies with applicable requirements.

Information Reviewed By: D. Flocken (NCWM)

Example(s) of Device:

