


## Reference Material Product Information Sheet

Epichem's Quality System conforms to ISO9001:2015 as certified by ECAAS Pty Ltd - Certification number 616061.

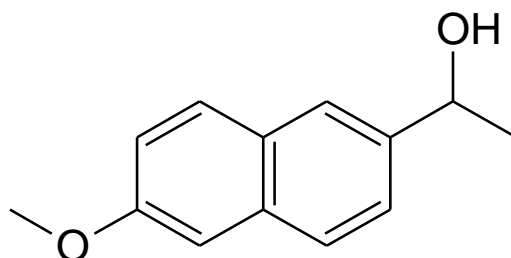

<b>Name</b>	(1 <i>RS</i> )-1-(6-methoxynaphthalen-2-yl)ethanol
<b>BP Name</b>	Naproxen Impurity K
<b>Synonym(s)</b>	1-(6-methoxy-2-naphthalenyl)ethanol; 6-methoxy- $\alpha$ -methyl-2-naphthalenemethanol; (+/-)-1-(6-methoxynaphthyl)ethanol; 1-(6 $\alpha$ -methoxy-2-naphthyl)ethanol; 2-(1-hydroxyethyl)-6-methoxynaphthalene; $\alpha$ -(6-methoxy-2-naphthyl)ethanol
<b>Epichem Item #</b>	EPL-AA180 Batch 1
<b>CAS #</b>	77301-42-9
<b>Molecular Formula</b>	C <sub>13</sub> H <sub>14</sub> O <sub>2</sub>
<b>Molecular Weight</b>	202.26 g/mol
<b>Appearance</b>	White powder
<b>Melting Point</b>	111.8-114.3°C
<b>Combustion Analysis</b>	Required (%): C:77.2; H:7.0; N:0.0. Found (%): C:77.3; H:7.1; N:0.0.
<b>Purity*</b>	99.4%
<b>Date of Manufacture</b>	9 October 2015
<b>Storage Requirements</b>	Protect from heat, light and moisture.
<b>Special Precautions</b>	<b>This compound is for laboratory use only. Its toxicological properties may not have been fully established. It should be handled only by suitably qualified personnel.</b>
<b>Intended Use</b>	This compound is suitable for the identification of impurities and degradants in pharmaceutical materials. The purity assay is considered as relative contribution.
<b>Date of Shipment</b>	TBA This certificate is valid for one year from the date of shipment provided the substance is unopened and stored under the recommended conditions.
<b>Retest Date</b>	TBA (Proper Storage and Handling Required)

\* NATA accreditation does not cover the performance of this service

EPL-AA180 Batch 1

Revision 2

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia

Tel + 61 (0)8 6167 5200

Fax + 61 (0)8 6167 5201

www.epichem.com.au

ABN 80 106 769 902

## I. Identity


The identity of this product was established using the following analyses:

### Ia. <sup>1</sup>H NMR Spectrum

Conditions: 400 MHz, CDCl<sub>3</sub>

<sup>1</sup>H NMR spectrum consistent with chemical structure.

SpinWorks 3: LBC219-065@11H

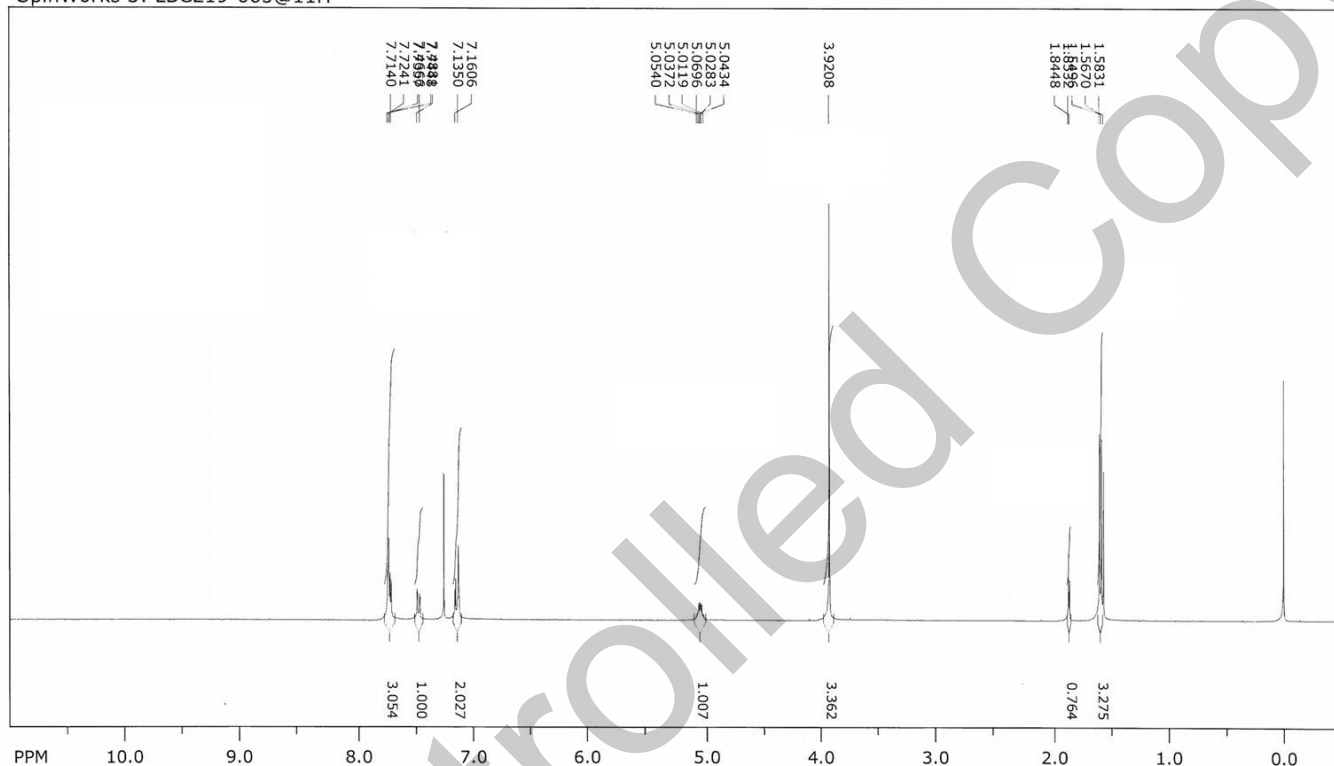

file: ... K\NMR data\LBC219-065@11H.fid\fid block# 1 expt: "s2pul"  
transmitter freq.: 400.175825 MHz  
time domain size: 26232 points  
width: 6402.56 Hz = 15.9994 ppm = 0.244074 Hz/pt  
number of scans: 64

freq. of 0 ppm: 400.173413 MHz  
processed size: 65536 complex points  
LB: 0.000 GF: 0.0000  
Hz/cm: 164.357 ppm/cm: 0.41071

EPL-AA180 Batch 1

Revision 2


Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

## Ib. Mass Spectrum

The mass spectrum of this material was analysed by Liquid Chromatography Mass Spectroscopy (LCMS) using in-house EM005.WI08.

Method: 5% to 100% ACN in water gradient (+0.1% formic acid)  
Poroshell 120 EC-C18, 4.6 x 50 mm, 2.7 micron

Retention Time (MS)	MS Area	Mol. Weight or Ion
2.995	2622293	225.10 I
		186.15 I
		185.15 I

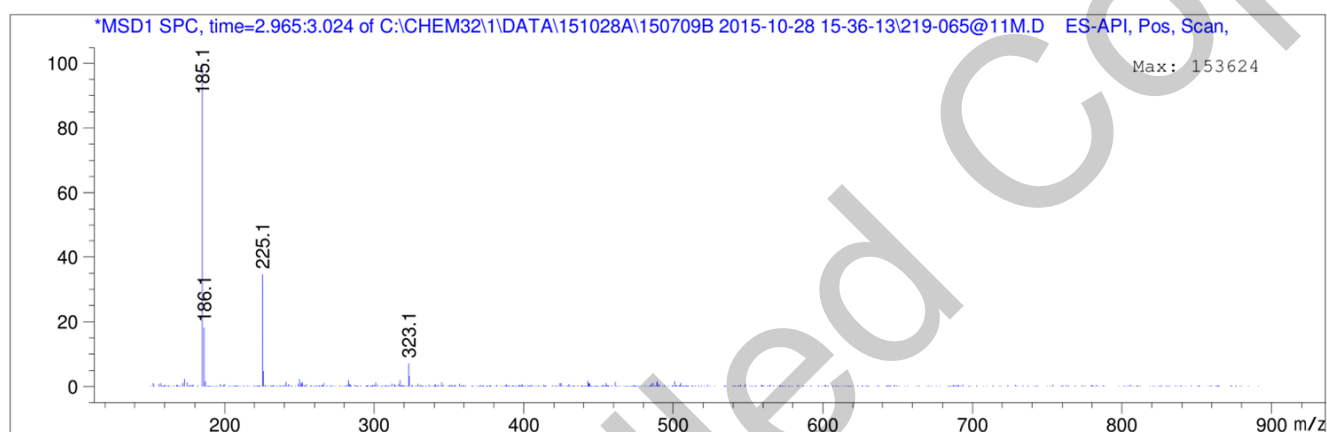


Theoretical value: 225.1 [M+Na]<sup>+</sup>.

The signal of the Mass Spectrum is consistent with the theoretical value and its interpretation is consistent with the structural formula.

### Ic. IR Spectrum

The infra-red spectrum of this material was analysed by Fourier-Transform Infrared Spectroscopy (FTIR) using in-house EM005.WI09.

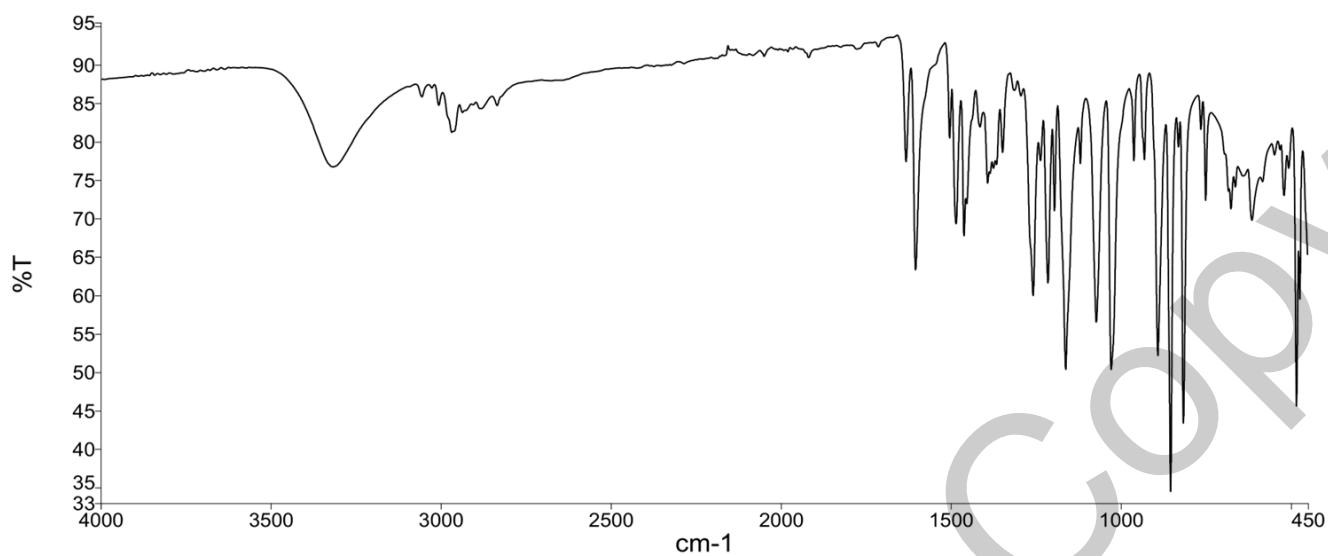

The interpretation of the signals of the Fourier-Transform Infrared Spectrum is consistent with the structural formula.

EPL-AA180 Batch 1

Revision 2


Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

## II. Purity

The purity of this material was analysed by high performance liquid chromatography (HPLC) using in-house EM005.WI07.

### HPLC Conditions:

Column	Conditions				Detector	Injector
Agilent Poroshell 120 EC-C18 4.6 x 50mm 2.7 micron	25°C				DAD 229nm	Auto 1.0 µL  0.18 mg/mL in 100% acetonitrile (NO MODIFIERS)
	Time (min)	% Line A (Water + 0.1% (v/v) TFA)	% Line B (Acetonitrile + 0.1% (v/v) TFA)	Flow rate (mL/min)		
	0.00	80	20	1.0		
	7.00	45	55	1.0		
	11.00	5	95	1.0		
	16.00	5	95	1.0		
	17.00	80	20	1.0		
	20.00	80	20	1.0		

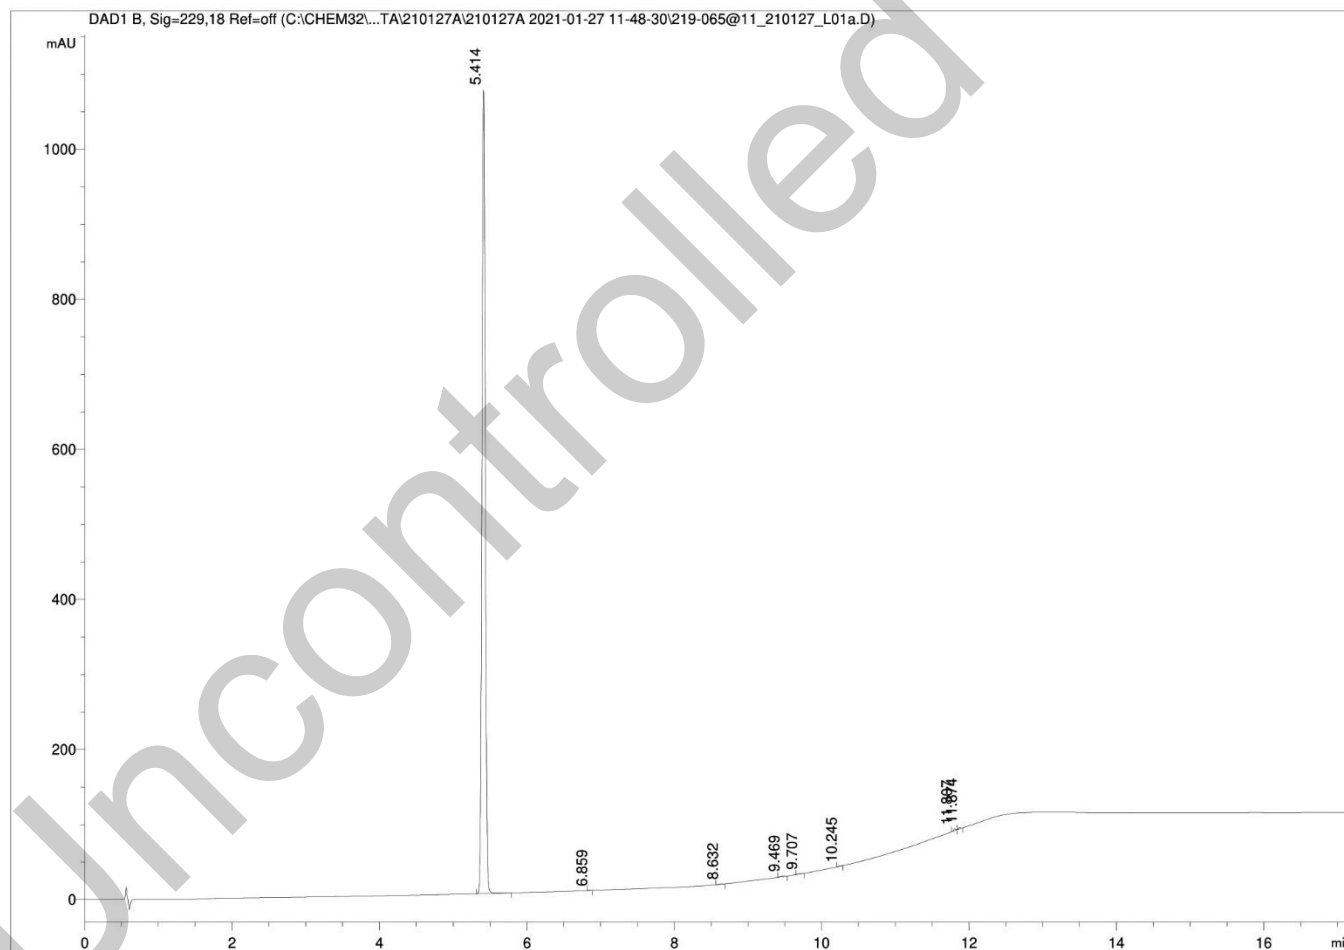

EPL-AA180 Batch 1

Revision 2

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

### Area Percent Report – Sorted by Signal

Peak Number	Retention Time (rounded)	Area	Area % (rounded)
1	5.41	3340.78	99.48
2	6.86	0.14	0.00
3	8.63	2.47	0.07
4	9.47	3.60	0.11
5	9.71	1.30	0.04
6	10.25	0.38	0.01
7	11.81	5.02	0.15
8	11.87	4.65	0.14
Totals			100 (rounded)

For the calculation the system peaks were ignored. The content of the analyte was determined as a ratio of the peak area of the analyte and the cumulative areas of the purities, added up to 100%.

#### Results:

Average 99.5% (average of 10 duplicate analyses)

### III. Water Content

Method: Karl-Fischer titration using in-house EM005.WI04.

**Results:**

Average 0.1%

### IV. Ash Content

Method: BP2018 Ash (Appendix XI J) Method II

**Result:**

Contains <0.1% ash.

### V. Residual Solvents

Method: <sup>1</sup>HNMR

**Result:**

No significant impurities detected by <sup>1</sup>H NMR analysis.

### VI. Final Result

Chromatographic purity (HPLC)	99.5%
Water content	0.1%
Ash content	<0.1%
Residual solvents	<0.1%
Purity*	99.4%

This purity is assessed to be 99.4%.

Product Reviewed By:

Product Released By:

James Rixson, PhD  
Head of Production

Carol Worth, PhD  
Quality Manager

Release Date: 28 June 2022

*\*NATA accreditation does not cover the performance of this service.*

The calculation of the purity follows the formula:

$$\text{Purity(\%)} = \frac{((\text{Chromatographicpurity[HPLC]}) \times (100 - (\text{watercontent} + \text{ashcontent} + \text{volatilecontents})))}{100}$$

EPL-AA180 Batch 1

Revision 2

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902