



Accredited for compliance with ISO 17034  
This document shall not be reproduced except in full.  
Accreditation Number: 20126  
Corporate Site Number: 24143


The results of the tests, calibrations and/or measurements included in this document are traceable to Australia/national standards.  
NATA is a signatory to the APLAC Mutual Recognition Arrangement for the mutual recognition of the equivalence of reference materials certificates.



Our Formula. Your Success.

## Reference Material Product Information Sheet

Epichem's Quality System conforms to ISO9001:2015 as certified by ECAAS Pty Ltd - Certification number 616061.

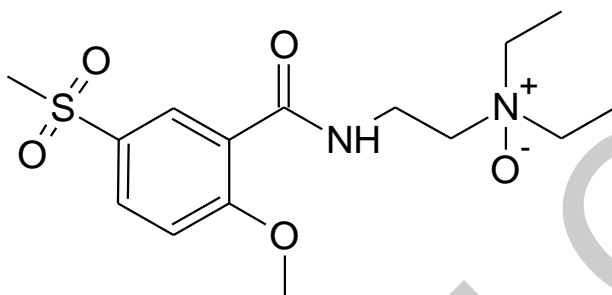

<b>Name</b>	<i>N</i> -(2-(diethylnitro)ethyl)-2-methoxy-5-(methylsulfonyl)benzamide
<b>Synonym(s)</b>	Tiapride <i>N</i> -oxide; <i>N,N</i> -diethyl-2-((2-methoxy-5-methylsulfonylbenzoyl)amino)ethanamine oxide
<b>Epichem Item #</b>	EPL-AA205 Batch 1
<b>CAS #</b>	63484-11-7
<b>Molecular Formula</b>	C <sub>15</sub> H <sub>24</sub> N <sub>2</sub> O <sub>5</sub> S
<b>Molecular Weight</b>	344.43 g/mol
<b>Appearance</b>	White powder
<b>Melting Point</b>	137.4-139.5°C
<b>Combustion Analysis</b>	Required (%): C:52.3; H:7.0; N:8.1. Found (%): C:51.6; H:7.1; N:8.0.
<b>Purity*</b>	97.1%
<b>Date of Manufacture</b>	13 September 2016
<b>Storage Requirements</b>	Hygroscopic. Deliquescent. Store in tightly closed vessel. Protect from heat, light and moisture.
<b>Special Precautions</b>	<b>This compound is for laboratory use only. Its toxicological properties may not have been fully established. It should be handled only by suitably qualified personnel.</b>
<b>Intended Use</b>	This compound is suitable for the identification of impurities and degradants in pharmaceutical materials. The purity assay is considered as relative contribution.
<b>Date of Shipment</b>	TBA This certificate is valid for one year from the date of shipment provided the substance is unopened and stored under the recommended conditions.
<b>Retest Date</b>	TBA (Proper Storage and Handling Required)

\* NATA accreditation does not cover the performance of this service

EPL-AA205 Batch 1

Revision 1

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902


## I. Identity

The identity of this product was established using the following analyses:

### Ia. <sup>1</sup>HNMR Spectrum

Conditions: 400 MHz, DMSO-d<sub>6</sub>

<sup>1</sup>HNMR spectrum consistent with chemical structure.

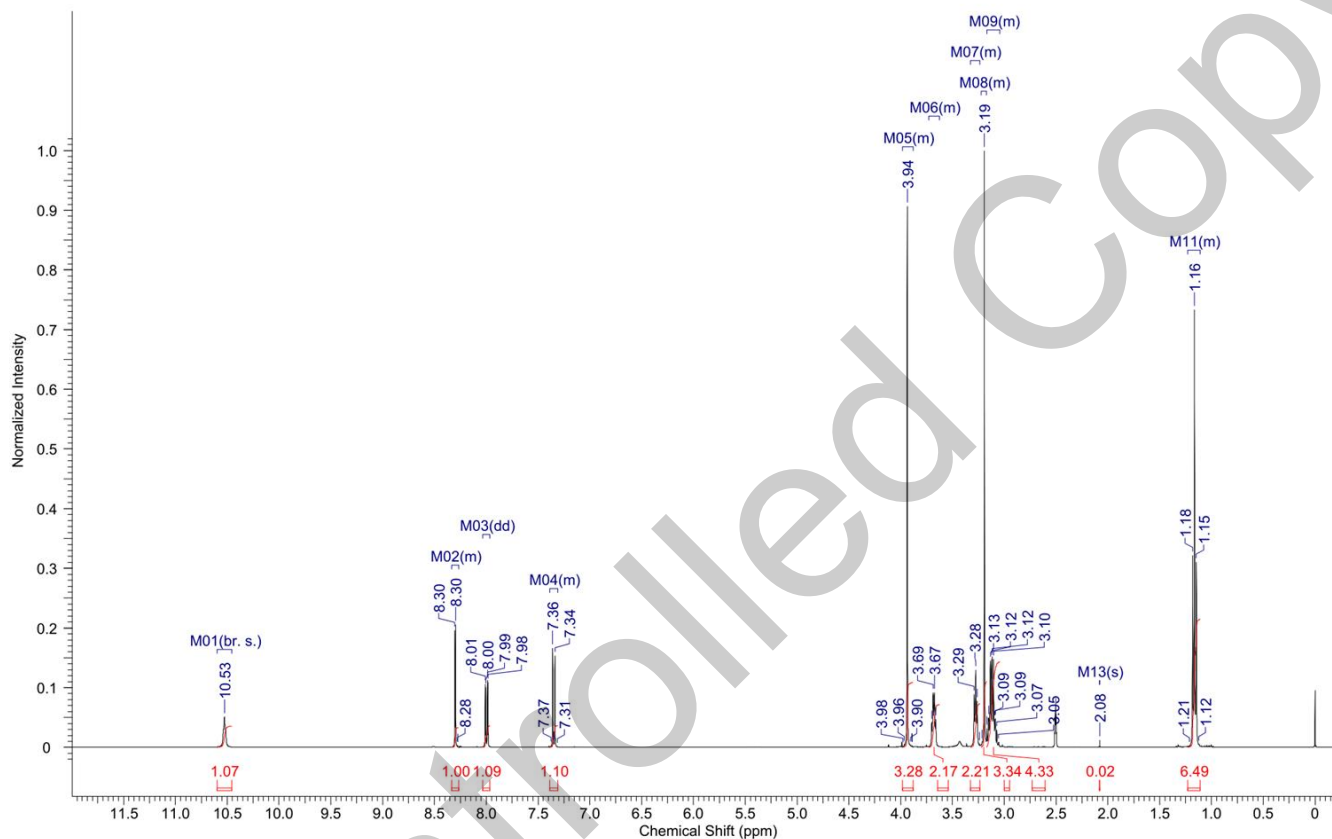

EPL-AA205 Batch 1

Revision 1

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia

Tel + 61 (0)8 6167 5200

Fax + 61 (0)8 6167 5201


www.epichem.com.au

ABN 80 106 769 902

## Ib. Mass Spectrum

The mass spectrum of this material was analysed by Liquid Chromatography Mass Spectroscopy (LCMS) using in-house EM005.WI08.

Method: 5% to 100% ACN in water gradient (+0.1% formic acid)  
Poroshell 120 EC-C18, 4.6 x 50 mm, 2.7 micron

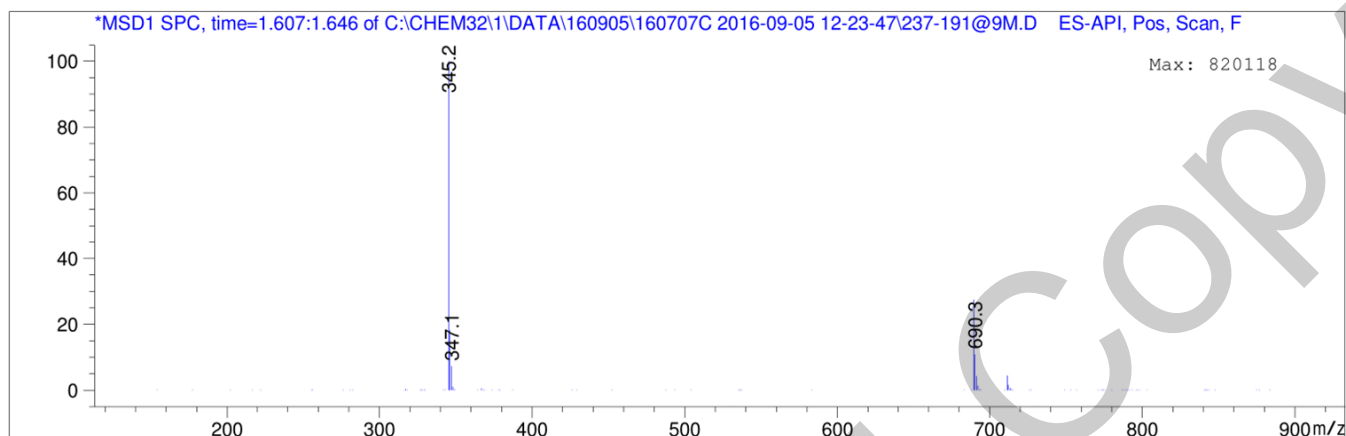

Theoretical value: 345.2 [M+H]<sup>+</sup>.

The signal of the Mass Spectrum is consistent with the theoretical value and its interpretation is consistent with the structural formula.


EPL-AA205 Batch 1

Revision 1

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

### Ic. IR Spectrum

The infra-red spectrum of this material was analysed by Fourier-Transform Infrared Spectroscopy (FTIR) using in-house EM005.WI09.

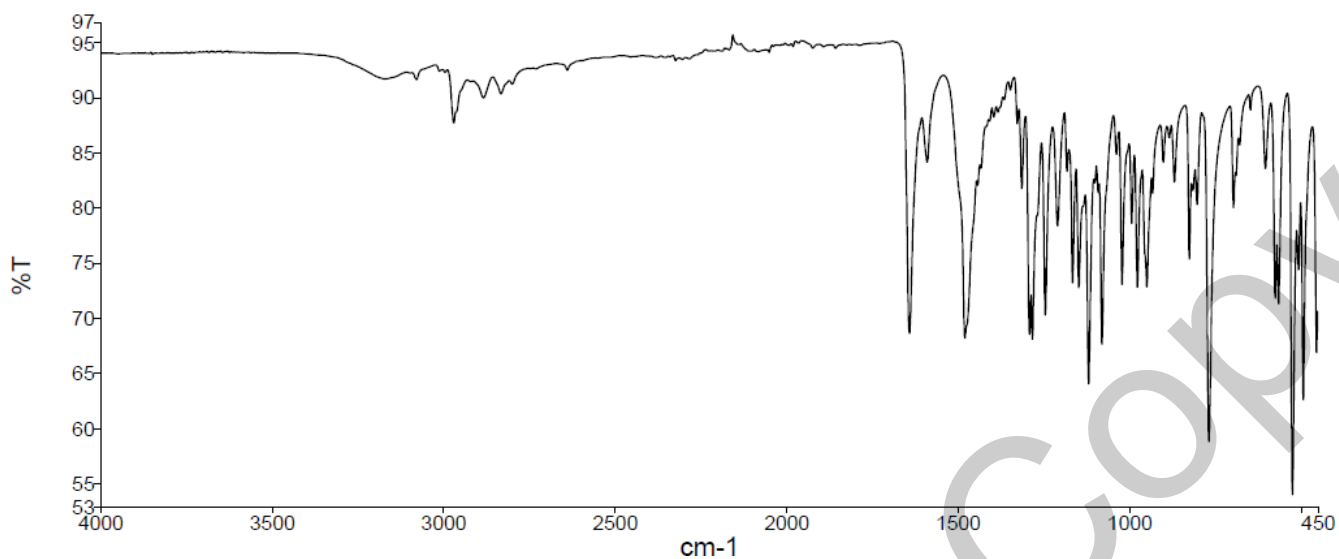


The interpretation of the signals of the Fourier-Transform Infrared Spectrum is consistent with the structural formula.

## II. Purity

The purity of this material was analysed by high performance liquid chromatography (HPLC) using in-house EM005.WI07.

### HPLC Conditions:

Column	Conditions				Detector	Injector
Agilent Poroshell 120 EC-C18  4.6 x 50mm  2.7 micron	25°C				DAD 220nm	Auto 1.0 µL 0.35 mg/mL 100% acetonitrile
	Time (min)	% Line A (Water + 0.1% (v/v) TFA)	% Line B (Acetonitrile + 0.1% (v/v) TFA)	Flow rate (mL/min)		
	0.00	94	6	1.0		
	6.00	76	24	1.0		
	13.10	5	95	1.0		
	18.10	5	95	1.0		
	19.10	94	6	1.0		
	24.10	94	6	1.0		

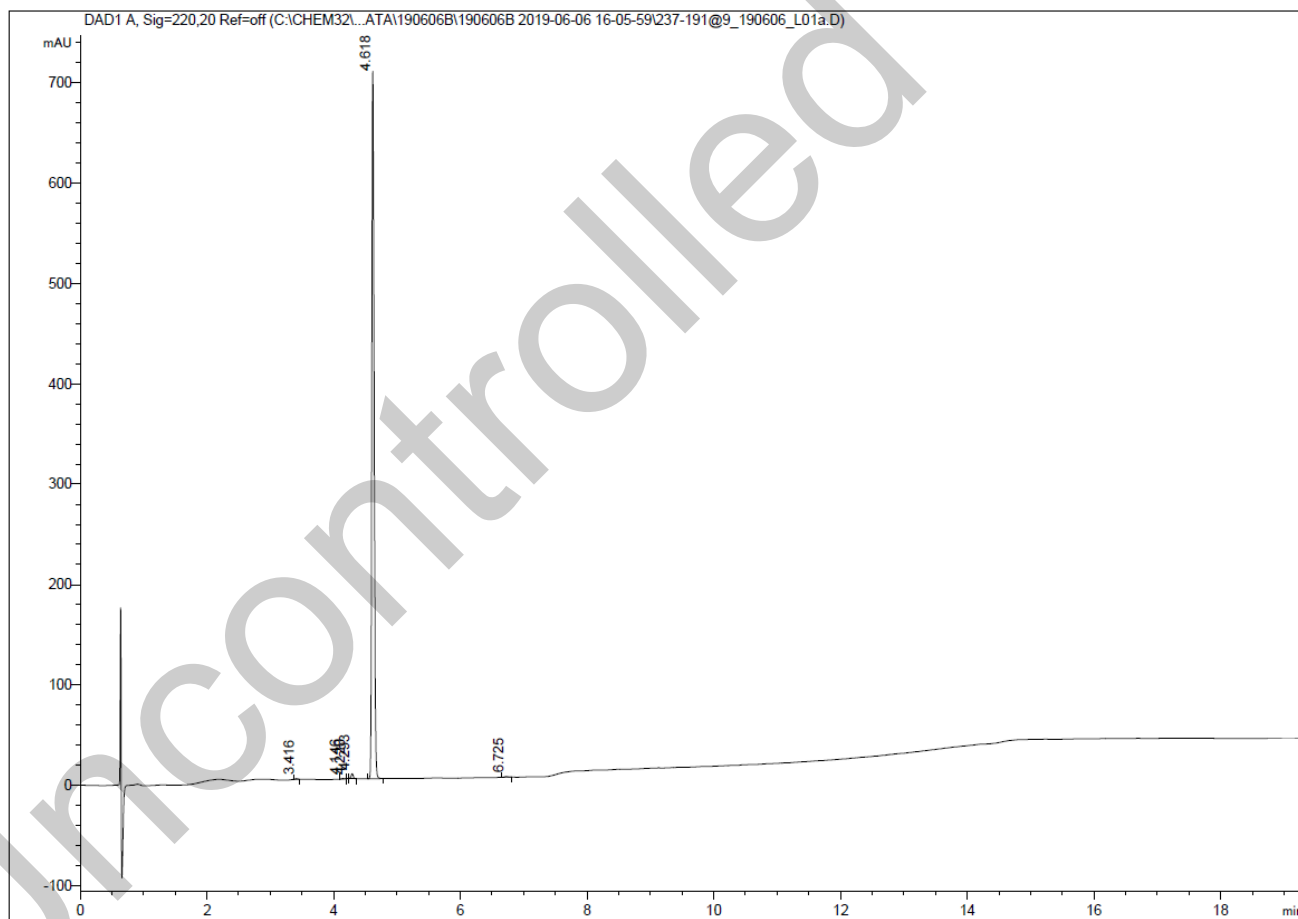

EPL-AA205 Batch 1

Revision 1

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

### Area Percent Report – Sorted by Signal

Peak Number	Retention Time (rounded)	Area	Area % (rounded)
1	3.42	1.88	0.1
2	4.15	0.83	0.05
3	4.22	0.2	0.01
4	4.29	12.01	0.67
5	4.62	1776.47	99.05
6	6.72	2.17	0.12
Totals			100 (rounded)

For the calculation the system peaks were ignored. The content of the analyte was determined as a ratio of the peak area of the analyte and the cumulative areas of the purities, added up to 100%.

#### Results:

Average                    99.0% (average of 10 duplicate analyses)

### III. Water Content

Method: Karl-Fischer titration using in-house EM005.WI04.

**Results:**

Average 1.4%

### IV. Ash Content

Method: BP2016 Ash (Appendix XI J) as per WS001/C29331

**Result:**

Contains 0.5% ash.

### V. Residual Solvents

Method: <sup>1</sup>HNMR

**Result:**

No significant impurities detected by <sup>1</sup>H NMR analysis.

### VI. Final Result

Chromatographic purity (HPLC)	99.0%
Water content	1.4%
Ash content	0.5%
Residual solvents	<0.1%
Purity*	97.1%

This purity is assessed to be 97.1%.

Product Reviewed By:

Product Released By:

John Moursounidis, PhD  
Head Reference Standards

Boon Tan  
Quality Manager

Release Date: 13 June 2019

\*NATA accreditation does not cover the performance of this service.

The calculation of the purity follows the formula:

$$\text{Purity(\%)} = \frac{((\text{Chromatographicpurity[HPLC]}) \times (100 - (\text{watercontent} + \text{ashcontent} + \text{volatilecontents})))}{100}$$

EPL-AA205 Batch 1

Revision 1

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902