


## Reference Material Product Information Sheet

Epichem's Quality System conforms to ISO9001:2015 as certified by ECAAS Pty Ltd - Certification number 616061.



<b>Name</b>	(RS)-2-chloro-1-(3-hydroxyphenyl)ethanol
<b>Synonym(s)</b>	(RS)-3-(2-chloro-1-hydroxyethyl)phenol; α-(chloromethyl)-3-hydroxy-benzenemethanol
<b>Epichem Item #</b>	EPL-AA223 Batch 2
<b>CAS #</b>	1378757-22-2
<b>Molecular Formula</b>	C <sub>8</sub> H <sub>9</sub> ClO <sub>2</sub>
<b>Molecular Weight</b>	172.61 g/mol
<b>Appearance</b>	White solid
<b>Melting Point</b>	107.5-110.1°C
<b>Combustion Analysis</b>	Required (%): C:55.7; H:5.3. Found (%): C:55.2; H:5.2.
<b>Purity*</b>	99.4%
<b>Date of Manufacture</b>	25 July 2018
<b>Storage Requirements</b>	Protect from heat, light and moisture.
<b>Special Precautions</b>	<b>This compound is for laboratory use only. Its toxicological properties may not have been fully established. It should be handled only by suitably qualified personnel.</b>
<b>Intended Use</b>	This compound is suitable for the identification of impurities and degradants in pharmaceutical materials. The purity assay is considered as relative contribution.
<b>Date of Shipment</b>	TBA This certificate is valid for one year from the date of shipment provided the substance is stored under the recommended conditions.
<b>Retest Date</b>	TBA (Proper Storage and Handling Required)

\* NATA accreditation does not cover the performance of this service

EPL-AA223 Batch 2

Revision 3

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

## I. Identity


The identity of this product was established using the following analyses:

### Ia. <sup>1</sup>H NMR Spectrum

Conditions: 400 MHz, DMSO-d<sub>6</sub>  
<sup>1</sup>H NMR spectrum consistent with chemical structure.

Acquisition Time (sec)	3.7547	Comment	LBC320-189@6Ha 1H DMSO {E:\data\external\epichem} cygoh 6				
Date	23 Jul 2018 17:50:56	Date Stamp	23 Jul 2018 17:50:56				
File Name	\naphthalene\company\NMR files\LBC320-189@6Ha\1\data\111r		Frequency (MHz)	400.13			
Nucleus	1H	Number of Transients	8	Origin	spect	Original Points Count	24038
Owner	nmr	Points Count	32768	Pulse Sequence	zg	Receiver Gain	203.00
SW(cyclical) (Hz)	6402.05	Solvent	DMSO-d6	Spectrum Offset (Hz)	2797.3647	Spectrum Type	STANDARD
Sweep Width (Hz)	6401.85	Temperature (degree C)	26.945				

LBC320-189@6Ha.001.001.1r.esp

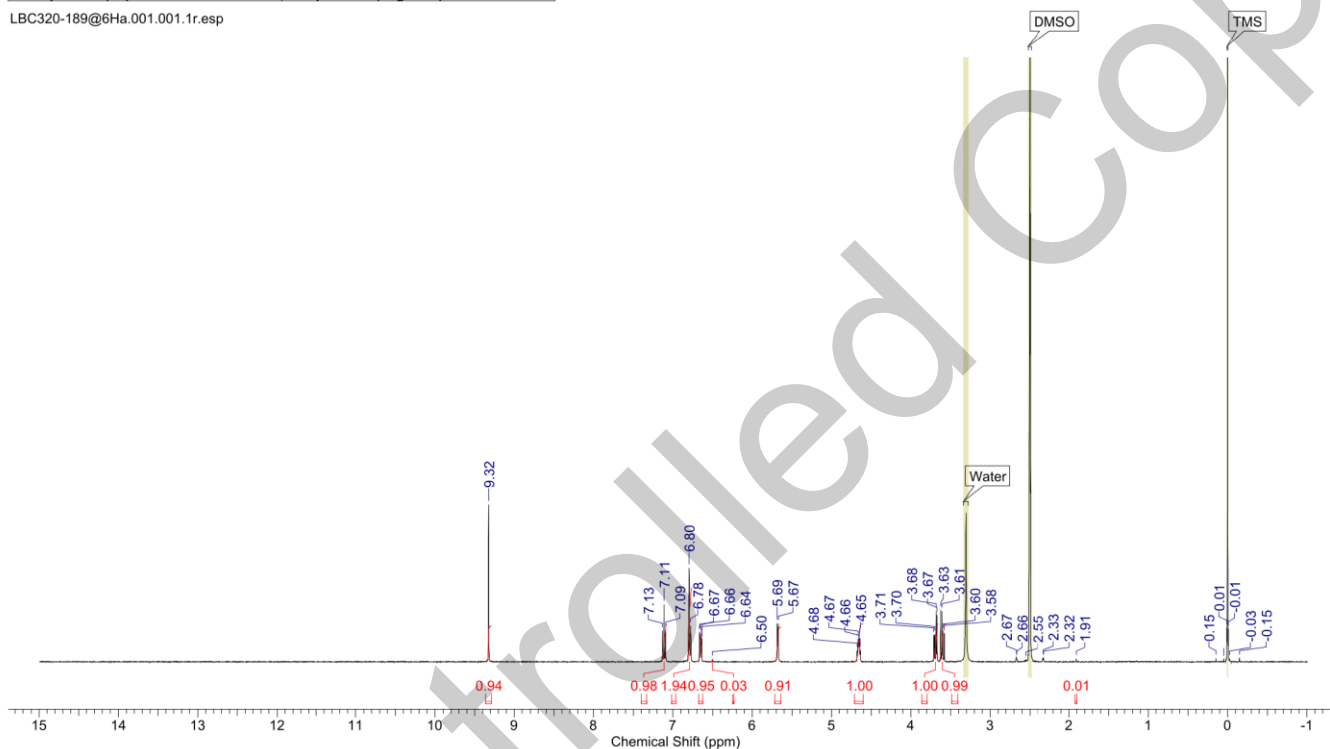

EPL-AA223 Batch 2


Revision 3

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

## Ib. Mass Spectrum

The mass spectrum of this material was analysed by Liquid Chromatography Mass Spectroscopy (LCMS) using in-house EM005.WI08.

Method: ACN/water gradient (+ 0.1% formic acid).  
Poroshell 120 EC-C8, 3 x 50 mm, 2.7 micron.

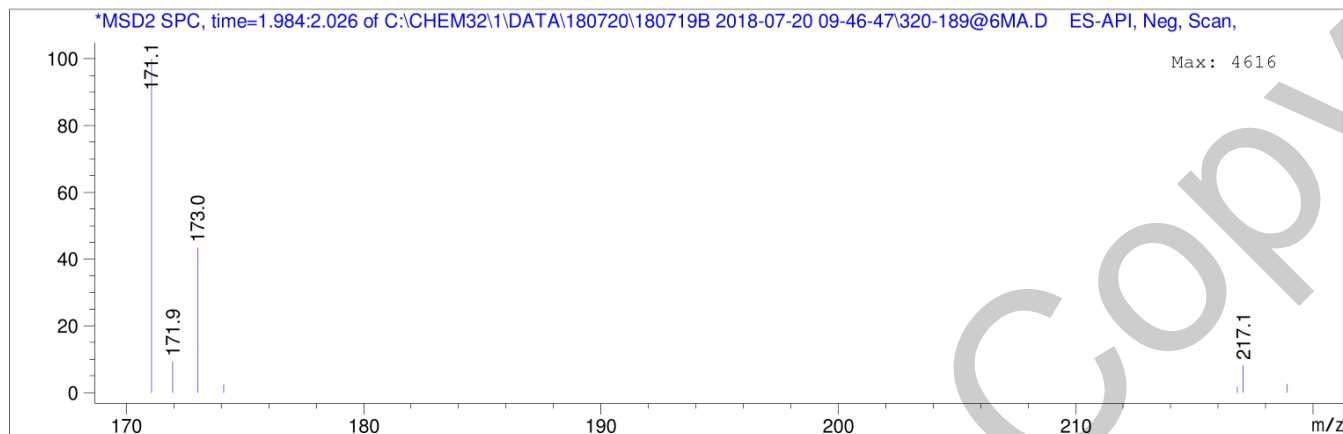

Theoretical value: 171.1 [M-H]<sup>-</sup>.

The signal of the Mass Spectrum is consistent with the theoretical value and its interpretation is consistent with the structural formula.


EPL-AA223 Batch 2

Revision 3

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

### Ic. IR Spectrum

The infra-red spectrum of this material was analysed by Fourier-Transform Infrared Spectroscopy (FTIR) using in-house EM005.WI09.

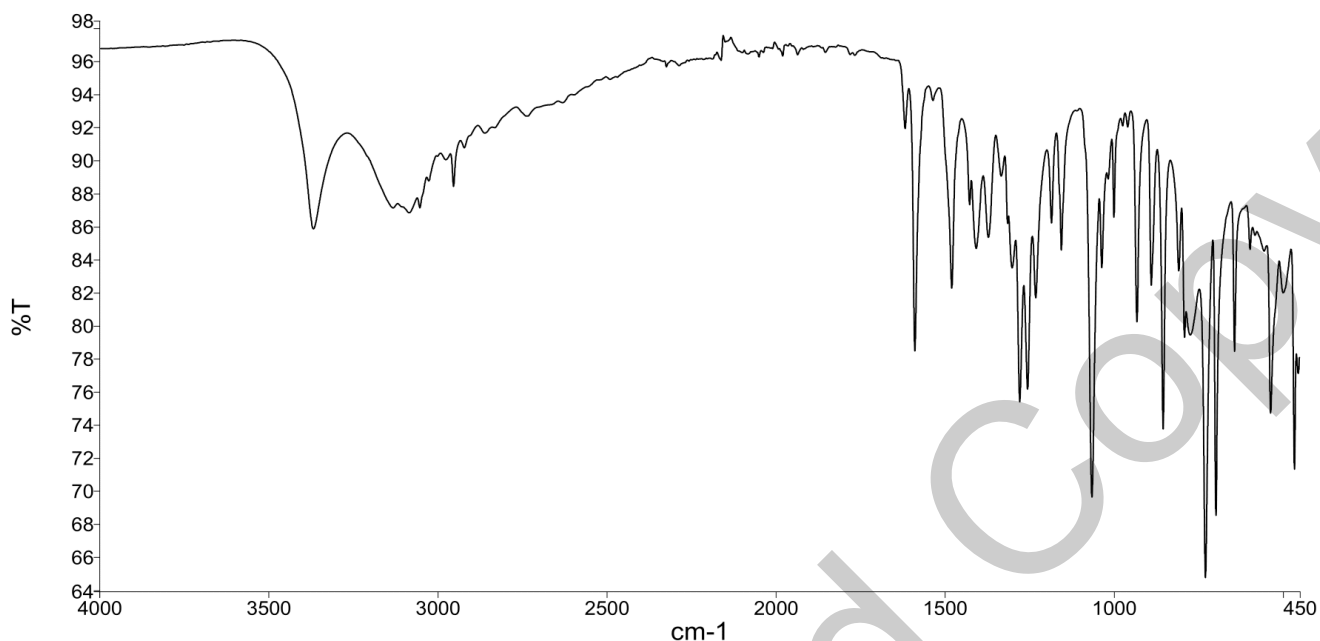

The interpretation of the signals of the Fourier-Transform Infrared Spectrum is consistent with the structural formula.

EPL-AA223 Batch 2

Revision 3


Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

## II. Purity

The purity of this material was analysed by high performance liquid chromatography (HPLC) using in-house EM005.WI07.

### HPLC Conditions:

Column	Conditions				Detector	Injector
Agilent Poroshell 120 EC-C18  4.6 x 50mm  2.7 micron	25°C				DAD  274nm	Auto  1.0 µL  1.0 mg/mL in 100% acetonitrile (NO MODIFIERS)
	Time (min)	% Line A (Water + 0.1% (v/v) TFA)	% Line B (Acetonitrile + 0.1% (v/v) TFA)	Flow rate (mL/min)		
	0.00	95	5	1.0		
	6.00	77	23	1.0		
	13.20	5	95	1.0		
	18.20	5	95	1.0		
	19.20	95	5	1.0		
	22.20	95	5	1.0		

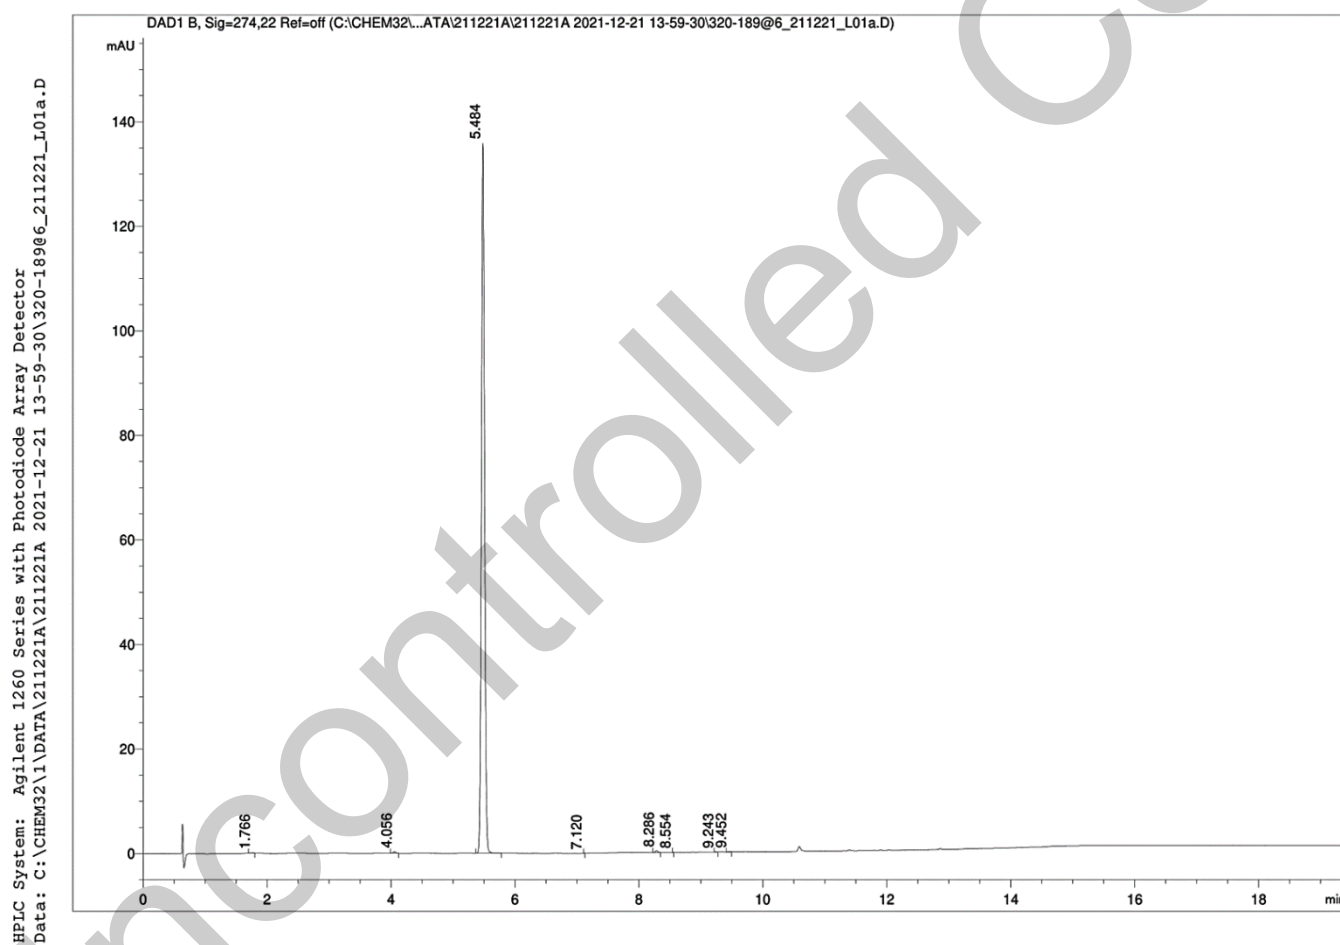

EPL-AA223 Batch 2

Revision 3

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

### Area Percent Report – Sorted by Signal

Peak Number	Retention Time (rounded)	Area	Area % (rounded)
1	1.77	0.12	0.03
2	4.06	0.85	0.18
3	5.48	478.97	99.57
4	7.12	0.01	0.00
5	8.29	0.84	0.17
6	8.55	0.02	0.00
7	9.24	0.08	0.02
8	9.45	0.14	0.03
Totals			100 (rounded)

For the calculation the system peaks were ignored. The content of the analyte was determined as a ratio of the peak area of the analyte and the cumulative areas of the purities, added up to 100%.

#### Results:

Average 99.6% (average of 10 duplicate runs)

EPL-AA223 Batch 2

Revision 3

Epicchem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epicchem.com.au ABN 80 106 769 902

### III. Water Content

Method: Karl-Fischer titration using in-house EM005.WI04.

**Results:**

Average 0.2%

### IV. Ash Content

Method: BP2018 Ash (Appendix XI J) Method II

**Result:**

Contains <0.1% ash.

### V. Residual Solvents

Method: <sup>1</sup>H NMR

**Result:**

No significant impurities detected by <sup>1</sup>H NMR analysis.

### VI. Final Result

Chromatographic purity (HPLC)	99.6%
Water content	0.2%
Ash content	<0.1%
Residual solvents	<0.1%
Purity*	99.4%

This purity is assessed to be 99.4%.

Product Reviewed By:

Product Released By:

James Rixson, PhD  
Head of Production

Carol Worth, PhD  
Quality Manager  
Release Date: 23 December 2021

\*NATA accreditation does not cover the performance of this service.

The calculation of the purity follows the formula:

$$\text{Purity(\%)} = \frac{((\text{Chromatographicpurity[HPLC]}) \times (100 - (\text{watercontent} + \text{ashcontent} + \text{volatilecontents})))}{100}$$

EPL-AA223 Batch 2

Revision 3

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902