

Accredited for compliance with ISO 17034 This document shall not be reproduced except in full. Accreditation Number: 20126

Corporate Site Number: 24143

The results of the tests, calibrations and/or measurements included in this document are traceable to Australia/national standards NATA is a signatory to the APLAC Mutual Recognition Arrangement for the mutual recognition of the equivalence of reference materials certificates



Our Formula. Your Success.

# **Reference Material Product Information Sheet**

Epichem's Quality System conforms to ISO9001:2015 as certified by ECAAS Pty Ltd - Certification number 616061.

Name	2-(diethylamino)-N-(2,3-dimethylphenyl)acetamide hydrochloride
BP Name	Lidocaine Impurity F hydrochloride
Synonym(s)	2-diethylamino-2',3'-acetoxylidide hydrochloride
Epichem Item #	EPL-AA237 Batch 1
CAS#	857170-72-0
Molecular Formula	C <sub>14</sub> H <sub>23</sub> ClN <sub>2</sub> O
Molecular Weight	270.80 g/mol
Appearance	White solid
<b>Melting Point</b>	107.7-111.1°C
<b>Combustion Analysis</b>	Required (%): C:62.1, H:8.6, N:10.3. Found (%): C:62.0, H:8.8, N:10.4.
Purity*	99.7%
Date of Manufacture	30 August 2019
<b>Storage Requirements</b>	Protect from heat, light and moisture.
<b>Special Precautions</b>	This compound is for laboratory use only. Its toxicological properties may not have been fully established. It should be handled only by suitably qualified personnel.
Intended Use	This compound is suitable for the identification of impurities and degradants in pharmaceutical materials. The purity assay is considered as relative contribution.
Date of Shipment	TBA
	This certificate is valid for one year from the date of shipment provided the substance is unopened and stored under the recommended conditions.
Retest Date	TBA (Proper Storage and Handling Required)

<sup>\*</sup> NATA accreditation does not cover the performance of this service

EPL-AA237 Batch 1

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

Form PC008.F07 **Product Information Sheet** Page 1 of 7


# I. Identity

The identity of this product was established using the following analyses:

# Ia. <sup>1</sup>HNMR Spectrum

Conditions: 400 MHz, DMSO-d<sub>6</sub>

<sup>1</sup>HNMR spectrum consistent with chemical structure.

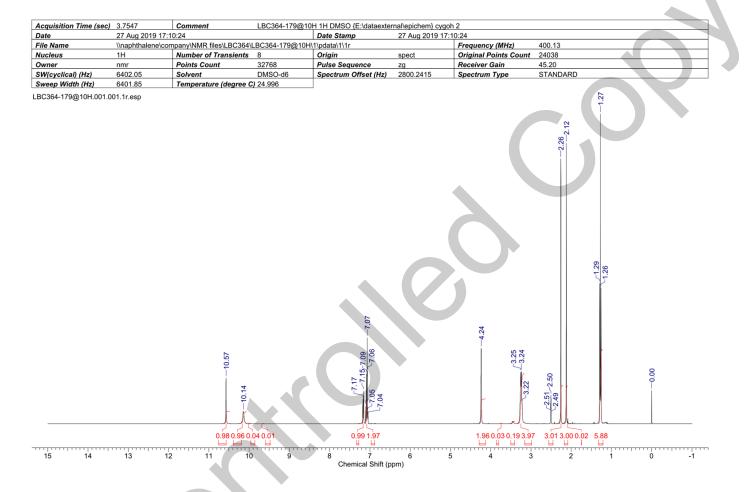


## **Ib.** Mass Spectrum

The mass spectrum of this material was analysed by Liquid Chromatography Mass Spectroscopy (LCMS) using inhouse EM005.WI08.

Method: ACN/water gradient (+ 0.1% formic acid).

ZORBAX SB-C8, 4.6 x 30 mm, 3.5 micron.

Retention		Mol. Weight
Time (MS)	MS Area	or Ion
2.102	19111624	236.20 I
		235.20 I

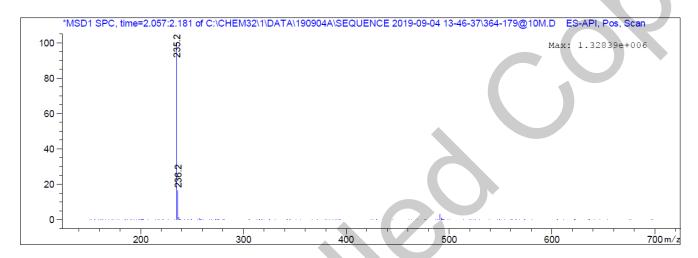


Theoretical value: 235.2 [M-Cl]<sup>+</sup>.

The signal of the Mass Spectrum is consistent with the theoretical value and its interpretation is consistent with the structural formula.

Form PC008.F07 Product Information Sheet Page 3 of 7

## Ic. IR Spectrum

The infra-red spectrum of this material was analysed by Fourier-Transform Infrared Spectroscopy (FTIR) using inhouse EM005.WI09.

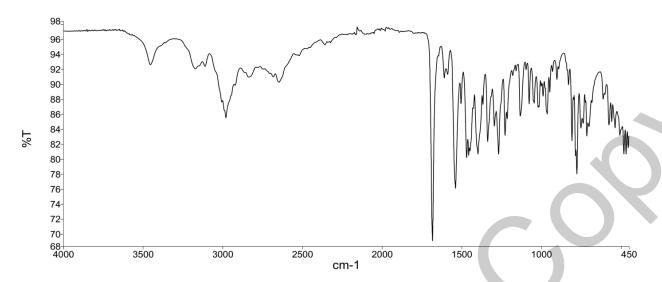


The interpretation of the signals of the Fourier-Transform Infrared Spectrum is consistent with the structural formula.

# II. Purity

The purity of this material was analysed by high performance liquid chromatography (HPLC) using in-house EM005.WI07.

## **HPLC Conditions:**

Column	Conditions			Detector	Injector	
Agilent Poroshell	25°C				DAD	Auto
120 EC C-18 4.6 x 50 mm	Time (min)	% Line A (Water + 0.1% (v/v) TFA)	% Line B (Acetonitrile + 0.1% (v/v) TFA)	Flow rate (mL/min)	220nm	1.0 µL 1.0mg/mL in water (+0.1% (v/v) TFA)
	0.00	95	5	1.0		(1111)
2.7 micron	6.00	77	23	1.0		
	13.20	5	95	1.0		
	18.20	5	95	1.0		
	19.20	95	5	1.0		
	22.20	95	5	1.0		

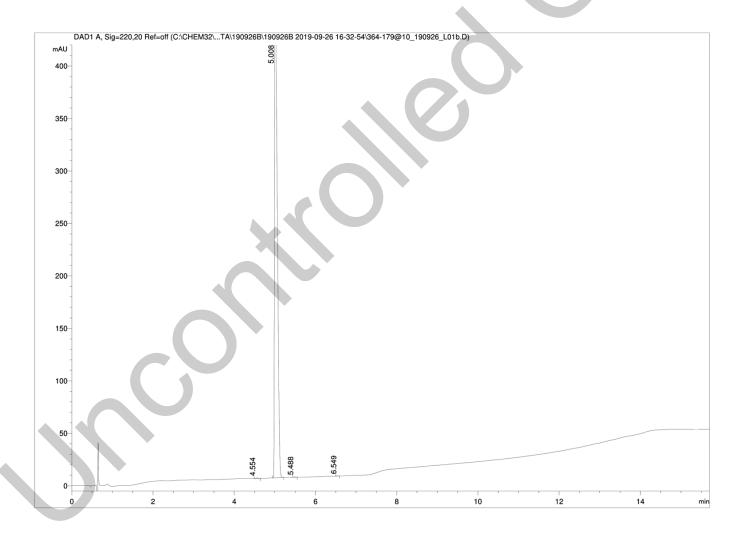

EPL-AA237 Batch 1

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902


## Area Percent Report - Sorted by Signal

Peak Number	Retention Time (rounded)	Area	Area % (rounded)
1	4.58	1.89	0.08
2	5.03	2229.19	99.89
3	5.52	0.36	0.02
4	6.58	0.26	0.01
Totals			100 (rounded)

For the calculation the system peaks were ignored. The content of the analyte was determined as a ratio of the peak area of the analyte and the cumulative areas of the purities, added up to 100%.

#### **Results:**

Average 99.9% (average of 10 duplicate analyses)



Form PC008.F07 Product Information Sheet Page 6 of 7

## **III. Water Content**

Method: Karl-Fischer titration using in-house EM005.WI04.

**Results:** 

Average 0.1%

# IV. Ash Content

Method: BP 2019 Ash Appendix XIJ Method II

**Result:** 

Contains <0.1% ash.

#### V. Residual Solvents

Method: <sup>1</sup>HNMR

**Result:** 

Contains 0.1% acetone by <sup>1</sup>H NMR analysis.

## VI. Final Result

Chromatographic purity (HPLC)	99.9%
Water content	0.1%
Ash content	<0.1%
Residual solvents	0.1%
Purity*	99.7%

This purity is assessed to be 99.7%.

Product Reviewed By:

Product Released By:

John Moursounidis, PhD Head Reference Standards

Boon Tan

Quality Manager

Release Date: 15 October 2019

 $Purity(\%) = \frac{((Chromatographicpurity[HPLC])x(100 - (watercontent + ashcontent + volatilecontents)))}{100}$ 

EPL-AA237 Batch 1

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

<sup>\*</sup>NATA accreditation does not cover the performance of this service.

The calculation of the purity follows the formula: