



Accredited for compliance with ISO 17034
This document shall not be reproduced except in full.
Accreditation Number: 20126
Corporate Site Number: 24143


The results of the tests, calibrations and/or measurements included in this document are traceable to Australia/national standards.
NATA is a signatory to the APLAC Mutual Recognition Arrangement for the mutual recognition of the equivalence of reference materials certificates.



Our Formula. Your Success.

Reference Material Product Information Sheet

Epichem's Quality System conforms to ISO9001:2015 as certified by ECAAS Pty Ltd - Certification number 616061.



| | |
|-----------------------------|---|
| Name | (3-endo, 8-syn)-8-methyl-8-(1-methylethyl)-3-((1-oxo-2-phenyl-2-propen-1-yl)oxy)-8-azoniabicyclo[3.2.1]octane bromide (1:1) |
| BP Name | Ipratropium bromide Impurity F |
| Synonym(s) | Apo-ipratropium bromide |
| Epichem Item # | EPL-AA240 Batch 1 |
| CAS # | 60018-35-1 |
| Molecular Formula | C ₂₀ H ₂₈ BrNO ₂ |
| Molecular Weight | 394.36 g/mol |
| Appearance | White powder |
| Melting Point | 256.5-257.1°C (decomposition) |
| Combustion Analysis | Required (%): C:60.9, H:7.2, N:3.5. Found (%): C:61.1, H:7.4, N:3.5. |
| Purity* | 99.8% |
| Date of Manufacture | 17 October 2019 |
| Storage Requirements | Protect from heat, light and moisture. |
| Special Precautions | This compound is for laboratory use only. Its toxicological properties may not have been fully established. It should be handled only by suitably qualified personnel. |
| Intended Use | This compound is suitable for the identification of impurities and degradants in pharmaceutical materials. The purity assay is considered as relative contribution. |
| Date of Shipment | TBA This certificate is valid for one year from the date of shipment provided the substance is unopened and stored under the recommended conditions. |
| Retest Date | TBA (Proper Storage and Handling Required) |

* NATA accreditation does not cover the performance of this service

EPL-AA240 Batch 1

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902


I. Identity

The identity of this product was established using the following analyses:

Ia. ¹H NMR Spectrum

Conditions: 400 MHz, DMSO-d₆

¹H NMR spectrum consistent with chemical structure.

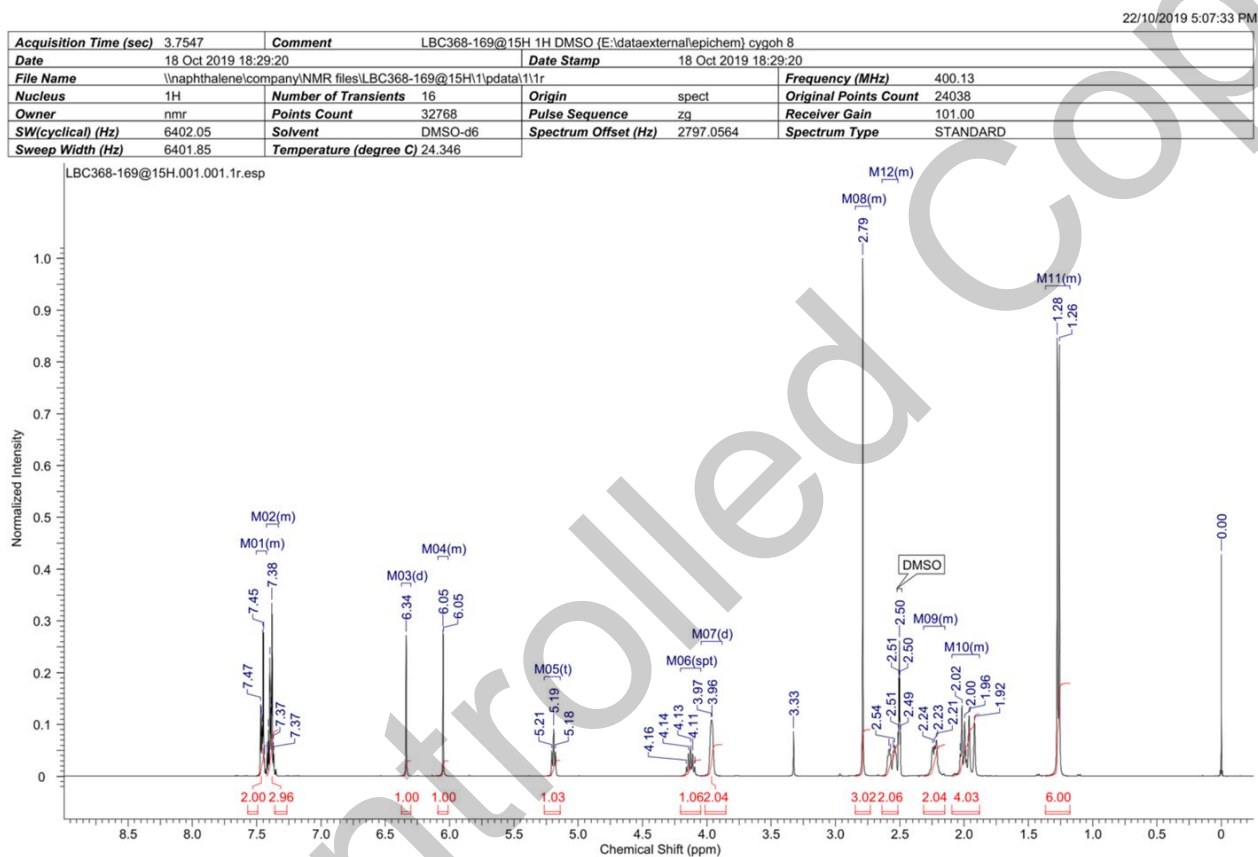

EPL-AA240 Batch 1

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia

Tel + 61 (0)8 6167 5200

Fax + 61 (0)8 6167 5201

www.epichem.com.au


ABN 80 106 769 902

Ib. Mass Spectrum

The mass spectrum of this material was analysed by Liquid Chromatography Mass Spectroscopy (LCMS) using in-house EM005.WI08.

Method: ACN/water gradient (+ 0.1% formic acid).
ZORBAX SB-C8, 4.6 x 30 mm, 3.5 micron.

| Retention Time (MS) | MS Area | Mol. Weight or Ion |
|---------------------|----------|----------------------|
| 2.566 | 15871777 | 315.20 I 314.20 I |

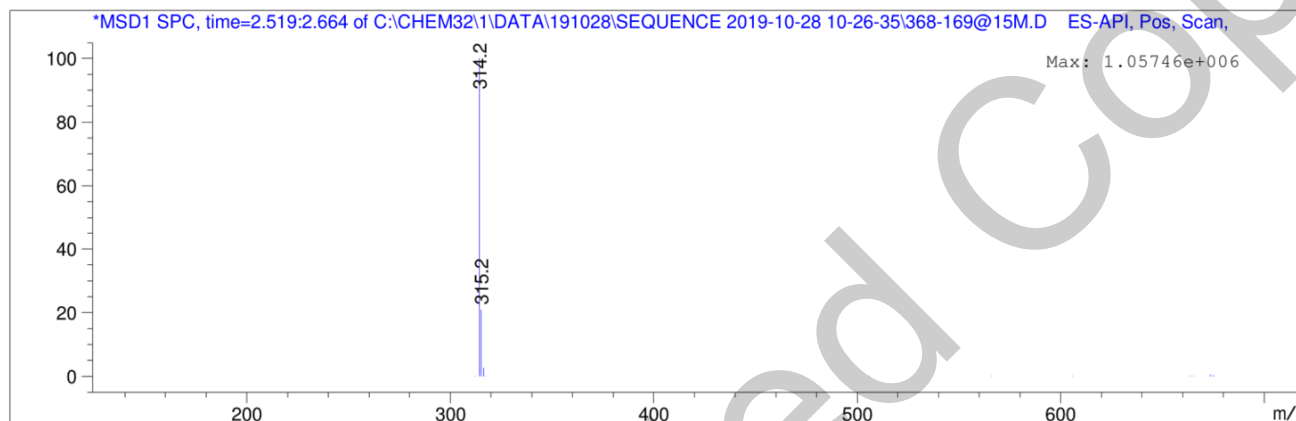

Theoretical value: 314.2 [M-Br]⁺.


The signal of the Mass Spectrum is consistent with the theoretical value and its interpretation is consistent with the structural formula.

EPL-AA240 Batch 1

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

Ic. IR Spectrum

The infra-red spectrum of this material was analysed by Fourier-Transform Infrared Spectroscopy (FTIR) using in-house EM005.WI09.

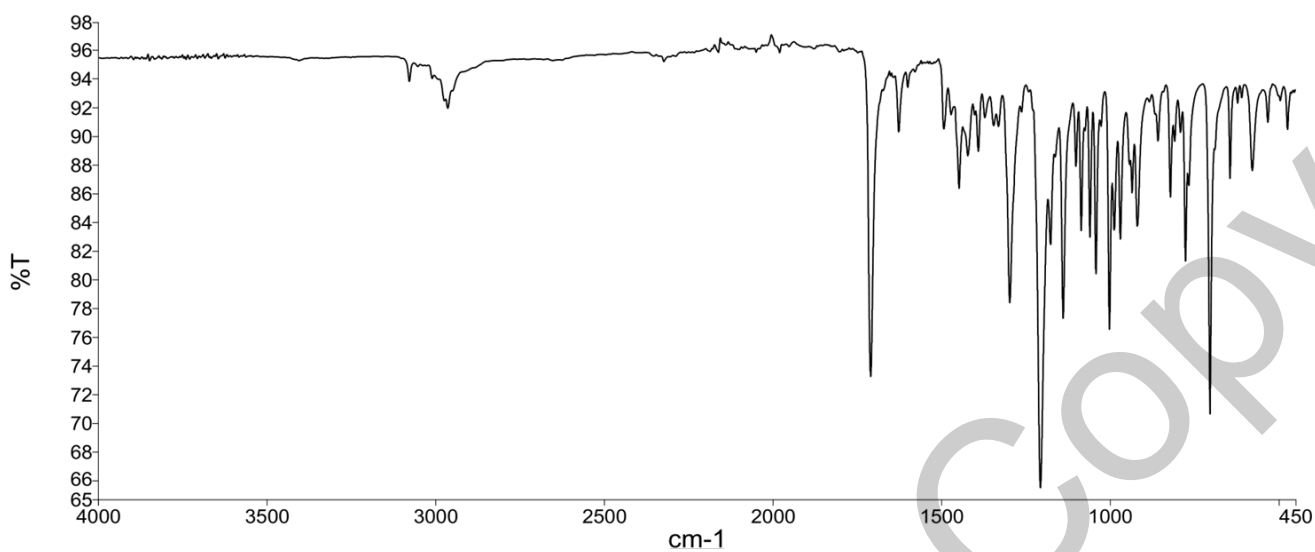

The interpretation of the signals of the Fourier-Transform Infrared Spectrum is consistent with the structural formula.

EPL-AA240 Batch 1


Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

II. Purity

The purity of this material was analysed by high performance liquid chromatography (HPLC) using in-house EM005.WI07.

HPLC Conditions:

| Column | Conditions | | | | Detector | Injector |
|---|------------|-----------------------------------|--|--------------------|--------------|--|
| Agilent Poroshell 120 EC C-18 4.6x50 mm 2.7 micron | 25°C | | | | DAD 248nm | Auto 1.0 µL 1.8mg/mL in 100% acetonitrile (NO MODIFIERS) |
| | Time (min) | % Line A (Water + 0.1% (v/v) TFA) | % Line B (Acetonitrile + 0.1% (v/v) TFA) | Flow rate (mL/min) | | |
| | 0.00 | 85 | 15 | 1.0 | | |
| | 6.00 | 55 | 45 | 1.0 | | |
| | 11.00 | 5 | 95 | 1.0 | | |
| | 16.00 | 5 | 95 | 1.0 | | |
| | 17.00 | 85 | 15 | 1.0 | | |
| | 20.00 | 85 | 15 | 1.0 | | |

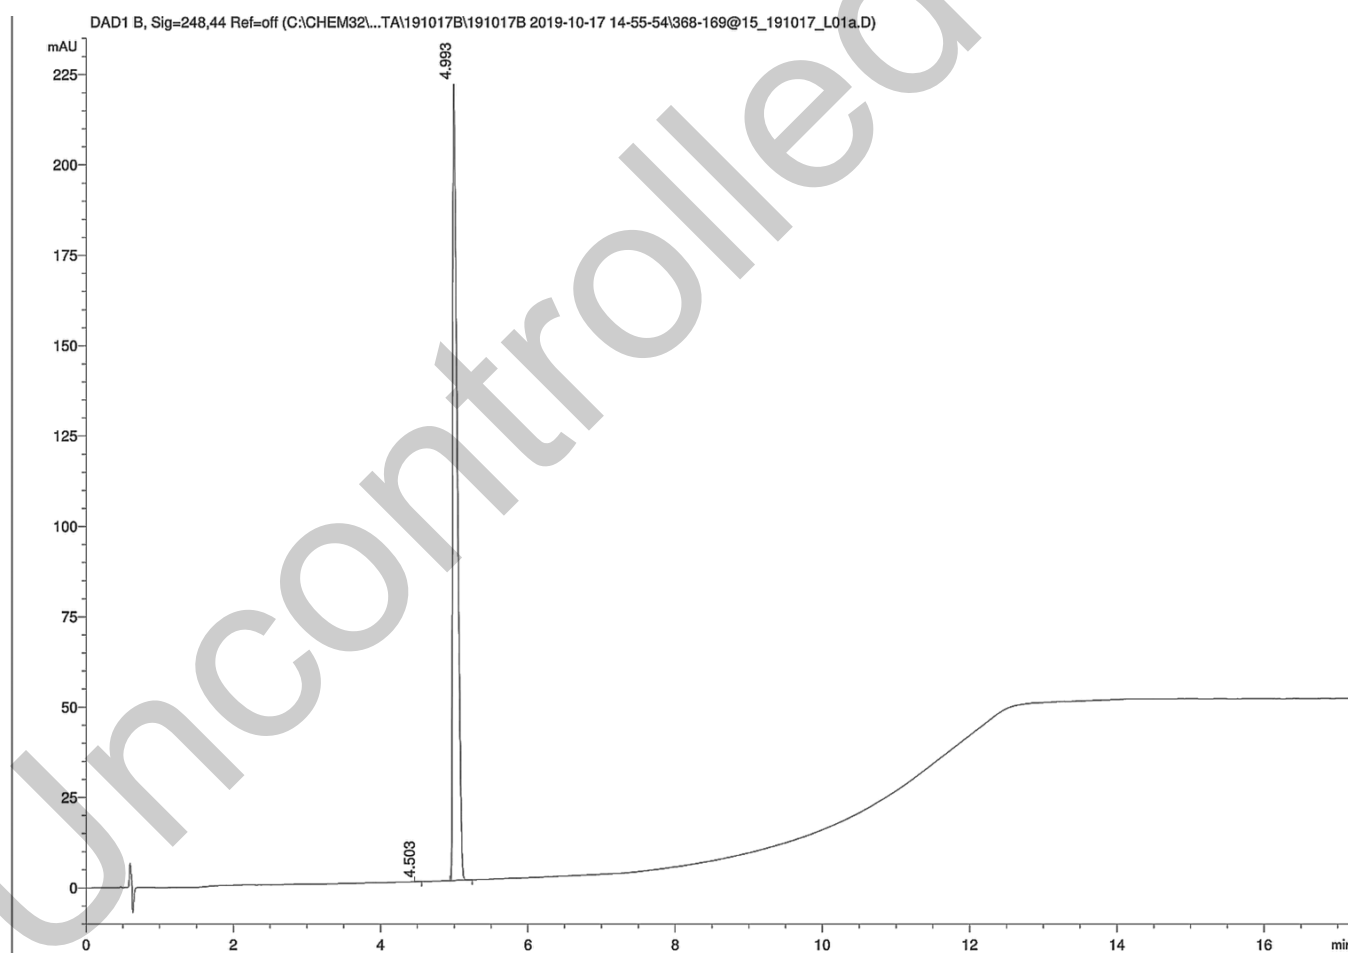

EPL-AA240 Batch 1

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

Area Percent Report – Sorted by Signal

| Peak Number | Retention Time (rounded) | Area | Area % (rounded) |
|-------------|--------------------------|--------|------------------|
| 1 | 4.50 | 0.16 | 0.02 |
| 2 | 4.99 | 951.04 | 99.98 |
| Totals | | | 100 (rounded) |

For the calculation the system peaks were ignored. The content of the analyte was determined as a ratio of the peak area of the analyte and the cumulative areas of the purities, added up to 100%.

Results:

Average 100.0% (average of 10 duplicate analyses)

EPL-AA240 Batch 1

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

III. Water Content

Method: Karl-Fischer titration using in-house EM005.WI04.

Results:

Average 0.1%

IV. Ash Content

Method: BP 2019 Ash Appendix XIJ Method II

Result:

Contains 0.1% ash.

V. Residual Solvents

Method: ¹H NMR

Result:

<0.1% by ¹H NMR analysis.

VI. Final Result

| | |
|-------------------------------|--------|
| Chromatographic purity (HPLC) | 100.0% |
| Water content | 0.1% |
| Ash content | 0.1% |
| Residual solvents | <0.1% |
| Purity* | 99.8% |

This purity is assessed to be 99.8%.

Product Reviewed By:

Product Released By:

John Moursounidis, PhD
Head Reference Standards

Boon Tan
Quality Manager

Release Date: 6 November 2019

*NATA accreditation does not cover the performance of this service.
The calculation of the purity follows the formula:

$$\text{Purity(\%)} = \frac{((\text{Chromatographicpurity[HPLC]}) \times (100 - (\text{watercontent} + \text{ashcontent} + \text{volatilecontents})))}{100}$$

EPL-AA240 Batch 1

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902