



Accredited for compliance with ISO 17034
This document shall not be reproduced except in full.
Accreditation Number: 20126
Corporate Site Number: 24143


The results of the tests, calibrations and/or measurements included in this document are traceable to Australia/national standards.
NATA is a signatory to the APLAC Mutual Recognition Arrangement for the mutual recognition of the equivalence of reference materials certificates.



Our Formula. Your Success.

Reference Material Product Information Sheet

Epichem's Quality System conforms to ISO9001:2015 as certified by ECAAS Pty Ltd - Certification number 616061.

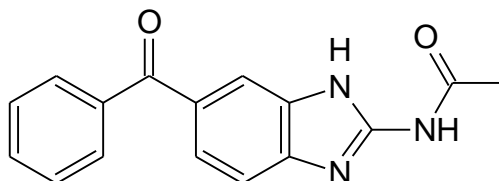

Name	<i>N</i> -(6-benzoyl-1 <i>H</i> -benzimidazol-2-yl)acetamide
Synonym(s)	<i>N</i> -(5-benzoyl-1 <i>H</i> -benzimidazol-2-yl)acetamide
Epichem Item #	EPL-AA248 Batch 1
CAS #	108227-95-8
Molecular Formula	C ₁₆ H ₁₃ N ₃ O ₂
Molecular Weight	279.30 g/mol
Appearance	White powder
Melting Point	303.4-309.0°C (decomposition)
Combustion Analysis	Required (%): C: 68.8, H: 4.7, N: 15.1. Found (%): C: 68.6, H: 4.4, N: 15.0.
Purity*	98.6%
Date of Manufacture	22 August 2019
Storage Requirements	Protect from heat, light and moisture.
Special Precautions	This compound is for laboratory use only. Its toxicological properties may not have been fully established. It should be handled only by suitably qualified personnel.
Intended Use	This compound is suitable for the identification of impurities and degradants in pharmaceutical materials. The purity assay is considered as relative contribution.
Date of Shipment	TBA
	This certificate is valid for one year from the date of shipment provided the substance is unopened and stored under the recommended conditions.
Retest Date	TBA (Proper Storage and Handling Required)

* NATA accreditation does not cover the performance of this service

EPL-AA248 Batch 1

Revision 1

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

I. Identity


The identity of this product was established using the following analyses:

Ia. ¹H NMR Spectrum

Conditions: 400 MHz, DMSO-d₆

¹H NMR spectrum consistent with chemical structure.

Acquisition Time (sec)	3.7547	Comment	LBC374-023@14H 1H DMSO (E:\data\external\epichem\cygoh 13		
Date	21 Aug 2019 18:22:56	Date Stamp	21 Aug 2019 18:22:56		
File Name	\naphthalene\company\NMR files\LBC374\LBC374-023@14H\1\data\1\1r		Frequency (MHz)	400.13	
Nucleus	1H	Number of Transients	8	Origin	spect
Owner	nmr	Points Count	1048576	Original Points Count	24038
SW(cyclical) (Hz)	6402.05	Solvent	DMSO-d6	Pulse Sequence	zg
Sweep Width (Hz)	6402.04	Temperature (degree C)	24.996	Receiver Gain	128.00
				Spectrum Offset (Hz)	2798.6941
				Spectrum Type	STANDARD

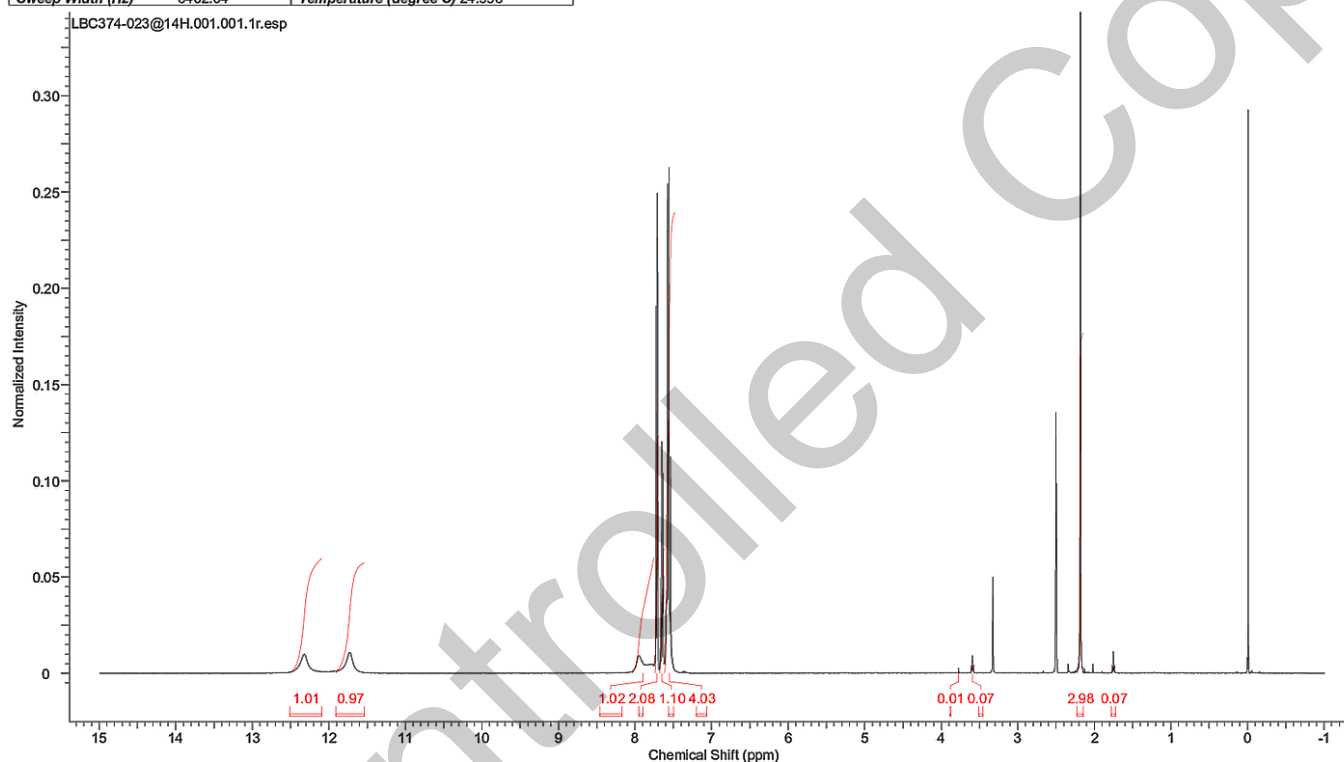

EPL-AA248 Batch 1

Revision 1

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia

Tel + 61 (0)8 6167 5200

Fax + 61 (0)8 6167 5201

www.epichem.com.au


ABN 80 106 769 902

Ib. Mass Spectrum

The mass spectrum of this material was analysed by Liquid Chromatography Mass Spectroscopy (LCMS) using in-house EM005.WI08.

Method: ACN/water gradient (+0.1% formic acid)
ZORBAX SB-C8, 4.6 x 30 mm, 3.5 micron

Retention Time (MS)	MS Area	Mol. Weight or Ion
2.563	6220806	281.10 I 280.10 I

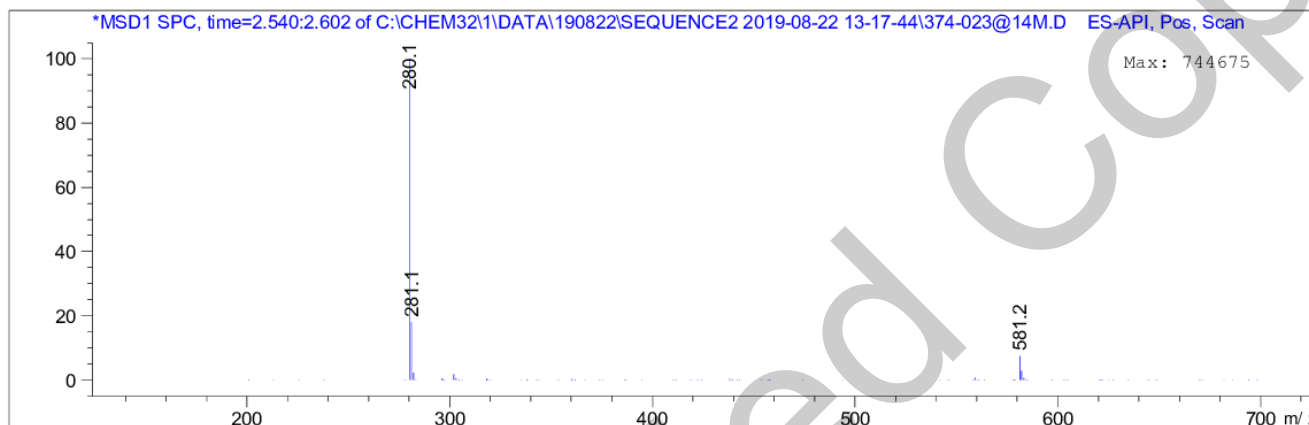


Theoretical value: 280.1 [M+H]⁺

The signal of the Mass Spectrum is consistent with the theoretical value and its interpretation is consistent with the structural formula.

Ic. IR Spectrum

The infra-red spectrum of this material was analysed by Fourier-Transform Infra-red Spectroscopy (FTIR) using in-house EM005.WI09.

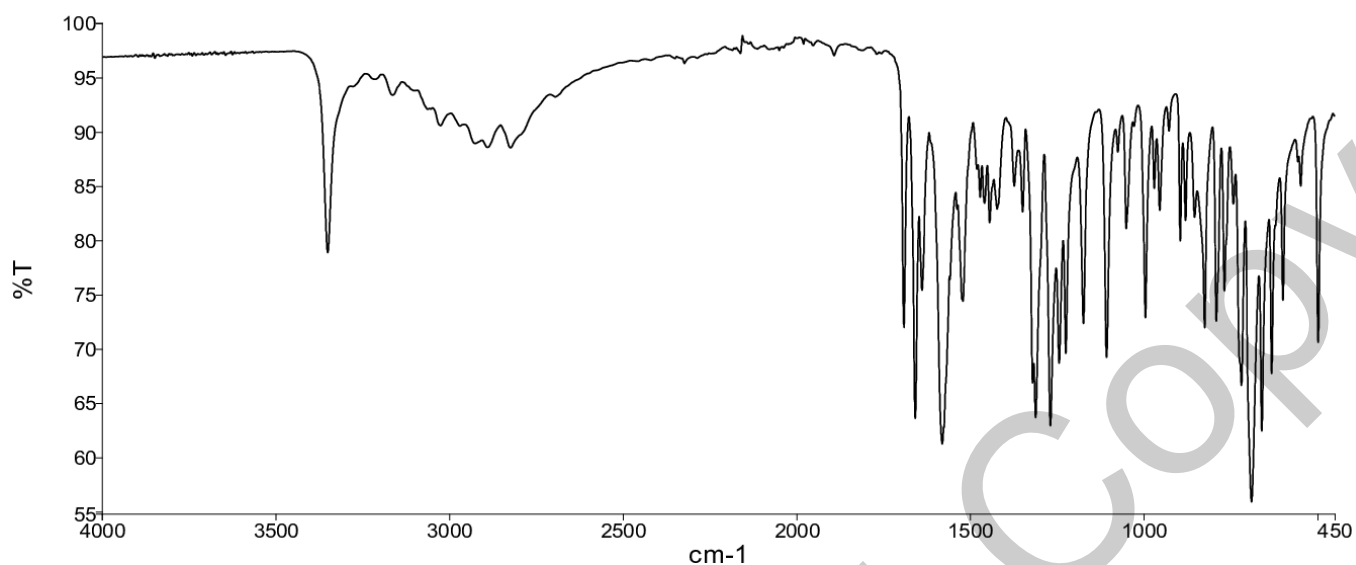


The interpretation of the signals of the Fourier Transform Infra-red Spectrum is consistent with the structural formula.

II. Purity

The purity of this material was analysed by high performance liquid chromatography (HPLC) using in-house EM005.WI07.

HPLC Conditions:

Column	Conditions				Detector	Injector
Agilent Poroshell 120 EC-C18 4.6 x 50mm 2.7 micron	25°C				DAD 295nm	Auto 1.0 µL 0.30mg/mL in 50% acetonitrile 50% dimethylsulfoxide (NO MODIFIERS)
	Time (min)	% Line A (Water + 0.1% (v/v) TFA)	% Line B (Acetonitrile + 0.1% (v/v) TFA)	Flow rate (mL/min)		
	0.00	90	10	1.0		
	6.00	66	34	1.0		
	12.10	5	95	1.0		
	17.10	5	95	1.0		
	18.10	90	10	1.0		
	21.10	90	10	1.0		

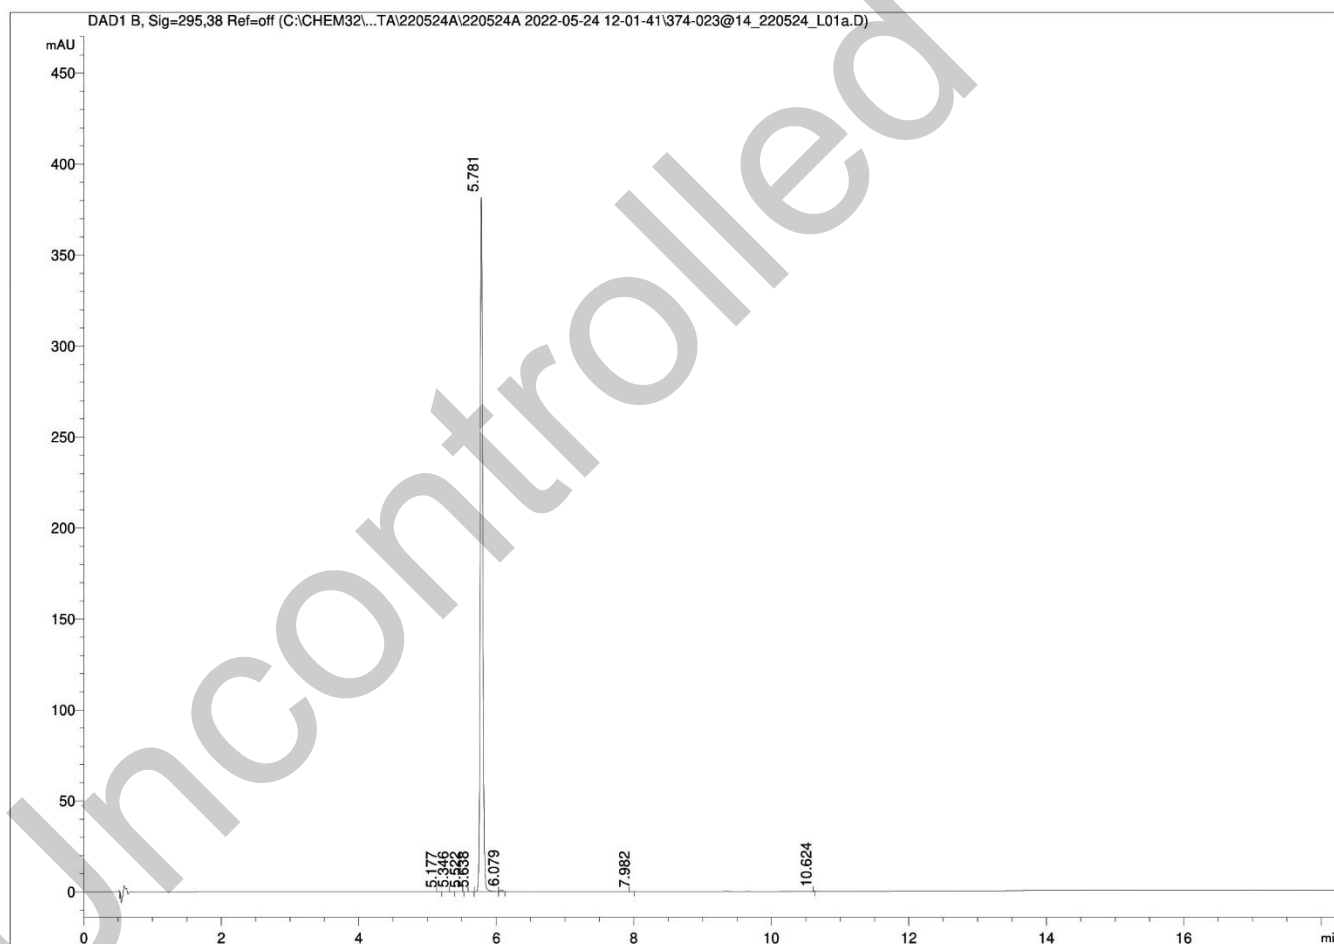

EPL-AA248 Batch 1

Revision 1

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

Area Percent Report – Sorted by Signal

Peak Number	Retention Time (rounded)	Area	Area % (rounded)
1	5.18	0.05	0.00
2	5.35	0.11	0.01
3	5.52	0.03	0.00
4	5.64	0.13	0.01
5	5.78	967.34	99.69
6	6.08	2.38	0.25
7	7.98	0.06	0.01
8	10.62	0.22	0.02
Totals			100 (rounded)

For the calculation the system peaks were ignored. The content of the analyte was determined as a ratio of the peak area of the analyte and the cumulative areas of the purities, added up to 100%.

Results:

Average 99.7% (average of 10 duplicate analyses)

III. Water Content

Method: Karl-Fischer titration using in-house EM005.WI04.

Results:

Average 0.1%

IV. Ash Content

Method: BP 2019 Ash Appendix XIJ Method II

Result:

Contains 0.6% ash.

V. Residual Solvents

Method: ¹H NMR

Result:

Contains 0.4 wt% tetrahydrofuran by ¹H NMR analysis.

VI. Final Result

Chromatographic purity (HPLC)	99.7%
Water content	0.1%
Ash content	0.6%
Residual solvents	0.4%
Purity*	98.6%

This purity is assessed to be 98.6%

Product Reviewed By:

Product Released By:

James Rixson, PhD
Head of Production

Jason Chaplin
Principal Chemist

Release Date: 2 June 2022

*NATA accreditation does not cover the performance of this service.

The calculation of the purity follows the formula:

$$\text{Purity(\%)} = \frac{((\text{Chromatographic purity [HPLC]}) \times (100 - (\text{water content} + \text{ash content} + \text{volatile contents})))}{100}$$

EPL-AA248 Batch 1

Revision 1

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902