



Accredited for compliance with ISO17034 and ISO/IEC17025.  
This document shall not be reproduced except in full.  
Accreditation Number: 20126


NATA is a signatory to the ILAC Mutual Recognition Arrangement for the mutual recognition of the equivalence of reference materials certificates.



Our Formula. Your Success.

## Reference Material Product Information Sheet

Epichem's Quality System conforms to ISO9001:2015 as certified by ECAAS Pty Ltd - Certification number 616061.

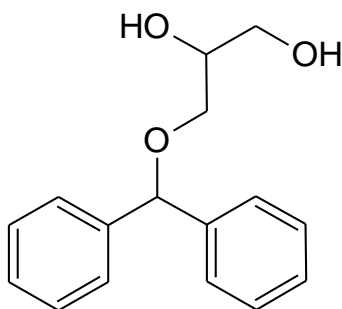

<b>Name</b>	(RS)-3-(benzhydryloxy)propane-1,2-diol
<b>Synonym(s)</b>	(RS)-3-(diphenylmethoxy)-1,2-propanediol; (RS)-3-(diphenylmethoxy)propane-1,2-diol
<b>Epichem Item #</b>	EPL-AA27 Batch 5
<b>CAS #</b>	19574-66-4
<b>Molecular Formula</b>	C <sub>16</sub> H <sub>18</sub> O <sub>3</sub>
<b>Molecular Weight</b>	258.32 g/mol
<b>Appearance</b>	White crystalline powder
<b>Melting Point</b>	51.4-54.7°C
<b>Combustion Analysis</b>	Required (%): C:74.4; H:7.0. Found (%): C:74.3; H:7.0.
<b>Purity*</b>	99.2%
<b>Date of Manufacture</b>	10 October 2017
<b>Storage Requirements</b>	Protect from heat, light and moisture.
<b>Special Precautions</b>	<b>This compound is for laboratory use only. Its toxicological properties may not have been fully established. It should be handled only by suitably qualified personnel.</b>
<b>Intended Use</b>	This compound is suitable for the identification of impurities and degradants in pharmaceutical materials. The purity assay is considered as relative contribution.
<b>Date of Shipment</b>	TBA This certificate is valid for one year from the date of shipment provided the substance is unopened and stored under the recommended conditions.
<b>Retest Date</b>	TBA (Proper Storage and Handling Required)

\* NATA accreditation does not cover the performance of this service

EPL-AA27 Batch 5

Revision 2

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902


## I. Identity

The identity of this product was established using the following analyses:

### Ia. <sup>1</sup>HNMR Spectrum

Conditions: 400 MHz, CDCl<sub>3</sub>

<sup>1</sup>HNMR spectrum consistent with chemical structure.

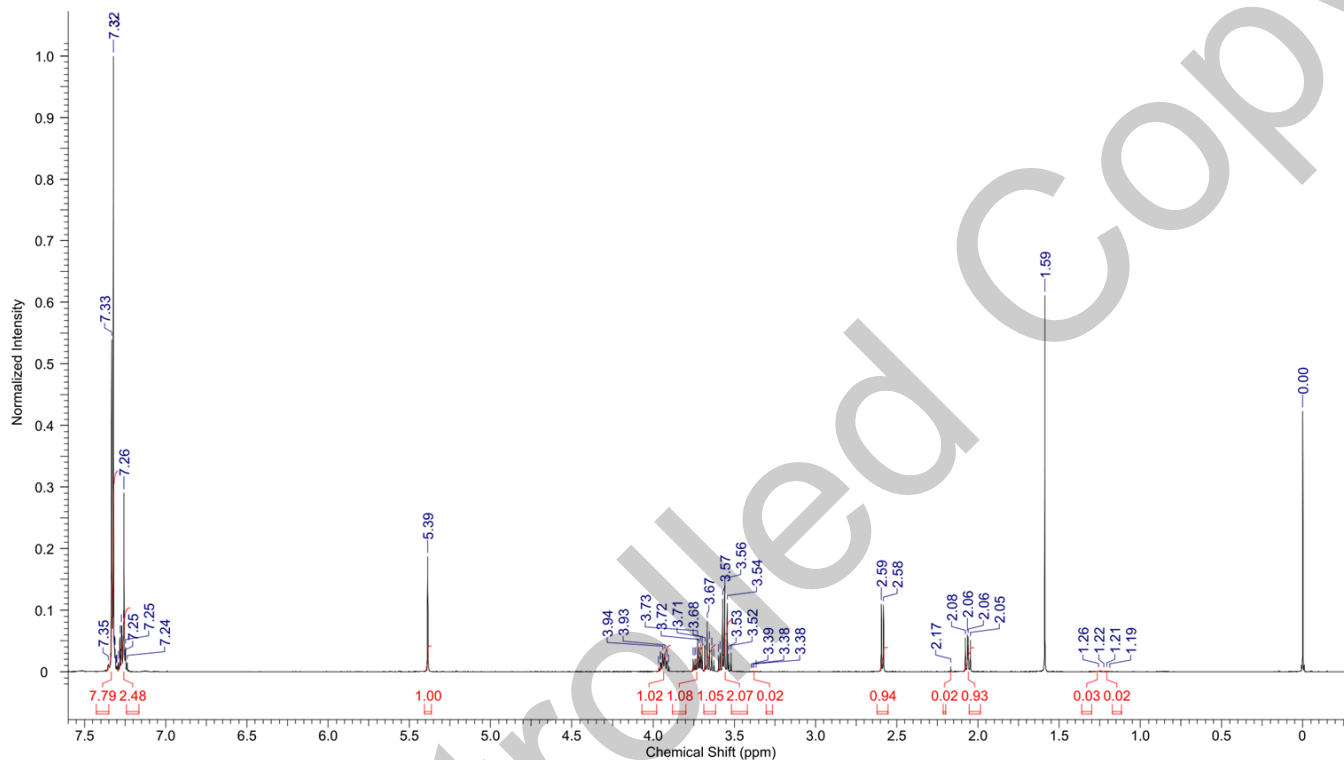

EPL-AA27 Batch 5

Revision 2


Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

## Ib. Mass Spectrum

The mass spectrum of this material was analysed by Liquid Chromatography Mass Spectroscopy (LCMS) using in-house EM005.WI08.

Method: 5% to 100% ACN in water gradient (+0.1% formic acid)  
Zorbax Eclipse XDB-C8, 3.0 x 100 mm, 3.5 micron

Retention Time (MS)	MS Area	Mol. Weight or Ion
3.816	2401507	282.10 I
		281.10 I
		168.10 I
		167.10 I
4.461	138520	243.20 I
		242.25 I
4.809	79126	242.30 I
4.968	263047	507.40 I
		502.30 I
		477.20 I
		464.30 I
		463.30 I
		458.30 I
		419.25 I
		414.25 I
		375.05 I

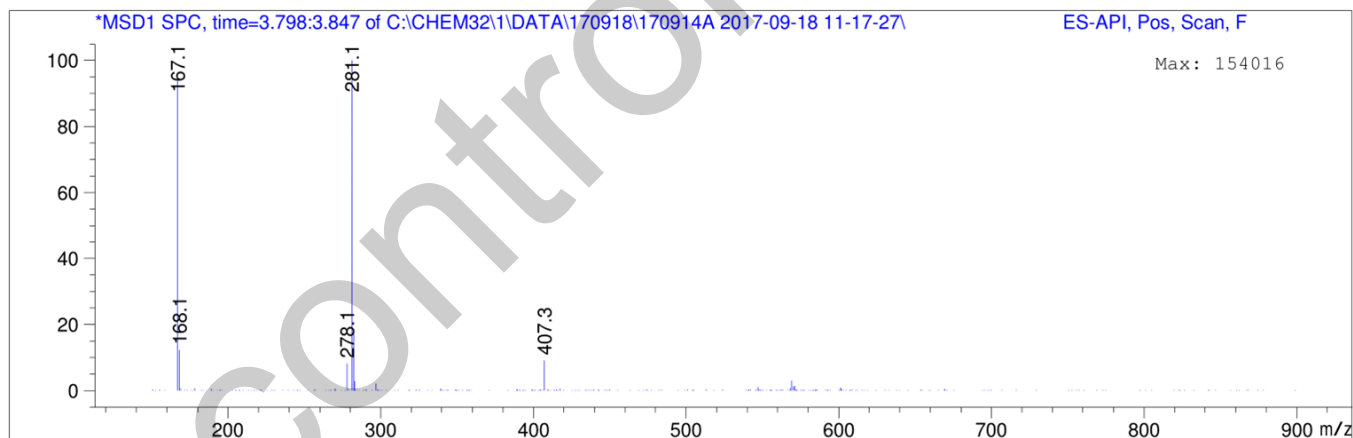

Theoretical value: 281.1 [M+Na]<sup>+</sup>.

The signal of the Mass Spectrum is consistent with the theoretical value and its interpretation is consistent with the structural formula.


EPL-AA27 Batch 5

Revision 2

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

### Ic. IR Spectrum

The infra-red spectrum of this material was analysed by Fourier-Transform Infrared Spectroscopy (FTIR) using in-house EM005.WI09.

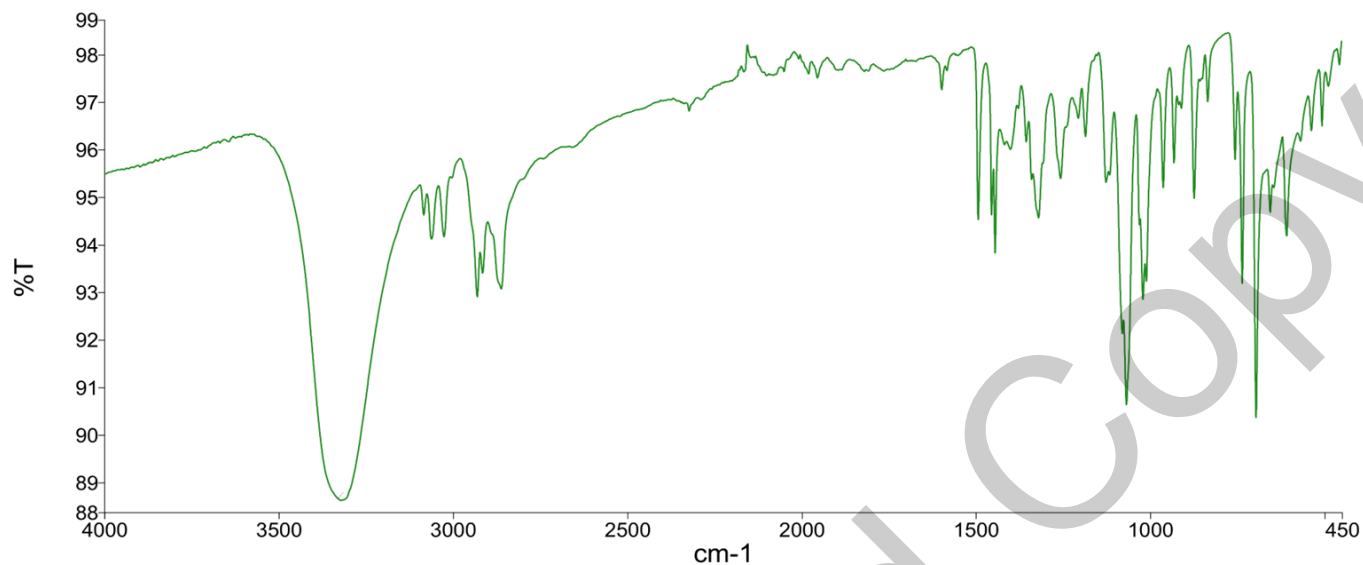

The interpretation of the signals of the Fourier-Transform Infrared Spectrum is consistent with the structural formula.

EPL-AA27 Batch 5

Revision 2


Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

## II. Purity

The purity of this material was analysed by high performance liquid chromatography (HPLC) using in-house EM005.WI07.

### HPLC Conditions:

Column	Conditions				Detector	Injector
Agilent Poroshell 120 EC-C18 4.6 x 50mm 2.7 micron	25°C				DAD 220nm	Auto 1.0 µL  0.8 mg/mL in 100% acetonitrile (NO MODIFIERS)
	Time (min)	% Line A (Water + 0.1% (v/v) TFA)	% Line B (Acetonitrile + 0.1% (v/v) TFA)	Flow rate (mL/min)		
	0.00	80	20	1.0		
	6.00	50	50	1.0		
	10.50	5	95	1.0		
	15.50	5	95	1.0		
	16.50	80	20	1.0		
	19.50	80	20	1.0		

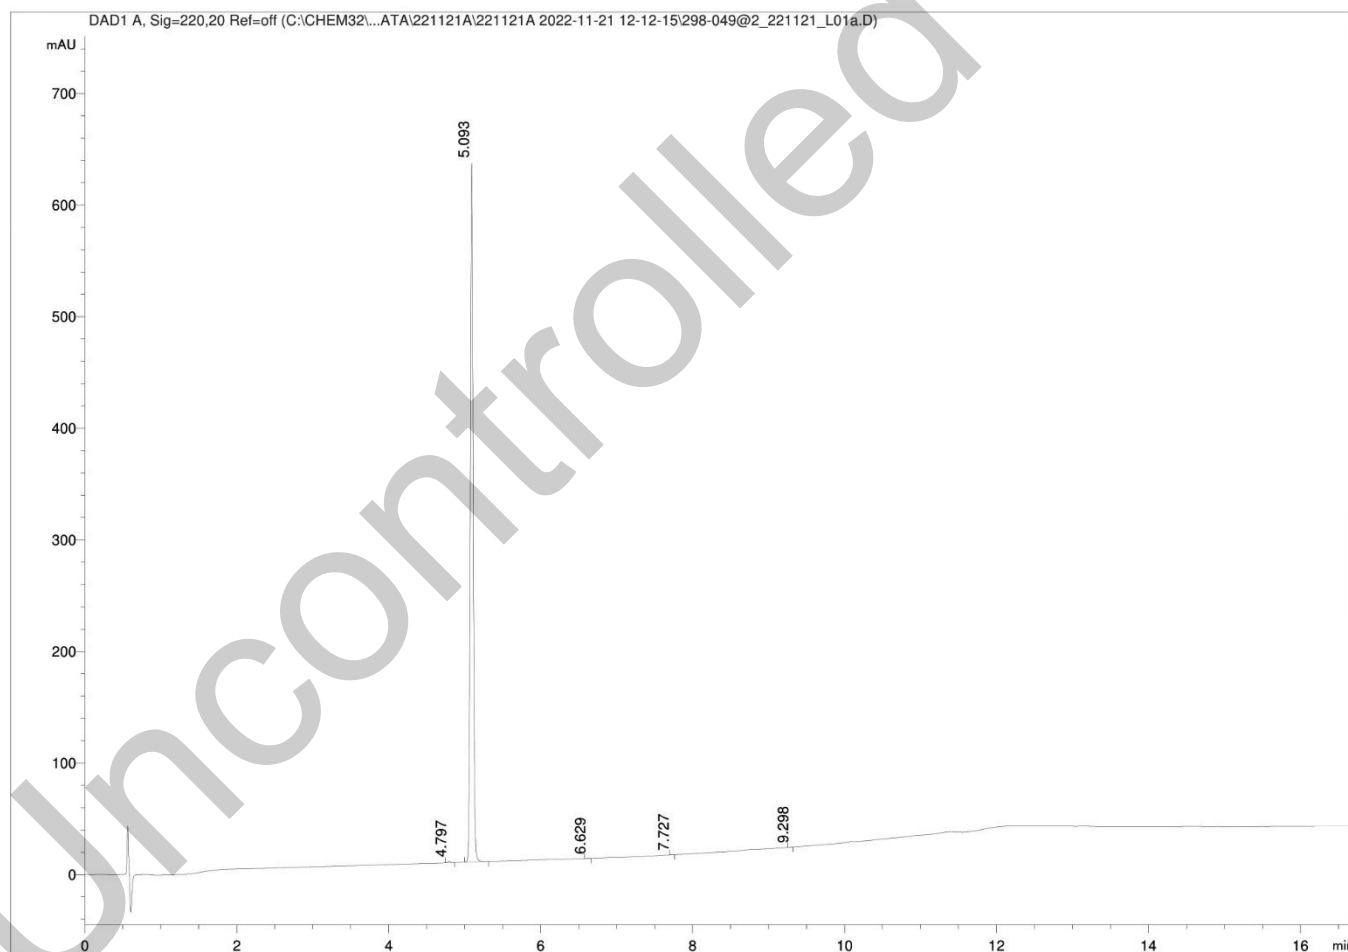

EPL-AA27 Batch 5

Revision 2

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

### Area Percent Report – Sorted by Signal

Peak Number	Retention Time (rounded)	Area	Area % (rounded)
1	4.80	3.75	0.23
2	5.09	1633.31	99.71
3	6.63	0.50	0.03
4	7.73	0.14	0.01
5	9.30	0.29	0.02
Totals			100 (rounded)

For the calculation the system peaks were ignored. The content of the analyte was determined as a ratio of the peak area of the analyte and the cumulative areas of the purities, added up to 100%.

#### Results:

Average 99.7% (average of 10 duplicate analyses)

### III. Water Content

Method: Karl-Fischer titration using in-house EM005.WI04.

**Results:**

Average 0.1%

### IV. Ash Content

Method: BP 2017 Ash (Appendix XI J) Method II

**Result:**

Contains 0.2% ash.

### V. Residual Solvents

Method: <sup>1</sup>H NMR

**Result:**

Contains 0.2% Diethyl ether by <sup>1</sup>H NMR analysis.

### VI. Final Result

Chromatographic purity (HPLC)	99.7%
Water content	0.1%
Ash content	0.2%
Residual solvents	0.2%
Purity*	99.2%

This purity is assessed to be 99.2%.

Product Reviewed By:

Product Released By:

Jacob Heppell, PhD  
Chemist

Carol Worth, PhD  
Quality Manager

Release Date: 23 November 2022

\*NATA accreditation does not cover the performance of this service.

The calculation of the purity follows the formula:

$$\text{Purity(\%)} = \frac{((\text{Chromatographic purity[HPLC]}) \times (100 - (\text{water content} + \text{ash content} + \text{volatile contents})))}{100}$$

EPL-AA27 Batch 5

Revision 2

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902