


## Reference Material Product Information Sheet

Epichem's Quality System conforms to ISO9001:2015 as certified by ECAAS Pty Ltd - Certification number 616061.

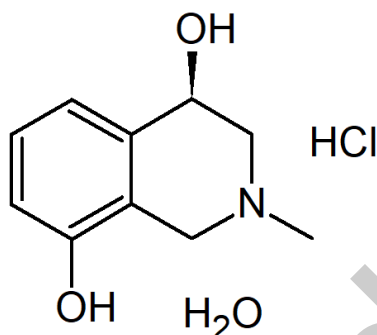

<b>Name</b>	(4R)-4,8-dihydroxy-N-methyl-1,2,3,4-tetrahydroisoquinoline hydrochloride monohydrate
<b>USP Name</b>	Phenylephrine Related Compound F
<b>Synonym(s)</b>	(4R)-2-methyl-1,2,3,4-tetrahydroisoquinoline-4,8-diol hydrochloride monohydrate; longimammamine hydrochloride monohydrate
<b>Epichem Item #</b>	EPL-AA3 Batch 18
<b>CAS #</b>	1007885-60-0
<b>Molecular Formula</b>	C <sub>10</sub> H <sub>13</sub> NO <sub>2</sub> .HCl.H <sub>2</sub> O
<b>Molecular Weight</b>	233.70 g/mol
<b>Appearance</b>	White crystalline powder
<b>Melting Point</b>	220.3-226.3°C (decomposition)
<b>Combustion Analysis</b>	Required (%): C:51.4; H:6.9; N:6.0. Found (%): C:51.5; H:7.0; N:5.9.
<b>Purity*</b>	100.0%
<b>Date of Manufacture</b>	29 January 2020
<b>Storage Requirements</b>	Protect from heat, light and moisture.
<b>Special Precautions</b>	<b>This compound is for laboratory use only. Its toxicological properties may not have been fully established. It should be handled only by suitably qualified personnel.</b>
<b>Intended Use</b>	This compound is suitable for the identification of impurities and degradants in pharmaceutical materials. The purity assay is considered as relative contribution.
<b>Date of Shipment</b>	TBA This certificate is valid for one year from the date of shipment provided the substance is stored under the recommended conditions.
<b>Retest Date</b>	TBA (Proper Storage and Handling Required)

\* NATA accreditation does not cover the performance of this service

EPL-AA3 Batch 18

Revision 4

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

## I. Identity

The identity of this product was established using the following analyses:


### Ia. <sup>1</sup>H NMR Spectrum

Conditions: 400 MHz, DMSO-d<sub>6</sub>  
<sup>1</sup>H NMR spectrum consistent with chemical structure.

29/01/2020 10:23:29 AM  
LBC383-127@17H 1H DMSO (E:\dataexternal\epichem) cygoh 13

Acquisition Time (sec)	3.7547	Comment	LBC383-127@17H 1H DMSO (E:\dataexternal\epichem) cygoh 13				
Date	29 Jan 2020 08:17:04	Date Stamp	29 Jan 2020 08:17:04				
File Name	\\naphthalene\company\NMR files\LBC383-127@17H\1\data\1\1r	Frequency (MHz)	400.13				
Nucleus	1H	Number of Transients	8	Origin	spect	Original Points Count	24038
Owner	nmr	Points Count	32768	Pulse Sequence	zg	Receiver Gain	203.00
SW(cyclical) (Hz)	6402.05	Solvent	DMSO-d6	Spectrum Offset (Hz)	2797.4246	Spectrum Type	STANDARD
Sweep Width (Hz)	6401.85	Temperature (degree C)	24.996				

<sup>1</sup>H NMR (400 MHz, DMSO-d<sub>6</sub>) δ ppm 2.97 (br. s., 3 H) 3.32 (s, 7 H) 3.48 (br. s., 1 H) 3.53 (br. s., 1 H) 4.01 (br. s., 1 H) 4.32 (br. s., 1 H) 4.81 (br. s., 1 H) 6.05 (d, *J*=4.69 Hz, 1 H) 6.84 (br. s., 2 H) 7.00 (br. s., 1 H) 7.10 - 7.24 (m, 1 H) 10.10 (br. s., 1 H)  
LBC383-127@17H.001.001.1r.esp

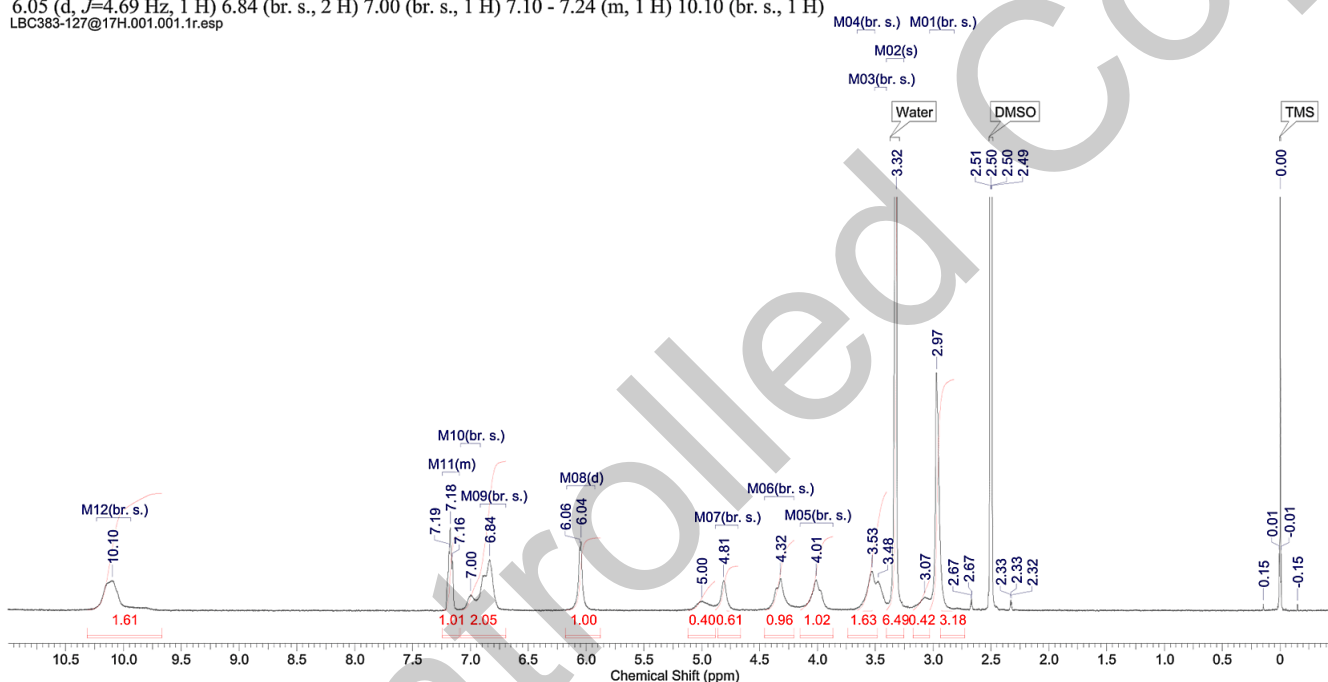

EPL-AA3 Batch 18

Revision 4

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia

Tel + 61 (0)8 6167 5200

Fax + 61 (0)8 6167 5201

www.epichem.com.au


ABN 80 106 769 902

## Ib. Mass Spectrum

The mass spectrum of this material was analysed by Liquid Chromatography Mass Spectroscopy (LCMS) using in-house EM005.WI08.

Method: ACN/water gradient (+ 0.1% formic acid).  
ZORBAX SB-C8, 4.6 x 30 mm, 3.5 micron.

Retention Time (MS)	MS Area	Mol. Weight or Ion
0.464	4219771	181.15   180.10

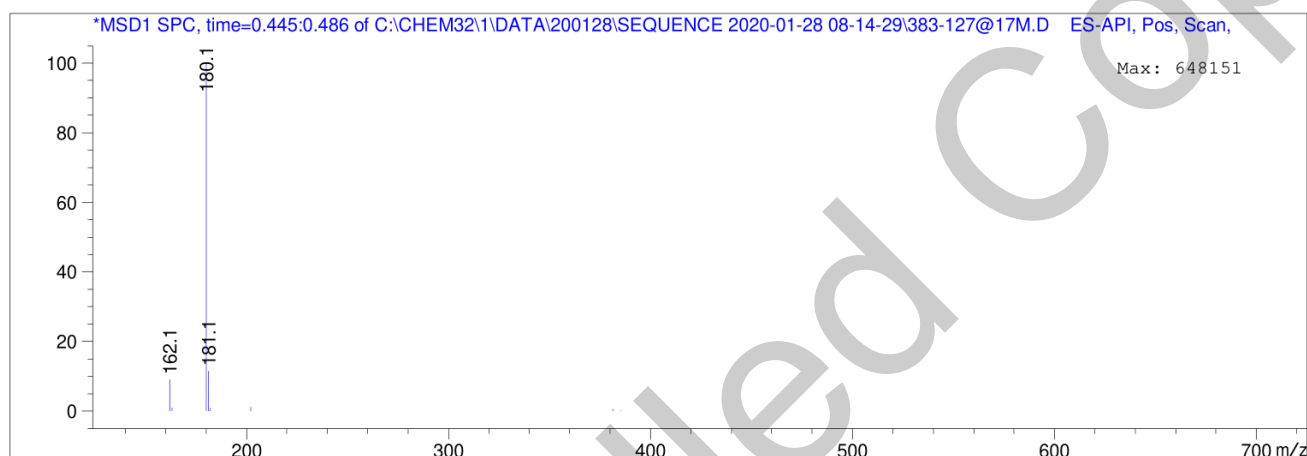

Theoretical value: 180.1 [M+H]<sup>+</sup>

The signal of the Mass Spectrum is consistent with the theoretical value and its interpretation is consistent with the structural formula.


EPL-AA3 Batch 18

Revision 4

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

### Ic. IR Spectrum

The infra-red spectrum of this material was analysed by Fourier-Transform Infrared Spectroscopy (FTIR) using in-house EM005.WI09.

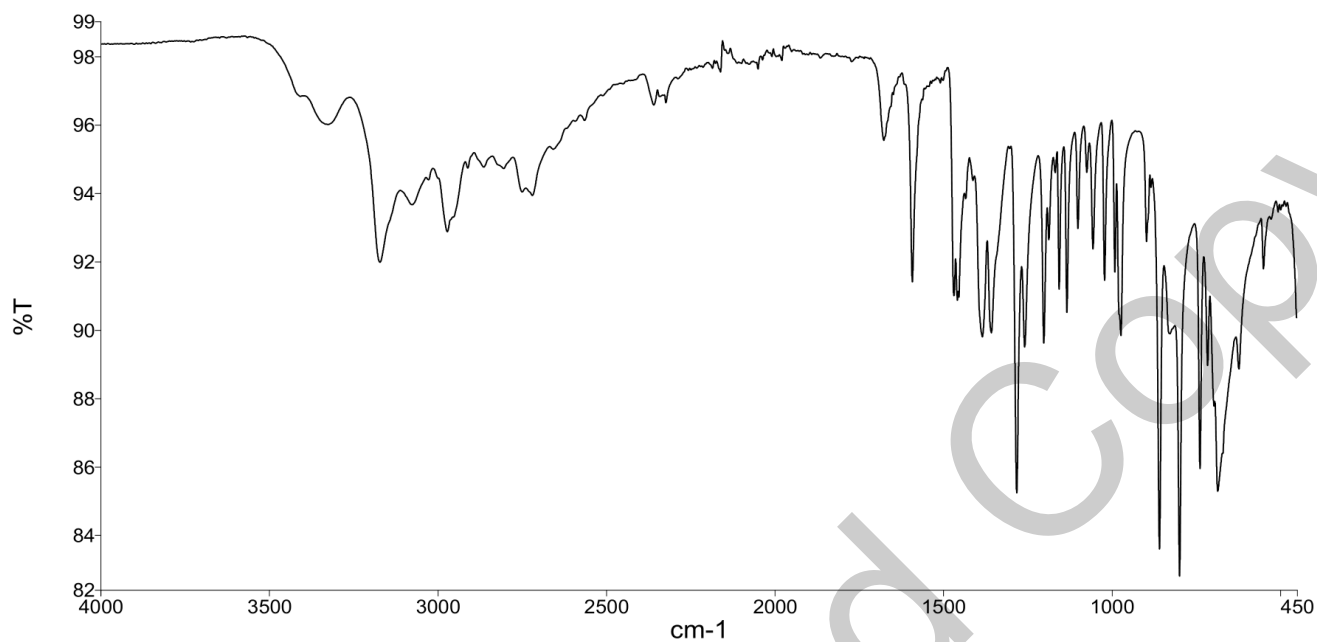

The interpretation of the signals of the Fourier-Transform Infrared Spectrum is consistent with the structural formula.

EPL-AA3 Batch 18

Revision 4


Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

## II. Purity

The purity of this material was analysed by high performance liquid chromatography (HPLC) using in-house EM005.WI07.

### HPLC Conditions:

Column	Conditions				Detector	Injector
Agilent Poroshell 120 EC-C8  3.0 x 100mm  2.7 micron	15°C				DAD  276nm	Auto  1.0 µL  1.0 mg/mL in 100% water (+0.1% TFA)
	Time (min)	% Line A (Water + 0.1% (v/v) TFA)	% Line B (Acetonitrile + 0.1% (v/v) TFA)	Flow rate (mL/min)		
	0.00	98	2	0.35		
	5.00	98	2	0.35		
	14.30	5	95	0.35		
	17.30	5	95	0.35		
	18.30	98	2	0.35		
26.80	98	2	0.35			

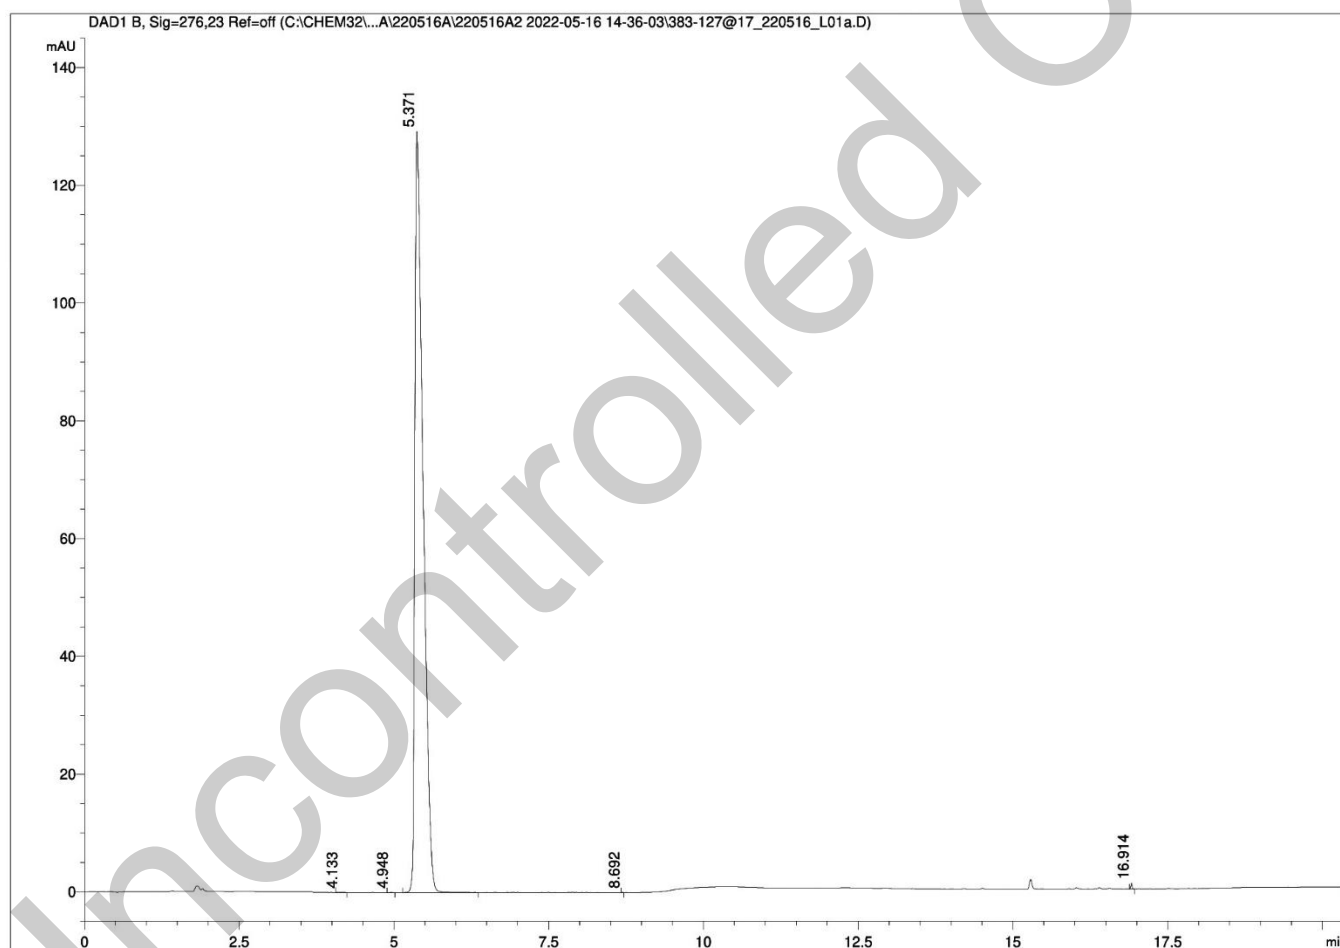

EPL-AA3 Batch 18

Revision 4

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

### Area Percent Report – Sorted by Signal

Peak Number	Retention Time (rounded)	Area	Area % (rounded)
1	4.13	0.13	0.01
2	4.95	0.03	0.00
3	5.37	1197.68	99.85
4	8.69	0.03	0.00
5	16.91	1.63	0.14
Totals			100 (rounded)

For the calculation the system peaks were ignored. The content of the analyte was determined as a ratio of the peak area of the analyte and the cumulative areas of the purities, added up to 100%.

#### Results:

Average 100% (average of 10 duplicate runs)

EPL-AA3 Batch 18

Revision 4

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902

### III. Water Content

Method: Karl-Fischer titration using in-house EM005.WI04.

**Results:**

Average 7.7% (consistent with monohydrate)

### IV. Ash Content

Method: BP 2019 Appendix XIJ Method II

**Result:**

Contains <0.1% ash.

### V. Residual Solvents

Method: <sup>1</sup>H NMR

**Result:**

No significant impurities detected by <sup>1</sup>H NMR analysis.

### VI. Final Result

Chromatographic purity (HPLC)	100.0%
Water content	7.7% (consistent with monohydrate)
Ash content	<0.1%
Residual solvents	<0.1%
Purity*	100.0%

This purity is assessed to be 100.0%.

Product Reviewed By:

James Rixson, PhD  
Head of Production

Product Released By:

Carol Worth, PhD  
Quality Manager  
Release Date: 18 May 2022

---

*\*NATA accreditation does not cover the performance of this service.*

The calculation of the purity follows the formula:

$$\text{Purity(\%)} = \frac{((\text{Chromatographicpurity[HPLC]}) \times (100 - (\text{watercontent} + \text{ashcontent} + \text{volatilecontents})))}{100}$$

EPL-AA3 Batch 18

Revision 4

Epichem Pty Ltd, Suite 5, 3 Brodie-Hall Drive, Bentley WA 6102, Australia  
Tel + 61 (0)8 6167 5200 Fax + 61 (0)8 6167 5201 www.epichem.com.au ABN 80 106 769 902