

1 **Sensitivity of SARS-CoV-2 antigen-detecting rapid tests for Omicron variant**

2 Meriem Bekliz¹, Francisco Perez-Rodriguez², Olha Puhach¹, Kenneth Adea¹, Stéfane
3 Marques Melancia², Stephanie Baggio^{3,4}, Anna-Rita Corvaglia¹, Frédérique
4 Jacquieroz-Bausch^{5,6,7}, Catia Alvarez¹, Manel Essaidi-Laziosi¹, Camille Escadafal⁸,
5 Laurent Kaiser^{2,5,9}, Isabella Eckerle^{1,5,9*}

6 ¹Department of Microbiology and Molecular Medicine, University of Geneva, Geneva,
7 Switzerland.

8 ²Laboratory of Virology, Division of Infectious Diseases and Division of Laboratory
9 Medicine, University Hospitals of Geneva & Faculty of Medicine, University of Geneva,
10 1205 Geneva, Switzerland.

11 ³Division of Prison Health, Geneva University Hospitals & University of Geneva, 1205
12 Geneva, Switzerland.

13 ⁴Institute of Primary Health Care (BIHAM), University of Bern, 3012 Bern, Switzerland.

14 ⁵Geneva Centre for Emerging Viral Diseases, University Hospitals Geneva, and
15 University of Geneva, Switzerland.

16 ⁶Division of Tropical and Humanitarian Medicine, Geneva University Hospitals,
17 Geneva, Switzerland

18 ⁷Primary Care Division, Geneva University Hospitals, Geneva, Switzerland

19 ⁸FIND, Geneva, Switzerland

20 ⁹Division of Infectious Diseases, Geneva University Hospitals, 1205 Geneva,
21 Switzerland.

22

23

24 *Corresponding author: Email: Isabella.Eckerle@hcuge.ch

25 **Keywords**

26 SARS-CoV-2; COVID19; Antigen-detecting rapid diagnostic tests; variants of concern;
27 Omicron variant

28 **Abstract**

29 **Background**

30 The emergence of each novel SARS-CoV-2 variants of concern (VOCs) requires
31 investigation of its potential impact on the performance of diagnostic tests in use,
32 including Antigen-detecting rapid diagnostic tests (Ag-RDT). Although anecdotal
33 reports have been circulating that the newly emerged Omicron variant is in principle
34 detectable by Ag-RDTs, few data on sensitivity are available.

35 **Methods**

36 We have performed 1) analytical sensitivity testing with cultured virus in eight Ag-RDTs
37 and 2) retrospective testing in duplicates with clinical samples from vaccinated
38 individuals with Omicron (n=18) or Delta (n=17) breakthrough infection on seven Ag-
39 RDTs.

40 **Findings**

41 Overall, we have found large heterogeneity between Ag-RDTs for detecting Omicron.
42 When using cultured virus, we observed a trend towards lower sensitivity for Omicron
43 detection compared to earlier circulating SARS-CoV-2 and the other VOCs. When
44 comparing performance for Delta and Omicron in a comparable set of clinical samples
45 in seven Ag-RDTs, 124/252 (49.2%) of all test performed showed a positive result for
46 Omicron compared to 156/238 (65.6%) for Delta samples. Sensitivity for both Omicron
47 and Delta between Ag-RDTs was highly variable. Four out of seven Ag-RDTs showed
48 significantly lower sensitivity ($p < 0.001$) to detect Omicron when compared to Delta
49 while three had comparable sensitivity to Delta.

50 **Interpretation**

51 Sensitivity for detecting Omicron is highly variable between Ag-RDTs, necessitating a
52 careful consideration when using these tests to guide infection prevention measures.
53 While analytical and retrospective testing may be a proxy and timely solution to
54 generate performance data, it is not a replacement for clinical evaluations which are
55 urgently needed. Biological and technical reasons for detection failure by some Ag-
56 RDTs need to be further investigated.

57 **Funding**

58 This work was supported by the Swiss National Science Foundation (grant numbers
59 196383, 196644 and 198412), the Fondation Ancrege Bienfaisance du Groupe Pictet,
60 the Fondation Privée des Hôpitaux Universitaires de Genève and FIND, the global
61 alliance for diagnostics.

62 **Introduction**

63 The emergence of each novel SARS-CoV-2 variants of concern (VOCs) requires
64 investigation of its potential impact on the performance of diagnostic tests in use.
65 SARS-CoV-2 antigen-detecting rapid diagnostic tests (Ag-RDT) offer quick, cheap and
66 laboratory-independent results at the point of care.¹ Although sensitivity is lower
67 compared to the gold standard method, RT-PCR, they enable reliable detection of
68 high viral load samples associated with infectious virus presence, making them
69 impactful public health tools.^{2,3} However, the majority of Ag-RDT validation studies
70 were performed prior to the emergence of SARS-CoV-2 variants of concern (VOC).⁴

71 The VOC Omicron was first reported at the end of November from South Africa and is
72 characterized by a high number of mutations compared to earlier circulating SARS-
73 CoV-2.⁵ The majority of mutations are located in the protein of the gene coding for the
74 Spike protein, and, according to preliminary data, are associated with considerable
75 escape from neutralization by both disease- and vaccine derived antibodies, and
76 probably also associated to lower vaccine effectiveness.^{6,7,8,9,10} Current
77 epidemiological data show that Omicron circulation is associated with a steep increase
78 in case numbers as well as an increased risk of reinfection.¹¹

79 Beyond the Spike mutations, Omicron also has also mutations in the nucleocapsid,
80 which is the target protein of almost all Ag-RDTs. Two mutations found in Omicron are
81 R203K and G204R that have been described already before Omicron in some SARS-
82 CoV-2 sequences. They were linked to increased sub-genomic RNA and increased
83 viral loads.¹²⁻¹⁴ In addition, a deletion (Del31-33) is found in the nucleocapsid of
84 Omicron, as well as another mutation P13L. No information on a potential impact of
85 these mutations on Ag-RDTs performance is available so far. Anecdotal reports
86 showed positive detection of Omicron-confirmed patient samples by Ag-RDTs but few
87 experimental data on Ag-RDT sensitivity for Omicron are available.

88 **Methods**

89 **Virus isolates**

90 All viruses were isolated from clinical samples. Isolates were grown in Vero-E6 cells
91 as described previously.¹⁵ The Omicron variant was initially isolated on Vero-TMPRSS
92 cells, then further passaged with a stock passage (p2) prepared on VeroE6. Vero
93 TMPRSS were kindly received from National Institute for Biological Standards and
94 Controls (NIBSC, Cat. Nr. 100978). The following mutations and deletion in the
95 nucleocapsid were present in the original patients' sequence as well as in the virus
96 isolate of the passage used in this study: R203K, G204R, P13L, Del31-33.

97 **Clinical specimens**

98 Nasopharyngeal swabs for diagnostics of SARS-CoV-2 by RT-PCR collected from
99 symptomatic individuals in the outpatient testing center of the Geneva University
100 Hospital were included in this study. Infection with SARS-CoV-2 was diagnosed by
101 RT-PCR assay (Cobas 6800, Roche). All samples originate from the diagnostic unit of
102 the virology laboratory of the hospital and were received for primary diagnosis of
103 SARS-CoV-2. Remaining samples were stored at -80°C, usually on the same day or
104 within 24h. All samples had one freeze-thaw cycle before inoculation on cell cultures
105 for infectious virus and for viral RNA quantification, for the majority of specimens the
106 Ag-RDT was performed at the same time. Due to logistical constraints, a subset of
107 specimens had one additional freeze-thaw cycle for Ag-RDT testing only. All
108 specimens were characterized by full genome sequencing for their infecting SARS-
109 CoV-2 variant.

110 **Viral load quantification**

111 Viral loads in each sample were determined by quantitative real-time reverse
112 transcription PCR (RT-qPCR) using SuperScript™ III Platinum™ One-Step qRT-PCR
113 Kit (Invitrogen) after thawing. RT-PCR for SARS-CoV-2 E gene and quantification of
114 genome copy number was performed as described previously.¹⁶ Presence of
115 infectious virus was determined by nucleocapsid staining for infectious foci in Vero
116 TMPRSS 24h after inoculation with the patient sample as described previously¹⁷.

117 **Ag-RDT performance**

118 The 8 commercially available Ag-RDT products used in the study are summarized in
119 **Table S1**.

120 *Analytical testing with cultured virus*

121 Each isolate has undergone serial dilutions at 1:2 in DMEM. For each variant, we
122 started the dilutions with the same virus concentration at 1.72E+04 PFU/mL. All Ag-
123 RDT assays were performed according to the manufacturers' instructions except that
124 viral dilutions were added to the buffer instead of a swab specimen. All dilutions used
125 for validation additionally were tested and quantified by RT-PCR assay for SARS-CoV-
126 2 RNA copy numbers/mL. For each serial dilution of each variant, 5 µl of dilution has
127 been applied to the proprietary buffer and then applied to the Ag-RDT using only
128 materials provided in the kit.

129 *Performance testing with clinical specimens*

130 For testing with clinical specimens, 5 µl of VTM of each specimen has been directly
131 added to the proprietary buffer, and then applied to the Ag-RDT in duplicates under

132 BSL3 conditions.¹⁸ Ag-RDT buffer without virus was used as a negative control. All
133 Ag-RDT assays were read visually in duplicate. All visible bands were considered as
134 a positive result. The entire study was performed under BSL-3 conditions.

135 **Statistics**

136 We first compared whether Log₁₀ SARS-CoV-2 copies, days post symptom onset, and
137 presence of infectious disease were significantly different between the Delta (n=18)
138 and Omicron (n=17) patients using simple linear and logistic regressions. We then
139 tested whether the overall sensitivities and discordances differed between Delta and
140 Omicron using proportion tests. Finally, we compared sensitivities for Delta (n=34) and
141 Omicron (n=36) tests separately for each Ag-RDT. To take into account that each
142 patient had two independent tests, we used mixed-effect logistic regressions with tests
143 nested into patients. Data were analysed using R4.1.2.

144 **Ethical approval**

145 Ethical approval for samples used in this study for virus isolation was waived by the
146 local ethics committee of the Geneva University Hospitals (HUG) that approves the
147 usage of anonymized leftover patient samples collected for diagnostic purposes in
148 accordance with our institutional and national regulations. The part of the study using
149 patient specimens linked to clinical data (retrospective testing) was approved by the
150 Cantonal ethics committee (CCER Nr. 2021-01488). For this part, all study participants
151 and/or their legal guardians provided informed consent.

152

153 **Results**

154 *Analytical testing with cultured SARS-CoV-2 isolates*

155 We have evaluated analytical sensitivity using cultured SARS-CoV-2 Omicron variant,
156 in comparison to previous data obtained on isolates of the other VOCs (Alpha, Beta,
157 Gamma and Delta) and an early-pandemic (pre-VOC) SARS-CoV-2 isolate (B.1.610)
158 in eight Ag-RDTs. Data on early pandemic SARS-CoV-2, Alpha, Beta, Gamma and
159 Delta have been published previously but were included here for comparison to
160 Omicron^{15,18}.

161 Eight Ag-RDTs were used: I) Panbio COVID-19 Ag Rapid test device (Abbott); II)
162 Standard Q COVID-19 Ag (SD Biosensor/Roche); III) Sure Status (Premier Medical
163 Corporation); IV) 2019-nCoV Antigen test (Wondfo); V) Beijing Tigsun Diagnostics Co.
164 Ltd (Tigsun); VI) Onsite COVID-19 Ag Rapid Test (CTK Biotech); VII) ACON biotech
165 (Flowflex) and VIII) NowCheck Covid-19 Ag test (Bionote). This list includes all three

166 Ag-RDTs on the WHO Emergency Use Listing (WHO-EUL) and the other tests that
167 are on the waiting list for WHO-EUL approval.

168 When assessing by infectious virus titers (PFU/mL) (**Fig 1A**), analytical sensitivity to
169 detect Omicron was lower than for the other VOCs in most of the tests evaluated. Two
170 tests showed a slightly higher sensitivity for Omicron than for Delta (Test V and VII),
171 but for these tests, both Delta and Omicron showed lower detection sensitivity than
172 the other VOCs and pre-VOC SARS-CoV-2. The same pattern of lowest sensitivity for
173 Omicron compared to the other VOCS was confirmed when assessing RNA copy
174 numbers (**Fig. 1B**). Significant heterogeneity was observed between different Ag-
175 RDTs to detect Omicron.

176 *Sensitivity testing in patient specimens*

177 In addition to this analytical work, we have tested seven Ag-RDTs with original patient
178 specimens as a retrospective sensitivity study with 35 nasopharyngeal specimens of
179 confirmed Omicron (n=18) or Delta (n=17) breakthrough infections in vaccinated
180 individuals during the first 5 days post-symptom onset. The two sample collections of
181 Omicron and Delta patients' specimens did not differ in RNA viral load, days post
182 symptom onset or specimens with infectious virus presence (**Table 1**).

183 Testing with clinical specimens was done in duplicates for each specimens using
184 seven Ag-RDTs to compare performance for Omicron and Delta infections (**Fig. 2**).
185 When assessing overall test positivity, for Omicron 124/252 (49.2%) of tests showed
186 a positive result compared to 156/238 (65.5%) ($z = -3.65$, $p < .001$). Of 126 test pairs,
187 14 showed a discordant result for Omicron vs. 7 in 119 test pairs performed for Delta
188 ($z = -1.46$, $p = .144$). When comparing sensitivity for Delta vs. Omicron for each Ag-
189 RDT, four Ag-RDTs showed significantly lower sensitivity ($p < 0.001$) while three tests
190 showed comparable performance (**Table 1 and Fig.3**). Sensitivity in our specimens
191 panel ranged between 22.2% and 88.9% for Omicron and 52.9% to 91.2% for Delta,
192 confirming the high variability of sensitivity between the different tests that was
193 observed in our testing. The three tests that performed equally well had sensitivities
194 between 47.2 and 91.2%.

195 **Discussion**

196 Newly emerging variants necessitate a rapid assessment of the performance of
197 diagnostic tests in use. Here we have performed a comprehensive laboratory-based
198 evaluation study of eight Ag-RDTs with cultured Omicron virus as well as a
199 retrospective clinical validation with 35 patient specimens.

200 Overall, we have observed a lower sensitivity to cultured virus across different Ag-
201 RDTs compared to earlier variants, suggesting that Omicron virus itself is detected
202 with lower sensitivity than other variants. We have observed differences between Ag-
203 RDTs from different manufacturers, but also between assessment for PFU and RNA
204 copy numbers. Reasons are most likely due to different ratios between infectious
205 particles and RNA copies among the different SARS-CoV-2 variants. Since the main
206 public health benefit of Ag-RDTs are the detection individuals with infectious virus
207 shedding and not just presence of viral RNA, assessment of infectious viral particles
208 is of higher relevance in this context, and an overall tendency towards lower sensitivity
209 was seen for both assessments. Of note, while in the analysis for infectious virus, the
210 previous VOCs Alpha, Beta, Gamma and Delta were mainly detected with comparable
211 or even higher sensitivity compared to pre-VOC SARS-CoV-2, and Omicron is the first
212 VOC demonstrating a trend towards lower analytical sensitivity across assays.

213 Omicron has additional mutations in the nucleocapsid that have been previously
214 observed in circulating SARS-CoV-2 before, although not largely present, in circulating
215 SARS-CoV-2 before but so far their impact on Ag-RDT performance is unknown. The
216 virus isolate used in our study carries all four of the known nucleocapsid mutations
217 (P13L, Del31-33, R203K, G204R), confirmed from both patient specimens and virus
218 isolate. Percentage of Omicron sequences with these mutations are 96.8% for P13L,
219 94.9% for Del31-33xx, 98.4 for R203K, and 98.4% for G204R of currently available
220 Omicron sequences¹⁹. As not all circulating Omicron lineages harbour all mutations,
221 additional analysis with such isolates would be of interest, however, at the time of
222 conducting the study, no such isolates were available. However, our isolate represents
223 the major circulating Omicron lineages.

224 In our clinical validation, we saw large heterogeneity between Ag-RDTs, with a loss
225 of sensitivity for four Ag-RDT specimens. Comparisons of diagnostic assay by using
226 different patient specimen collections are not trivial, and we have aimed for similar
227 characteristics for the main determinants for rapid test performance, which is viral load,
228 presence of infectious virus and time since days post symptom onset.^{20,21}
229 Furthermore, we had access to detailed clinical data, and all specimens were from
230 previously mRNA vaccinated individuals, followed by a Delta or Omicron breakthrough
231 infection. At least in most high-income countries with high vaccination rates, this group
232 of individuals is comprising the majority of Omicron infections observed, therefore our
233 results are of immediate public health interest.

234 Few data are available so far on Ag-RDT performance for Omicron case detection. A
235 small number of heterogeneous studies are available, but with little assessment for
236 sensitivity and with conflicting results. A recent report from the U.S. Food & Drug

237 Agency (FDA) announced that early data suggest reduced sensitivity for Omicron, in
238 line with our findings, although no primary data are given.²² A study performed by
239 Public Health England (PHE) with cultured isolated of Omicron and wild-type SARS-
240 CoV-2 across dilutions ranging from 12.5 to 1250 focus forming units/mL and 30.000
241 to 4.070.000 viral copy numbers did not find a loss in sensitivity for five Ag-RDTs²³.
242 Only one of the Ag-RDTs validated here, the Flowflex Ag-RDT, was also validated in
243 our study. In our analytical testing, reduced sensitivity was seen for Omicron compared
244 to wild-type SARS-CoV-2 in this test, but we did not see a difference in the clinical
245 testing when compared to Delta. Overall, in both our assessments, this was the most
246 sensitive Ag-RDT for most variants including Omicron. Another study used two nasal
247 swab samples each from Omicron and Delta-infected individuals and validated the
248 Abbott Binax Now Ag-RDT, a test that was not included in our study²⁴ They conclude
249 that Omicron can be detected by this test, although no extensive validation for
250 sensitivity was performed. For the same test, data from a single clinical validation
251 study are available from an outpatient testing Centre in the US using nasal swabs.²⁵
252 Sensitivity of a single antigen test was 95.2% for individuals with a cycle threshold
253 value of the RT-PCR < 30, indicating good sensitivity with high viral load. A high failure
254 rate was observed when oral specimens (cheek swabs) were used.

255 Strength of our study is that we have validated eight and seven Ag-RDT side-by-side
256 for analytical and retrospective clinical sensitivity, respectively. Our selection of Ag-
257 RDTs cover all of the three Ag-RDTs on the WHO-EUL, and three others that are on
258 the WHO-EUL waiting list for approval, thus of high global public health relevance.^{26,27}
259 If the lower sensitivity towards Omicron that we observed here is confirmed by findings
260 from clinical validations at the point of care, the use of Ag-RDTs in the early
261 symptomatic period of an Omicron infection or in asymptomatic patients could be less
262 reliable, with possibly important implications for public health measures. However, all
263 Ag-RDTs were able to detect Omicron infections and so far, there is no reason to
264 change advice on how to implement RDTs to support testing and COVID response
265 strategies. As our evaluation here was rather focused at the lower end of detection,
266 results might be of higher relevance to testing in an asymptomatic population or in the
267 very early infection phase, but not necessarily to the acute symptomatic infection
268 phase when peak viral loads are reached.

269 Our study has several limitations. For cultured virus, the ratio between infectious virus,
270 viral protein and RNA copies might differ considerably to original human specimens.
271 The retrospective testing is done with only a low number of patients swab samples
272 that have been submerged in viral transport medium, whereas the recommended
273 sample type for Ag-RDT use is fresh swabs. This has introduced an extra dilution
274 factor as well as an additional freeze/thaw cycle. Although we tried to reduce the

275 number of freeze-thaw cycles to a minimum, we cannot exclude loss of RNA, protein
276 or infectious virus, thus not reflecting fully the characteristics of a fresh patient
277 specimen. To correct for loss of RNA after the first freeze-thaw cycle, we have re-
278 tested viral RNA loads by RT-PCR and have used these values for comparison.
279 Another limitation is that to compare across assays we have used the same approach
280 as we did for analytical testing, with only 5 μ L of the original patient VTM added to the
281 buffer of each kit to be able to use the same specimens for testing with a high number
282 of tests in parallel. The volume of viral transport medium added to the buffer was lower
283 than what was recommended by some manufacturers, and for some Ag-RDTs there
284 was no recommendation on the use of swab samples in VTM. Therefore, viral loads
285 of the original sample and sensitivities observed in our sample collection cannot be
286 compared to results obtained from clinical validations performed on fresh samples and
287 our results should be interpreted as a comparison between Ag-RDTs and not as
288 sensitivity thresholds for absolute viral loads and/or presence of infectious virus.
289 Rather, we have investigated the lower end of sensitivity in the Ag-RDTs tested.
290 Therefore, a reduced sensitivity in some tests, but not complete failure to detect
291 Omicron could be of higher relevance in the beginning of the infection, when viral loads
292 are still on the rise, and of less relevance once peak viral loads are reached.

293 Lower sensitivity observed in this study could be due to a variant-specific impact on
294 Ag-RDT performance. However, since many Omicron infections are currently
295 observed in vaccinated individuals, it remains unclear if virus shedding and test
296 performance differs between unvaccinated and vaccinated individuals, and no studies
297 are available investigating Ag-RDT performance in unvaccinated vs. vaccinated
298 individuals are available yet. To date, most validation studies of Ag-RDTs were done
299 in the first year of the pandemic, before circulation of VOCs and in mostly immune-
300 naïve individuals experiencing their primary SARS-CoV-2 infection. Other factors,
301 such as *in vivo* shedding of infectious virus and overall viral can be one reason for
302 differences in test performance. However, we have shown recently that neither RNA
303 viral loads nor infectious titers differ significantly between Omicron and Delta
304 breakthrough infections, thus differences in viral load are unlikely the reason for lower
305 sensitivity in Omicron in some tests.¹⁷

306 Importantly, while analytical and retrospective testing may be a proxy for clinical
307 sensitivity, is not a replacement for clinical evaluations at the point of care. The
308 discrepancies in our results between testing with cultured virus and retrospective
309 patient samples highlights the need for proper clinical studies in well-defined patient
310 cohorts. Therefore, further studies on diagnostic accuracy of Ag-RDTs performed at
311 the point of care for the newly emerged VOC Omicron are urgently needed to guide
312 public health responses.

313 **Funding**

314 This work was supported by the Swiss National Science Foundation (grant number
315 196383), the Fondation Ancrege Bienfaisance du Groupe Pictet, and FIND, the global
316 alliance for diagnostics. The Swiss National Science Foundation and the Fondation
317 Ancrege Bienfaisance du Groupe Pictet had no role in data collection, analysis, or
318 interpretation. Antigen rapid diagnostic tests were provided by FIND and FIND was
319 involved in methodology, data analysis and interpretation. CE is an employee of FIND.

320

321 **Acknowledgments**

322 We thank the patients for participating in our study. We thank Pauline Vetter for help
323 with clinical data. We thank Silvio Steiner, Jenna Kelly and Volker Thiel for sequencing
324 of the Omicron isolate.

325

326 **Conflicts of Interest**

327 The authors declare no competing interests.

328 References

- 329 1. Nordgren J, Sharma S, Olsson H, et al. SARS-CoV-2 rapid antigen test: High sensitivity to detect
330 infectious virus. *J Clin Virol* 2021; **140**: 104846.
- 331 2. World Health Organization (WHO) Antigen-Detection in the Diagnosis of SARS-CoV-2 Infection
332 Using Rapid Immunoassays. [(accessed on 28 April 2021)]; Available online:
333 [https://www.who.int/publications/i/item/antigen-detection-in-the-diagnosis-of-sars-cov-](https://www.who.int/publications/i/item/antigen-detection-in-the-diagnosis-of-sars-cov-2infection-using-rapid-immunoassays)
334 [2infection-using-rapid-immunoassays](https://www.who.int/publications/i/item/antigen-detection-in-the-diagnosis-of-sars-cov-2infection-using-rapid-immunoassays).
- 335 3. Mina MJ, Parker R, Larremore DB. Rethinking Covid-19 Test Sensitivity - A Strategy for
336 Containment. *N Engl J Med* 2020; **383**(22): e120.
- 337 4. World Health Organization (WHO) Weekly epidemiological update on COVID-19.
338 [https://www.who.int/publications/m/item/weekly-epidemiological-update-on-covid-19---](https://www.who.int/publications/m/item/weekly-epidemiological-update-on-covid-19---10-august-2021)
339 10-august-2021 Date: August, 10 2021 Date.
- 340 5. World Health Organization (WHO). [https://www.who.int/en/activities/tracking-SARS-CoV-2-](https://www.who.int/en/activities/tracking-SARS-CoV-2-variants/)
341 [variants/](https://www.who.int/en/activities/tracking-SARS-CoV-2-variants/) (accessed 08.12.2021).
- 342 6. Wilhelm A, Widera M, Grikscheit K, et al. Reduced Neutralization of SARS-CoV-2 Omicron
343 Variant by Vaccine Sera and monoclonal antibodies. *medRxiv* 2021: 2021.12.07.21267432.
- 344 7. Cele S, Jackson L, Khan K, et al. SARS-CoV-2 Omicron has extensive but incomplete escape of
345 Pfizer BNT162b2 elicited neutralization and requires ACE2 for infection. *medRxiv* 2021:
346 2021.12.08.21267417.
- 347 8. Rössler A, Riepler L, Bante D, Laer Dv, Kimpel J. SARS-CoV-2 B.1.1.529 variant (Omicron)
348 evades neutralization by sera from vaccinated and convalescent individuals. *medRxiv* 2021:
349 2021.12.08.21267491.
- 350 9. Dejnirattisai W, Shaw RH, Supasa P, et al. Reduced neutralisation of SARS-COV-2 Omicron-
351 B.1.1.529 variant by post-immunisation serum. *medRxiv* 2021: 2021.12.10.21267534.
- 352 10. Gardner BJ, Kilpatrick AM. Estimates of reduced vaccine effectiveness against hospitalization,
353 infection, transmission and symptomatic disease of a new SARS-CoV-2 variant, Omicron
354 (B.1.1.529), using neutralizing antibody titers. *medRxiv* 2021: 2021.12.10.21267594.
- 355 11. Pulliam JRC, van Schalkwyk C, Govender N, et al. Increased risk of SARS-CoV-2 reinfection
356 associated with emergence of the Omicron variant in South Africa. *medRxiv* 2021:
357 2021.11.11.21266068.
- 358 12. <https://covariants.org/per-country> (accessed 09.12.2021).
- 359 13. Leary S, Gaudieri S, Parker MD, et al. Generation of a novel SARS-CoV-2 sub-genomic RNA due
360 to the R203K/G204R variant in nucleocapsid. *bioRxiv* 2021: 2020.04.10.029454.
- 361 14. Mourier T, Shuaib M, Hala S, et al. Saudi Arabian SARS-CoV-2 genomes implicate a mutant
362 Nucleocapsid protein in modulating host interactions and increased viral load in COVID-19
363 patients. *medRxiv* 2021: 2021.05.06.21256706.
- 364 15. Bekliz M, Adea K, Essaidi-Laziosi M, et al. SARS-CoV-2 antigen-detecting rapid tests for the
365 delta variant. *Lancet Microbe* 2021.
- 366 16. Corman VM, Landt O, Kaiser M, et al. Detection of 2019 novel coronavirus (2019-nCoV) by
367 real-time RT-PCR. *Euro Surveill* 2020; **25**(3).
- 368 17. Puhach O, Adea K, Hulo N, et al. Infectious viral load in unvaccinated and vaccinated patients
369 infected with SARS-CoV-2 WT, Delta and Omicron. *medRxiv* 2022: 2022.01.10.22269010.
- 370 18. Bekliz M, Adea K, Essaidi-Laziosi M, et al. SARS-CoV-2 rapid diagnostic tests for emerging
371 variants. *Lancet Microbe* 2021; **2**(8): e351.
- 372 19. Outbreak.info. SARS-CoV-2 (hCoV-19) Mutation Reports: Mutation prevalence across
373 lineages. 2022. [https://outbreak.info/compare-](https://outbreak.info/compare-lineages?pango=Delta&pango=Omicron&pango=Alpha&pango=Beta&pango=Gamma&pango=Zeta&gene=N&threshold=70&nthresh=1&sub=false&dark=true)
374 [lineages?pango=Delta&pango=Omicron&pango=Alpha&pango=Beta&pango=Gamma&pang](https://outbreak.info/compare-lineages?pango=Delta&pango=Omicron&pango=Alpha&pango=Beta&pango=Gamma&pango=Zeta&gene=N&threshold=70&nthresh=1&sub=false&dark=true)
375 [o=Zeta&gene=N&threshold=70&nthresh=1&sub=false&dark=true](https://outbreak.info/compare-lineages?pango=Delta&pango=Omicron&pango=Alpha&pango=Beta&pango=Gamma&pango=Zeta&gene=N&threshold=70&nthresh=1&sub=false&dark=true) (accessed 13.01.2022).

- 376 20. Berger A, Nsoga MTN, Perez-Rodriguez FJ, et al. Diagnostic accuracy of two commercial SARS-
377 CoV-2 antigen-detecting rapid tests at the point of care in community-based testing centers.
378 *PLoS One* 2021; **16**(3): e0248921.
- 379 21. Ngo Nsoga MT, Kronig I, Perez Rodriguez FJ, et al. Diagnostic accuracy of Panbio rapid antigen
380 tests on oropharyngeal swabs for detection of SARS-CoV-2. *PLoS One* 2021; **16**(6): e0253321.
- 381 22. Agency USFD. SARS-CoV-2 Viral Mutations: Impact on COVID-19 Tests. 12/28/2021 2021.
382 [https://www.fda.gov/medical-devices/coronavirus-covid-19-and-medical-devices/sars-cov-](https://www.fda.gov/medical-devices/coronavirus-covid-19-and-medical-devices/sars-cov-2-viral-mutations-impact-covid-19-tests#omicronvariantimpact)
383 [2-viral-mutations-impact-covid-19-tests#omicronvariantimpact](https://www.fda.gov/medical-devices/coronavirus-covid-19-and-medical-devices/sars-cov-2-viral-mutations-impact-covid-19-tests#omicronvariantimpact) (accessed 13.01.2022).
- 384 23. Agency UHS. SARS-CoV-2 variants of concern and variants under investigation in England,
385 2021.
- 386 24. Regan J, Flynn JP, Choudhary MC, et al. Detection of the omicron variant virus with the Abbott
387 BinaxNow SARS-CoV-2 Rapid Antigen Assay. *medRxiv* 2021: 2021.12.22.21268219.
- 388 25. Schrom J, Marquez C, Pilarowski G, et al. Direct Comparison of SARS CoV-2 Nasal RT- PCR and
389 Rapid Antigen Test (BinaxNOW(TM)) at a Community Testing Site During an Omicron Surge.
390 *medRxiv* 2022: 2022.01.08.22268954.
- 391 26. World Health Organization (WHO). 2021.
392 [https://extranet.who.int/pqweb/sites/default/files/documents/211125_EUL_SARS-CoV-](https://extranet.who.int/pqweb/sites/default/files/documents/211125_EUL_SARS-CoV-2_products_list.pdf)
393 [2_products_list.pdf](https://extranet.who.int/pqweb/sites/default/files/documents/211125_EUL_SARS-CoV-2_products_list.pdf).
- 394 27. FIND. 2021. <https://www.finddx.org/sarscov2-eval-antigen/> (accessed 17.12.2021).

395

396 **Tables**

	Omicron (n=18)	Delta (n=17)	p ¹
Log ₁₀ SARS-CoV-2 copies, mean (SD)	7.9 (0.7)	8.0 (0.7)	.510
DPOS, mean (SD)	2.0 (1.2)	1.9 (1.3)	.892
Presence of infectious virus, n (%)	14/18 (77.8%)	14/17 (82.4%)	.613


397 **Table 1.** Characteristics of clinical specimens. ¹p-values for simple linear regressions
398 (Log₁₀ SARS-CoV-2 copies, DPOS) and simple logistic regression (Presence of
399 infectious virus) are reported.

400

	Sensitivity (%)		p ¹
	Delta (n=34)	Omicron (n=36)	
Panbio	67.7	36.1	<.001
Standard Q	52.9	22.2	<.001
Sure Status	52.9	27.8	<.001
Onsite	64.7	47.2	<.001
Wondfo	76.5	75.0	.984
Tigsun	52.9	47.2	.634
Flowflex	91.2	88.9	.918

401 **Table 2.** Detailed sensitivity for the seven Ag-RDTs tested with clinical samples. ¹ p-
402 values for logistic mixed-effect models (with tests nested into patients) are reported.


403 **Figures**

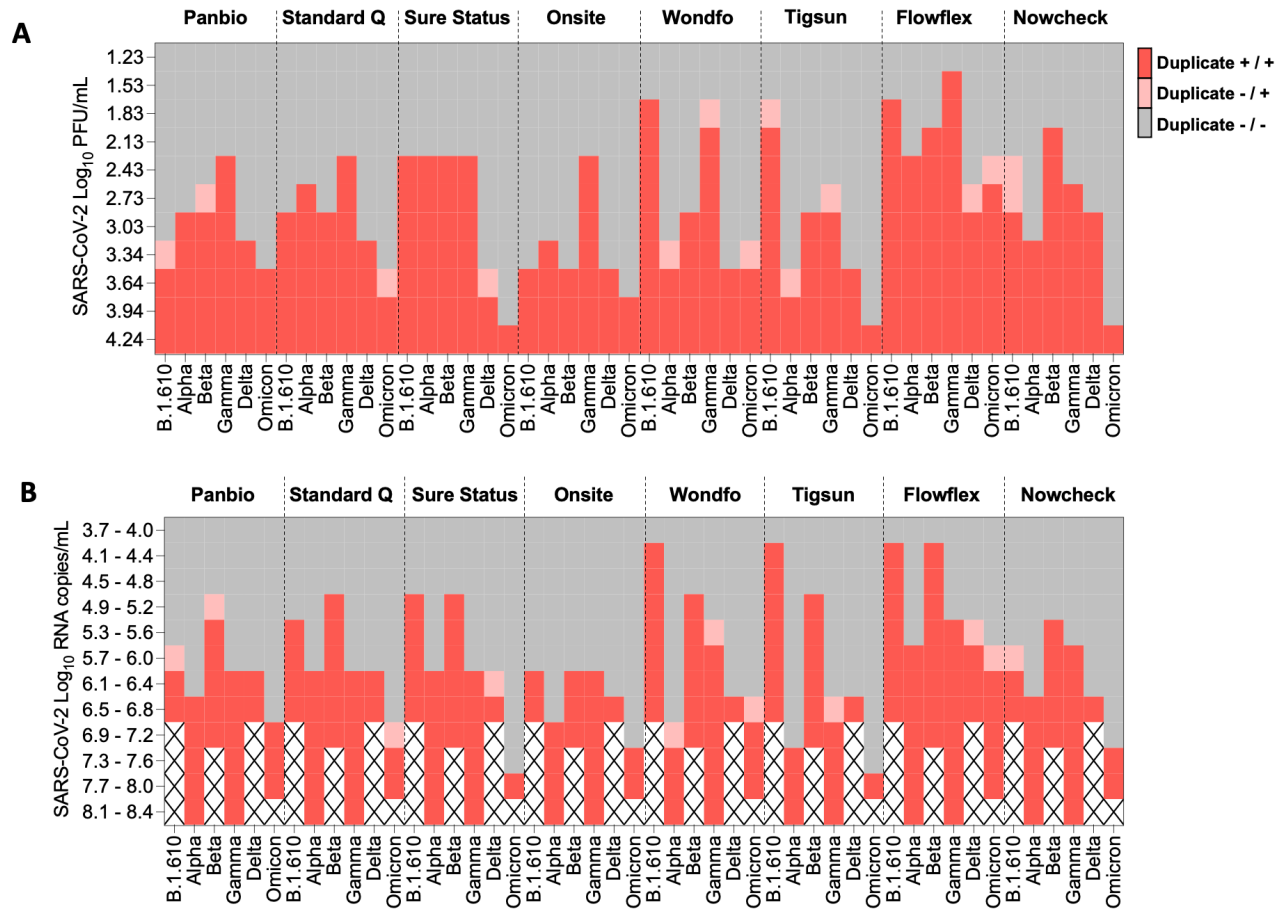

404

405 **Figure 1.** Heatmap based on Log₁₀ PFU/mL (**Fig 1A**) and on RNA viral load ranges
 406 (**Fig 1B**) for analytical sensitivity of eight Ag-RDTs assays with an early-pandemic
 407 SARS-CoV-2 isolate (B.1.610), the VOCs Alpha, Beta, Gamma and Delta in
 408 comparison Omicron.


409 Note: Analytical sensitivity for early-pandemic SARS-CoV-2 B.1.610, Alpha, Beta,
 410 Gamma and Delta have already been published before but were added here for
 411 consistency reasons and better interpretability of the data on Omicron.^{15,16}

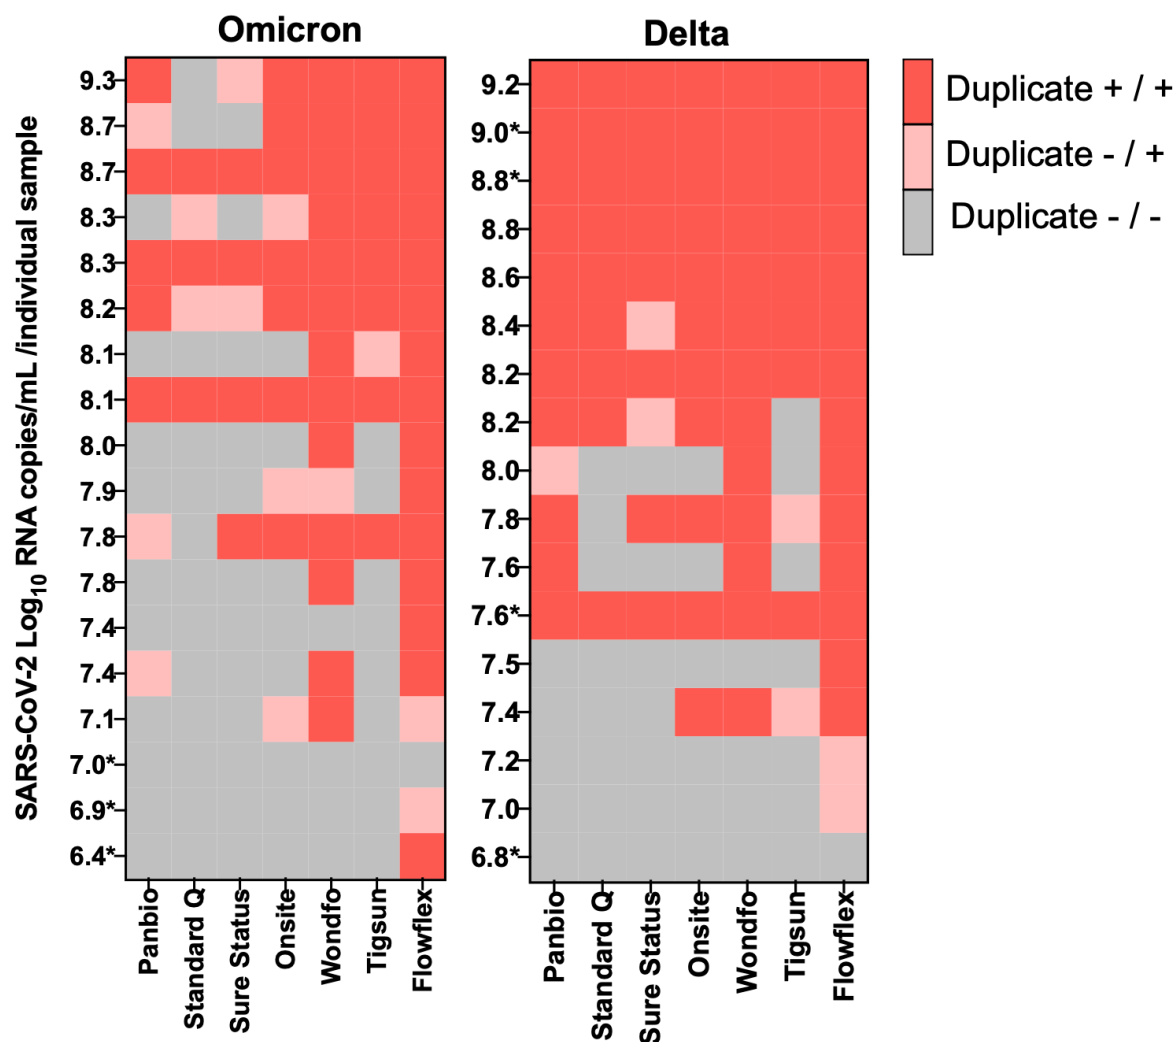

412

413 **Figure 2.** Heatmap of retrospective testing of original nasopharyngeal patient swab
 414 specimens from Omicron (n=18) and Delta (n=17) breakthrough infections in seven
 415 Ag-RDT assays per SARS-CoV-2 log₁₀ RNA copies/mL, performed in duplicates.
 416 Infectious virus was detected from all patient specimens unless marked with * (* = no
 417 infectious virus isolated).

418

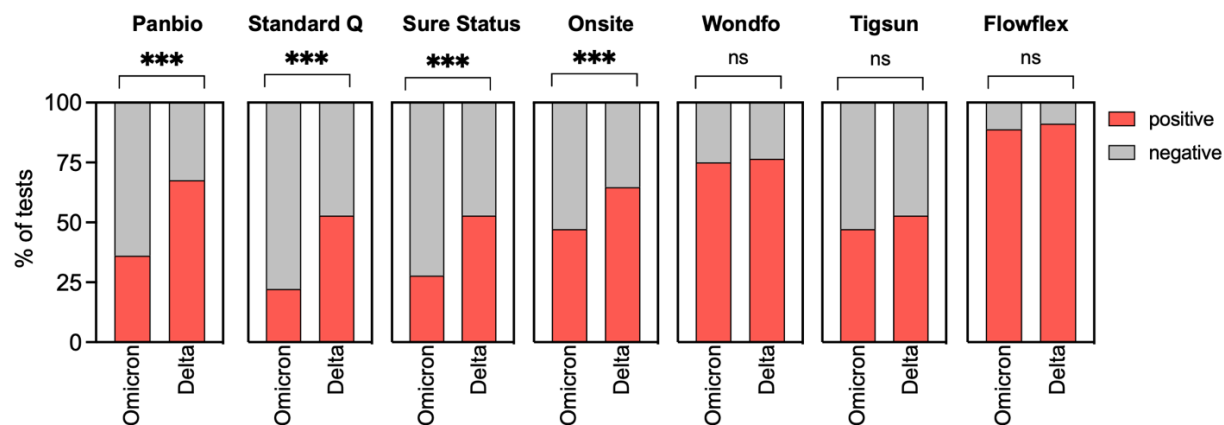

419

420 **Figure 3.** Percentage of positive/negative results for Omicron and Delta vaccine
421 breakthrough infections per number of tests performed (Omicron n=36, Delta n=34).
422 *** p<0.001, n.s., non-significant.

423

424 **Supplementary material**

425 **Tables**

426 **Table S1.** Overview of Ag-RDTs kits evaluated in the study.

427

	Name of kit	Manufacturer	Target protein
I	Panbio, COVID-19 Ag Rapid test device	Abbott	Nucleocapsid
II	Standard Q COVID-19 Ag	SD BIOSENSOR (Roche)	Nucleocapsid
III	Sure Status	Premier Medical Corporation	Nucleocapsid
IV	2019-nCoV Antigen test	Wondfo	Nucleocapsid
V	Beijing Tigsun Diagnostics Co. Ltd	Tigsun	Nucleocapsid
VI	CTK biotech	Onsite	Nucleocapsid
VII	ACON biotech	Flowflex	Nucleocapsid
VIII	NowCheck Covid- 19 Ag test	Bionote	Nucleocapsid

428