



Certificate of Analysis

Disposable Syringe Filters

Product Item : PVDF013N045I


Page : 1/1

Lot No. : 0621C16A3

Date : 2016/09/22

Sampling : Samples pulled at defined intervals throughout the lot, 10 units per lot

Test	Specification	Results
Bubble point test	>1.5bar	Conform
Hold-up volume	<25ul	Conform
HPLC Extractables	<0.004 Absorbance units	Conform
Dimensional Conformity of Luer Fittings	Withstands gauge tolerances in accordance with ISO594-1	Conform
Housing Burst Test	Burst pressure of ≥ 150 psi	Conform

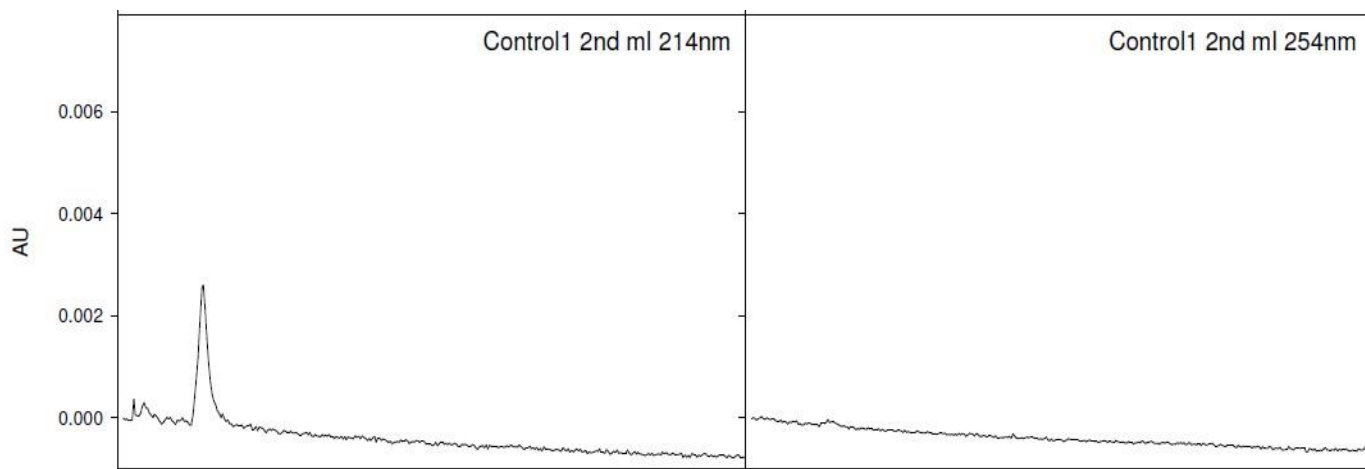

The information is based on our present state of knowledge and is intended to provide general notes on our products on their use. It should therefore not be constructed as guaranteeing specific properties of the products described or their suitability for a particular application. Any existing industrial property rights must be observed. The quality of our products guaranteed under our General Condition of Sale.