Clinical Line

Biosafety Dental Bleaching Dentistry and Prosthodontics Endodontics





Exacto

Glass fiber intraradicular conical post



Support of restorations and prosthetic crowns.

PRESENTATIONS

PRESENTATIONS	
911	Opaque - Package with 5 posts Nº 1 and 1 bur Nº 1
912	Opaque - Package with 5 posts Nº 2 and 1 bur Nº 2
913	Opaque - Package with 5 posts Nº 3 and 1 bur Nº 3
914	Opaque - Package with 15 posts (5 of each Nº 1, Nº 2
	and Nº 3) and 3 burs (1 of each Nº 1, Nº 2 and Nº 3)
915	Opaque - Package with 5 posts Nº 1
916	Opaque - Package with 5 posts Nº 2
917	Opaque - Package with 5 posts Nº 3
9087	Translucent - Package with 5 posts Nº 0.5 and 1 bur Nº 0.5
9117	Translucent - Package with 5 posts Nº 1 and 1 bur Nº 1
9127	Translucent - Package with 5 posts Nº 2 and 1 bur Nº 2
9137	Translucent - Package with 5 posts Nº 3 and 1 bur Nº 3
9147	Translucent - Package with 15 posts (5 of each Nº 1,
	Nº 2 and Nº 3) and 3 burs (1 of each Nº 1, Nº 2 and Nº 3)
9097	Translucent - Package with 5 posts Nº 0.5
9157	Translucent - Package with 5 posts Nº 1
9167	Translucent - Package with 5 posts Nº 2
9177	Translucent - Package with 5 posts Nº 3

Reforpost® Metallic I

Stainless steel intraradicular posts



Support of restorations and prosthetic crowns

PRESENTATIONS

Γ	749	Mini Kit I - Package with 20 units (5 units of each post
		size), 1 size 2 Largo bur, radiographic guide and post key
Γ	751	Refill 1 - Package with 5 units of size 1 post
Γ	752	Refill 2 - Package with 5 units of size 2 post
Γ	753	Refill 3 - Package with 5 units of size 3 post
Γ	754	Refill 4 - Package with 5 units of size 4 post
Г	759	Package with 1 Post key

Reforpost[®] Glass Fiber and Carbon Fiber

Glass fiber and carbon fiber parallel intraradicular post with conical tip



Retentive shape

Support of restorations and prosthetic

PRESENTATIONS

PRESENTATIONS		
711	Carbon - Refill 1 - Package with 5 posts nº 1	
712	Carbon - Refill 2 - Package with 5 posts nº 2	
713	Carbon - Refill 3 - Package with 5 posts nº 3	
720	Glass - Kit - Package with 30 posts (10 nº 1, 10 nº 2 and	
	10 nº 3), 3 Peeso (Largo) drills (1 nº 3, 1 nº 4 and 1 nº 5)	
	and 1 radiographic guide	
721	Glass - Refill 1 - Package with 5 posts nº 1	
722	Glass - Refill 2 - Package with 5 posts nº 2	
723	Glass - Refill 3 - Package with 5 posts nº 3	
724	Glass - Mini kit - Package with 15 posts (5 nº 1, 5 nº 2	
	and 5 nº 3) and 1 radiographic guide	
726	Glass - Refill 1 - Package with 10 posts nº 1	
727	Glass - Refill 2 - Package with 10 posts nº 2	
728	Glass - Refill 3 - Package with 10 posts nº 3	

Gates Drill

Endodontic access burs

BROCA DE CATES Angelos 1 mm NTI-D2211

INDICATION

 Preparation of the middle third and cervical of canals and consequential compensatory abrasion; pulpectomy and disobturation of root canals
 PRESENTATIONS

RESENTATIONS

1962	nº 1 - 32 mm - Package with 1 unit
1964	nº 2 - 32 mm - Package with 1 unit
1966	nº 3 - 32 mm - Package with 1 unit
1968	nº 4 - 32 mm - Package with 1 unit
1970	nº 5 - 32 mm - Package with 1 unit
1972	nº 6 - 32 mm - Package with 1 unit

Reforpin®





Post/core construction in one session

INDICATION

Construction of prefabricated core build-up with prefabricated posts

PRESENTATIONS

934	Mini Kit Anterior - Package with 9 anterior
	cores (3P, 3M, 3G)
935	Mini Kit Premolar - Package with 9 premolar
	cores (3P, 3M, 3G)

Peeso Drill



INDICATION

Intraradicular procedures

Resistance and Longevity

PRESENTATIONS		
162	nº 1 - Package with 1 unit	
164	nº 2 - Package with 1 unit	
166	nº 3 - Package with 1 unit	
168	nº 4 - Package with 1 unit	
170	nº 5 - Package with 1 unit	
172	nº 6 - Package with 1 unit	



INDICATION

· For root canal filling

PRESENTATION

826 Tubes (30 g) - Package with 1 tube of base paste (12 g), 1 tube of catalyst paste (18 g) and 1 mixing pad Syringe (4 g) - Package with 1 syringe (4 g), 15 automixing tips and 1 mixing pad Tubes (12 g) - Package with 1 tube of base paste (7,2 g), 1 tube of catalyst paste (4,8 g) and 1 mixing pad 8288

MTA Angelus[®]

Bioceramic reparative cement



- 820
 Package with 1 g of Gray MTA Angelus, 3 ml of distilled water and 1 scoop

 821
 Package with 2 g of Gray MTA Angelus, 3 ml of distilled water and 1 scoop

 822
 Package with 1 g of White MTA Angelus, 3 ml of distilled water and 1 scoop
- 824 Package with 2 applications of 0.28 g each White MTA Angelus , 3 ml of distilled water and 1 scoop

Intrument to apply MTA

MTA Repair HP

Bioceramic high-plasticity reparative cement The same efficiency with better plasticity INDICATIONS • Treatment of iatrogenic or decay-related perforation (root and furcation) · Treatment of root perforation associated with internal resorption · Surgical treatment of root perforation · Parendodontic surgery with retrofilling (Apicoectomy)

- Direct pulp capping
- Pulpotomy
- Apexigenesis
- Apexification

PRESENTATION

843 Package with 2 powder capsules with 0.085 grams each and 2 flasks Package with 5 powder capsules with 0.085 grams each and 5 flasks 8469 Package with 10 powder capsules with 0.085 grams each and 10 flasks


Merely illustrative images.


PRESENTATIONS

Design and

lightness

INDICATION

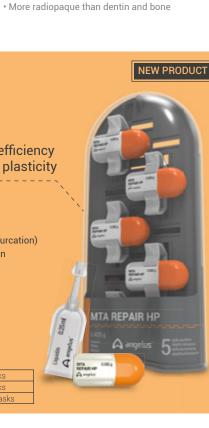

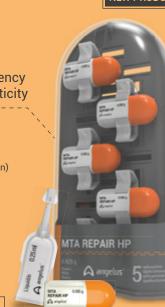



• To apply mixed MTA and other materials as Ca(OH), in various cavities

155Package with 1 unit (medium)156Package with 1 unit (small)

Angelus[®] Östby Rubber Dam Frame

Frame for absolute isolation



Autoclavable

INDICATION • Rubber dam sheet support PRESENTATION 350 Package with 1 unit

Endodontic Ruler

Endodontic ruler (Gauge in millimeters)



INDICATION • Measurements in endodontic procedures PRESENTATION 850 Package with 1 unit

Endodontic Files Angelus®

Manual endodontic files



High resistance to fractures

INDICATION

• Biomechanical preparation (instruments) of the root canals

PRESENTATIONS

Files Tipe K 1st and 2nd series (consult)
 Limas Hedstroen 1st and 2nd series (consult)

Endo Dam


Light-curable resin for absolute isolation sealing





INDICATION • Absolute isolation sealing PRESENTATION 1215 Package with 1 syringe (2g) + 03 tips

Intermedium Calibrating ruler for gutta-percha points



INDICATION
Calibration of gutta-percha points and preparation of intermediate size points
PRESENTATION
854 Package with 1 unit

Endometric Support for endodontic files



INDICATION

Support of endodontic files.

PRESENTATIONS

800Package with 1 container and 30 units of fabric support802Package with 50 units of fabric support (refill)

Amarrilho Ligatures for rubber dam isolation




Ideal sealing for the isolation

INDICATION • Sealing of the rubber dam in dental procedures under absolute isolation PRESENTATION

370 Package with 24 units (12 anterior and 12 posterior)

Stop fabricated with silicone



INDICATION • Working length indication in files during endodontic procedures


PRESENTATIONS

7001.5 mm - Package with 100 units7011.0 mm - Package with 100 units





Merely illustrative images.

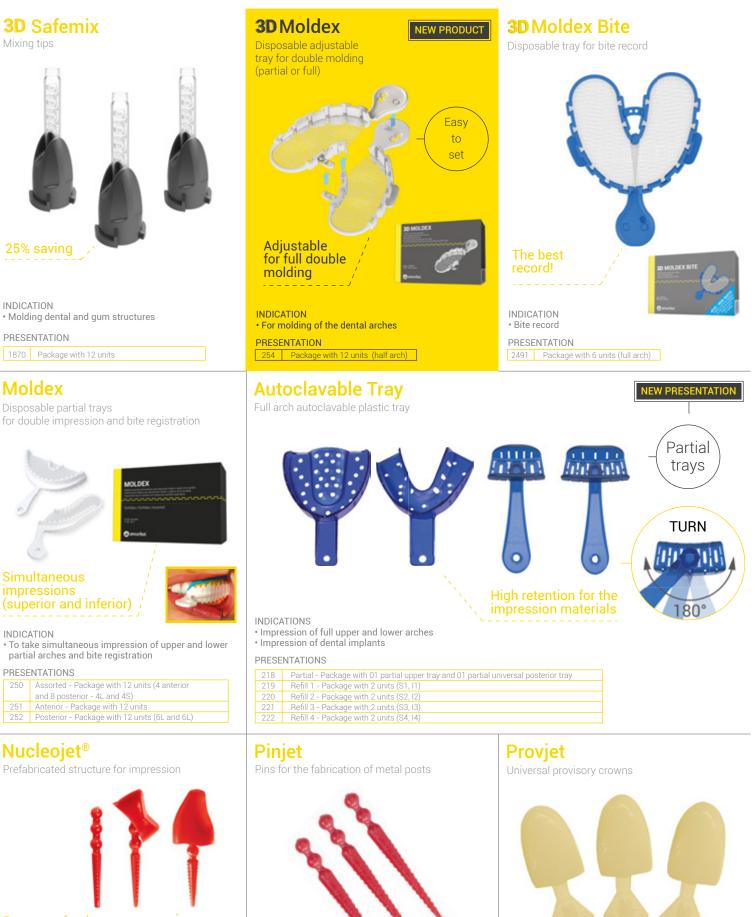

Posts confection in 15 minuts

INDICATION • Fabrication of metal posts (technique of root canal impression)

PRESENTATIONS

 PRESENTATIONS

 100
 Assorted - Package with 17 units - 10 pin and core - anteriors (2S, 4M, 4L) and 7 premolars (2S, 2M, 3L), 2 extra units of pins

 101
 Anterior - Package with 17 pin and core (5P, 8M, 4G)

 102
 Premolar - Package with 17 pin and core (5P, 8M, 4G)

 103
 Pins - Package with 30 units (without core)

INDICATION • Fabrication of metal posts directly and indirectly PRESENTATION 500 Package with 50 units

Chemical adhesion

to acrylic resin

INDICATION • Fabrication of temporary





6 lateral incisors (2S, 2M, 2L)

Proovisory crowns

Contacto Paper and Arch

Articulating paper



INDICATION

· Registration of occlusal contacts in adjustment procedures of restorations, prostheses and dental surfaces

PRESENTATIONS

552Arch - Package with 12 units560Paper - Package with 12 units

Silano

Adhesion promoter for porcelain (ceramic) and glass fiber



SILANO 5 ml ۵a

INDICATIONS

- Treatment of internal surfaces of porcelain restorations and glass fiber posts before cementation
- with resin cements · Treatment of porcelain surfaces before repair
- with composite resin Treatment of porcelain surfaces before bonding of porcelain

PRESENTATION

479 Package with 1 bottle (5 ml)

Fusion-Duralink® Phosphoric Acid

37% Phosphoric Acid (H_2PO_4)

Total etching



INDICATION

· Etching of dental surfaces (dentin and enamel) to improve the adhesion of materials in direct and indirect restorations and pit and fissure sealing and for the bonding of orthodontic brackets

PRESENTATION

6050 Package with 3 syringes (3 g each)

Merely illustrative images



Package with 140 units

Package with 280 units

More safety in adhesion of resin to ceramic

Conditioning of metal free restorations fabricated

with porcelain (ceramic) before cementation with resin

· Conditioning of porcelain fragments before bonding

Porcelain

10% Hydrofluoridric Acid

Etchant

INDICATIONS

PRESENTATION

Bonding System

and light

INDICATION

PRESENTATIONS

602

604

or repair with composite resin

952 Package with 1 syringe (2.5 g)

Fusion-Duralink®

· For direct restorations with composite resin Adhesive cementation of prefabricated posts (metal and fiber), cast metal posts and indirect restorations (metal, porcelain and composite resin)

Catalyst - Package with bottle (2 ml)

Adhesive - Package with 1 bottle (4 ml) Primer - Package with 1 bottle (4 ml)

Kit - Package with 1 bottle of Primer (4 ml), 1 bottle of

Adhesive (4 ml) and 1 bottle of Catalyst (2 ml)

Bonding of orthodontic brackets

• Technique of adhesive amalgam

The second se New format:





VO FORMATO

RETENTIV

METALPIN

۵

INDICATION

Alta

opacidade

 Masking of dark and stained teeth, metal surfaces and carbon fiber posts

PRESENTATIONS
 493
 B 0.5 - Package with 1 syringe (1.5 g)

 494
 A 3 - Package with 1 syringe (1.5 g)

Aplik

Micro applicators for dental use



Versatility for the application


INDICATION

- · Application of acids, primers and adhesives on the tooth, prior to restorations
- · Application of acid and silane in prostheses,
- Regular (green) Package with 100 units Fine (blue) Package with 100 units
- 124
- prior to cementation PRESENTATIONS
 - - Extrafine (white) Package with 100 units

Interlig®

570 | Package with 30 units

Braided glass fiber impregnated with light-cured composite resin

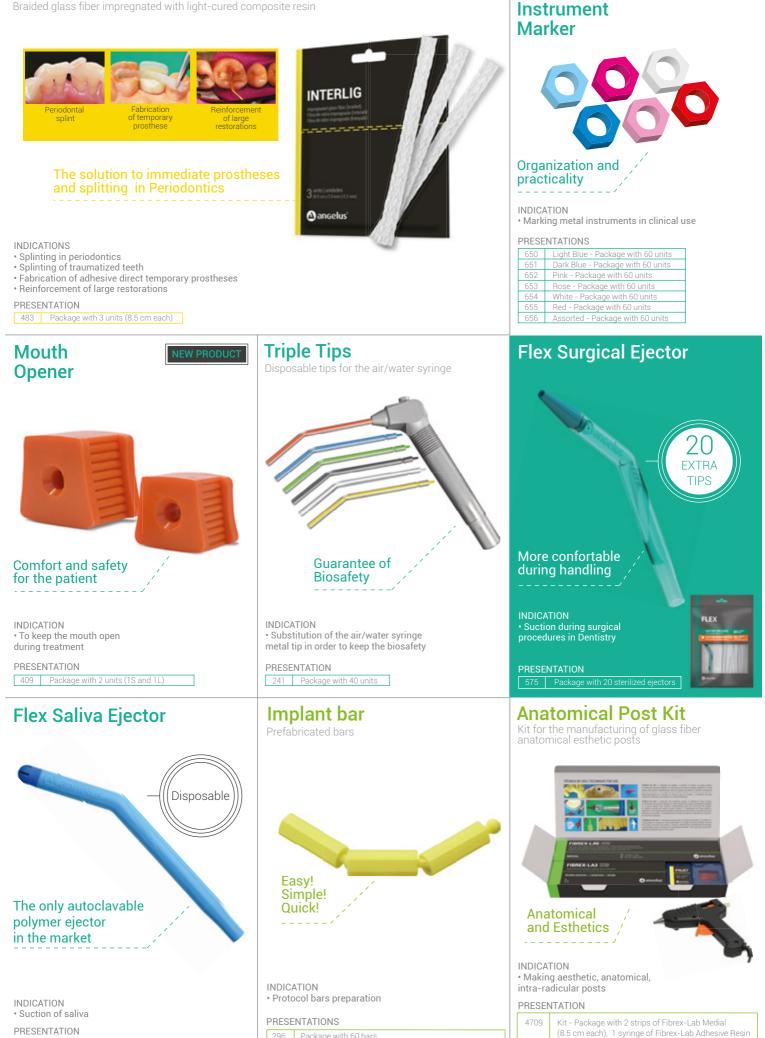

296 Package with 60 bars

Package with 30 bars

Silicon

C (2 g), 10 Pinjet pins and 1 hot glue gun (free)

Fibrex-Lab Pontic System

System with prefabricated glass fiber pontics for the structural reinforcement of adhesive prostheses



Adhesive prostheses in minutes

INDICATIONS

- Structural reinforcement of adhesive bridges fabricated with laboratory resin
 Structural reinforcement for the fabrication of direct (immediate) temporary prostheses

PRESENTATIONS

461	Refill - Package with 24 prefabricated pontics: 12 anterior (4S, 4M, 4L) and 12 posterior (4S, 4M, 4L)
460	Kit - Package with 12 prefabricated pontics: 6 anterior (2S, 2M, 2L), 6 posterior (2S, 2M, 2L), 21 cm of Fibrex Medial,
	2 g of universal adhesive resin and 4 ml of union agent

Spatula

Spatula for the sculpture of ceramic/porcelain and resins with ultra flexible blades and depth gauge

Ultra flexible blades and depth gauge

INDICATIONS

- · Sculpture of ceramic/porcelain and resins
- Depth measurement · Cutting of connectors, mamelons and incisal edges
- · Removal of ceramics from palatal, occlusal and buccal surfaces

DRECENTATIONS

PRESENTATIONS	
505	Kit - 1 Package wirh spatula and 12 blades (2 units
	of each type)
509	Blade Refill #1 - Package with 6 units (porcelain)
510	Blade Refill #2 - Package with 6 units (porcelain)
511	Blade Refill #3 - Package with 6 units (porcelain)
512	Blade Refill #4 - Package with 6 units (resin)
513	Blade Refill #5 - Package with 6 units (resin)
514	Blade Refill #6 - Package with 6 units (resin)

Large Silicone Container



Flexible

INDICATION • For handling plaster, alginate and other dental materials

PRESENTATION

Silicon Dappen Silicone Dappen



two concavities

INDICATION • Handling of medicaments PRESENTATION 600 Package with 1 unit

Plaster Spatula



INDICATION · For handling gesso and alginate PRESENTATION

MZ Primer



To increase the adhesion of composite and acrylic resins to metal and Zirconia structures
To increase adhesion in the cementation of crowns with metal or Zirconia frameworks and to treat metal surfaces during crown repair procedures with

964 Package with 1 bottle (5 ml)

Silicon Dappen



INDICATION • Handling of medicaments

PRESENTATIONS

598	Extra Large (mixing colors) - Package with 1 unit
599	Large (mixing colors) - Package with 1 unit
601	Small (mixing colors) - Package wih 1 unit

Paladon Jar Silicone jar with lid



INDICATION · For the manipulation of acrylic resin

PRESENTATION 621 01 Paladon jar unit with lid

Simplified!

Customer Service +55 (43) 2101-3200

www.angelus.ind.br

