

DERMATHOD 345 RADIANCE PROTOCOL + GUIDE



BY KIN AESTHETICS

Published by:
by KIN AESTHETICS
Ann Arbor, MI

(c) 2023 by KIN AESTHETICS

All rights reserved. No part of this workbook may be reproduced or altered in any form or by any means without the prior written permission of the publisher, excepting brief quotes used in connection with reviews written specifically for inclusion in a magazine, newspaper, online, or broadcast media. Subscribers may reproduce to hard copy only.


This workbook expresses the author's views and opinions. The information contained in this workbook is provided without any express, statutory, or implied warranties. Neither the authors, by KIN AESTHETICS, nor its resellers, or distributors will be held liable for any damages caused or alleged to be caused either directly or indirectly by this workbook.

by KIN AESTHETICS is a trademark of by KIN AESTHETICS. All other trademarks are property of their respective owners.

ABOUT

Dermethod's Radiance ampoule is part of their Derma Level collection, and is a micro-channeling system for professional use only. The "microneedle stimulator" maximizes the absorption of the ampoule by creating fine channels in the skin. The length of the needles can be adjusted depending on the skin condition.

This treatment comes in a safe, sterile, disposable ampoule-integrated adjustable microneedle stimulator. The needles are made of medical-grade acryl which prevents allergies. The adjustable depth includes three levels: .3, .4 and .5

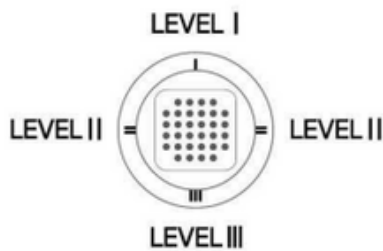

- Safe, sterile, disposable ampoule-integrated adjustable microneedle stimulator
 - Sterilized disposable device fully hygienic by EO gas
 - Convenience - Ampoule is filled in airless (vacuum) container for simultaneous skin stimulation and ampoule dispense
 - Customized skincare with 3-stage adjustable levels for several skin concerns and areas
 - LEVEL I : For skin glowing and moisturizing
 - LEVEL II : Also for pore tightening and silky texture
 - LEVEL III : Also for serious skin concerns and trouble areas
 - Number of Needles - 32
 - Thickness of Needle - 34 Gauge
- * This product is a skin stimulator, not a medical device.
* DERMA LEVEL 345 enables hygienic and safe treatment by sterilizing product in individual package.

This treatment is specifically for hyperpigmentation (age spots, sun damage, and melasma) or for those looking for a brighter complexion.

Triple Mela Complex, comprised of tranexamic acid, HEPES, and Niacinamide effectively suppress the overactive melanocytes which causes hyperpigmentation.


sh-Oligopeptide-1 (10ppm x 10%) is an epidermal growth factor (EGF) which is a key component of cell growth and the regeneration process. They increase collagen and elastin production. 10ppm EGF is the maximum concentration allowed in cosmetics by the KFDA.

Camellia Sinensis Hydrosol is derived from green tea leaves and is produced via vapor distillation. It is a powerful antioxidant and has incredible anti-inflammatory benefits. It can repair DNA damaged by UV rays, and can protect the skin from UVB radiation. It also helps prevent trans-epidermal water loss.

HydroxyEthylPiperazine Ethane Sulfonic Acid also known as HEPES, activates natural enzymes in the skin which help break the bonds that bind dead skin cells to the surface, resulting in gentle exfoliation.

Tranexamic Acid is an incredible pigment fighter which is safe for all skin types, and Fitzpatrick's. It's quickly becoming the gold standard in the treatment of hyperpigmentation caused by melasma.

MELA CONTROL SYSTEM

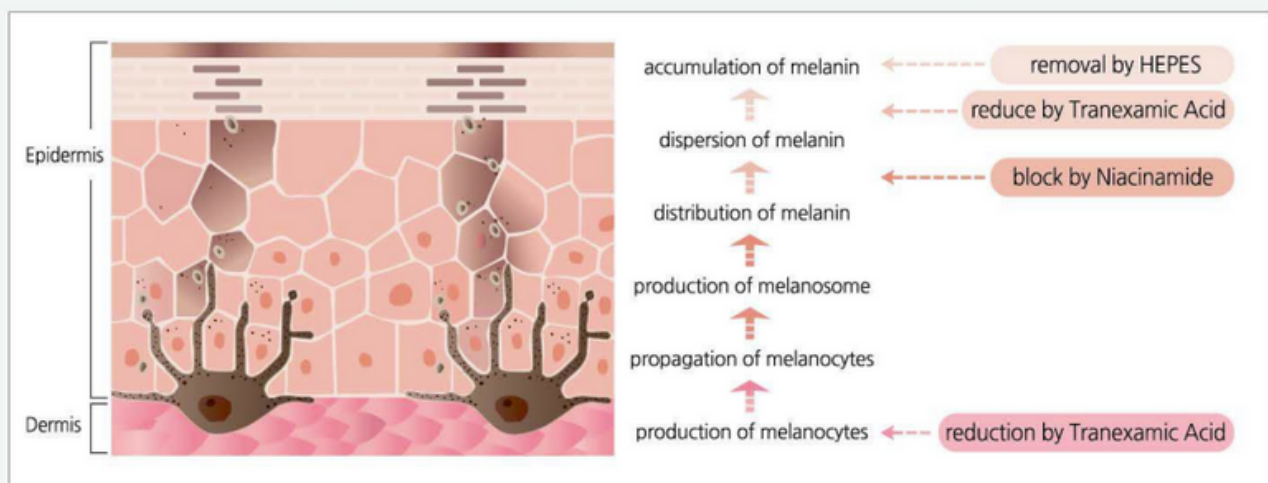

BENEFITS

- Improves hyperpigmentation
- Glycated skin will benefit from antioxidants

CONTRAINDICATIONS

Allergy to any of the ingredients

Dermatitis (eczema, psoriasis, etc)

Sunburn

Severe barrier impairment or inflammation

Pregnancy

WHAT YOU'LL NEED

1. Dermethod Revive Cleansing Gel
2. Dermethod Priming Peel Booster (Optional)
3. Dermethod 345 Radiance Ampoule
4. Dermethod Triple Revive Sheet Mask
5. Dermethod Ami-Sterol Cream
6. Dermethod Sun saver SPF

PROTOCOL

1. Cleanse the skin
2. Use Priming Peel Booster Pad (optional)
3. Without rinsing proceed by stamping the skin with the ampoule. 1 to 3 passes is recommended.
4. Apply Triple Revive Sheet Mask for 10-15 minutes
5. Finish with Ami-Sterol Cream and SPF

DERMA LEVEL 345

Point Tip!

Recommended adjusting the needle length to the level I, II, and III by client's skin concerns, pains, and thickness of the Skin.



POSTCARE

DO NOT EXFOLIATE

Do not exfoliate the skin for at least 7 days post treatment

PROTECT

Keep skin hydrated with appropriate moisturizer and SPF daily.

SESSIONS + INTERVALS

Can be done every three to four weeks

ACCUTANE OR RETIN-A

Do not use on any clients who have used Accutane within a year.

Have clients stop using Retin-A at least 7 days before treatment depending on strength.

ADDITIONAL PROTOCOLS

This treatment can be added into any brightening facial when appropriate. This would be the last step.

LET'S CONNECT

[JOIN OUR FACEBOOK GROUP](#)

[FOLLOW US ON INSTAGRAM](#)

[CHECK OUT OUR CATALOG](#)

[WATCH US ON YOUTUBE](#)

SEND US AN EMAIL:
Info@esthisupply.com