Revision 006

DESIGN SHEET


특이사항 : 별색유무 : 사이즈: 160*130 제품명 : 영문 Q 설명서 인쇄업체/제조국: 날짜: 2019.08.09

- 홈페이지 주소 수정



CONTENTS 1. Important Safeguards

- 2. Important Symbols
- 3. Indications for use
- 4. Components and assembly
- 5. Button Control 6. Pumping Guide
- 7. Getting started
- 8. How to use the dual pump 9. Cleaning and disinfection
- 10. How long can I store breast milk?
- 11. How do I thaw and use stored breast milk?
- 12. Use and Storage environment
- 13. Trouble shooting
- 14. Specifications
- 15. Limited Warranty
- 16. EMC



When using electrical products, especially when children are present, basic safety precautions should always

- ① If you are a mother who is infected with Hepatitis B, Hepatitis C or Human Immunodeficiency Virus (HIV), pumping breast milk will not reduce or remove the risk of transmitting the virus to your baby through your breast
- ② Before each use visually inspect the individual components for cracks, chips, tears, discoloration or deterioration. In the event that damage to the device is observed, please discontinue use until the parts have been replaced.
- READ ALL INSTRUCTIONS BEFORE USING. When using electrical products, basic safety precautions should always be followed This is a single user product.
 - Use by more than one person may present a health risk and performance questions and voids the warranty.
- - To reduce the risk of electrocution. ① DO NOT USE WHILE BATHING.
 - ② DO NOT PLACE OR STORE PRODUCT WHERE IT CAN FALL OR BE PULLED. ③ DO NOT PLACE IN OR DROP INTO WATER OR OTHER LIQUOD.
 - ④ DO NOT REACH FOR A PRODUCT THAT HAS FALLEN INTO WATER, UNPLUG THE PRODUCT IMMEDIATELY.
 - ⑤ DO NOT SANITIZE THE KIT IN MICROWAVE OVEN, NEVER IMMERSE MAIN BODY IN WATER.






To reduce the risk of burns, electrocution, fire, or injury to persons. ① THIS PRODUCT SHOULD NEVER BE LEFT UNATTENDED WHEN PLUGED IN. ② CLOSE SUPERVISTION IN NECESSARY WHEN


- THIS PRODUCT IS USED NEAR INFANTS OR CHILDEN. $\ensuremath{\Im}$ USE THIS PRODUCT ONLY FOR ITS INTENDED USE AS DESCRIBED IN THIS MANUAL.
- DO NOT USE ATTACHMENTS NOT RECOMMENDED BY THE UZINMEDICARE CO. ④ NEVER OPERATE THIS PRODUCT IF IT HAS A DAMAGED CORD OR PLUG. IF IT IS NOT WORKING PROPERLY, IF IT HAS BEEN DROPPED OR DAMAGED.
- DROPPED INTO WATER, OR IF ANY PARTS ARE BROKEN OR MISSING. **⑤** KEEP THE CORD AWAY FROM HEATED SURFACES. 6 NEVER USE WHILE SLEEPING OR DROWSY.
- $\ensuremath{{\mathbb T}}$ DO NOT USE OUTDOORS OR OPERATE WHERE AEROSOL SPRAY. PRODUCTS ARE BEING USED OR WHERE OXYGEN IS BEING ADMINISTERED. ® THE AC/DC ADAPTOR CORD SHOULD BE UNPLUGGED FROM THE OUTLET WHEN NOT IN USE.
- 10 DO NOT INHALE OR SWALLOW SMALL PARTS. ① ALLERGIC REACTIONS MAY OCCUR. ② LINT, DUST, LIGHT (INCLUDING SUNLIGHT), ETC CAN BE ADVERSELY AFFECT SAFETY AND
- ESSENTIAL PERFORMANCE. (3) AC/DC ADAPTOR MUST BE EASY TO UNPLUG POSITION DURING USAGE. $\textcircled{\scriptsize 0}$ BE CAREFUL NOT TO DROP PRODUCT. IF DROPPED OR IMPACTED, CONTACT NEARBY
- SERVICE CENTER. ⓑ DO NOT USE ACCESSORIES OF OTHER BRAND WITH THIS PRODUCT. BREAST SHIELD OF THIS PRODUCT IS COMPLYING WITH BIOCOMPATIBILITY OF MEDICAL DEVICE.
- If you feel pain in your breast or nipple, turn the pump off or adapter plug out and remove from your breast.
- Consult your healthcare professional (Suction can be broken by inserting finger between the breast and breast shield or by shutting the pump off)
- 2




9 DO NOT DISASSEMBLE OR MODIFY THE PRODUCT.

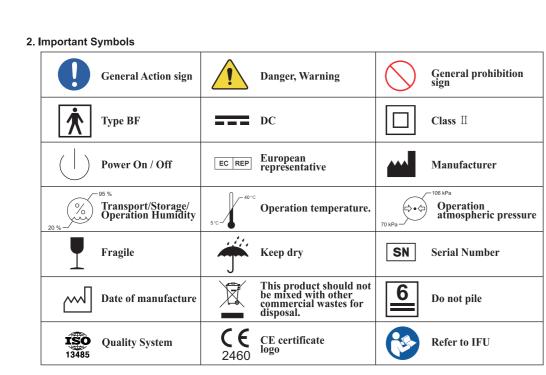

WARNING! This is designed to be a single user product. Use of this breast pump by anyone other than the original owner may present health risks,




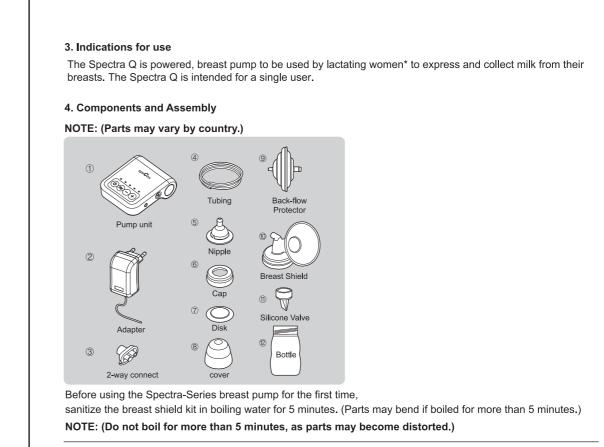



* Gender : Female / Age : Adult


4




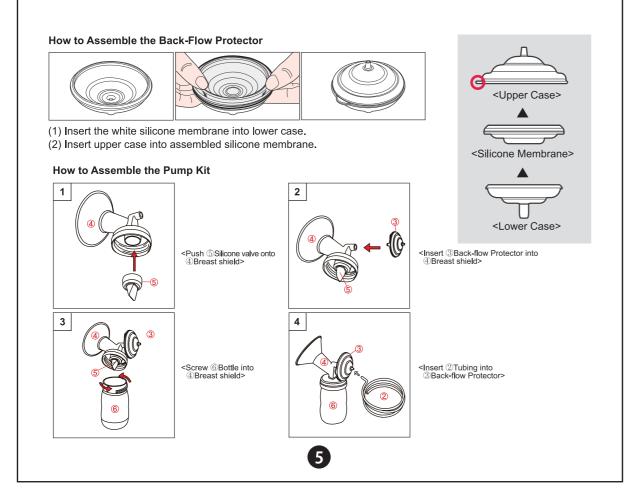


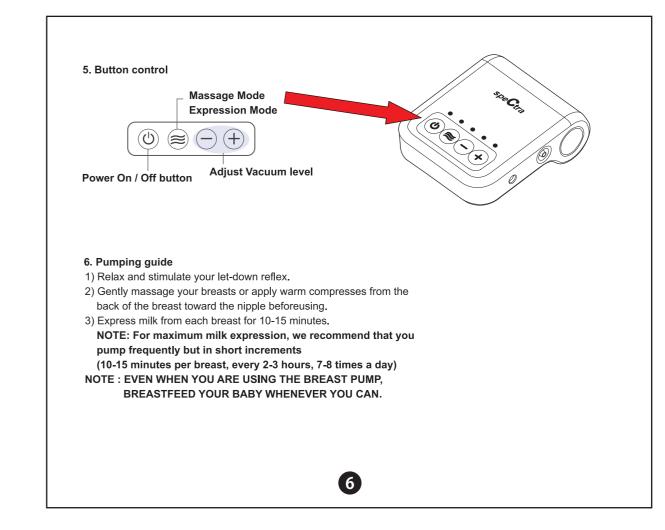


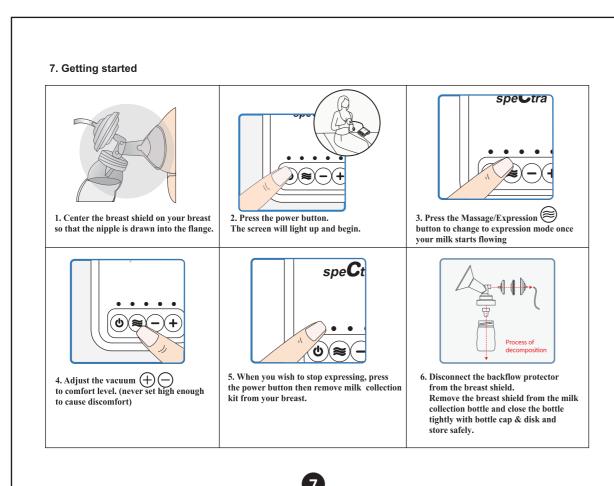

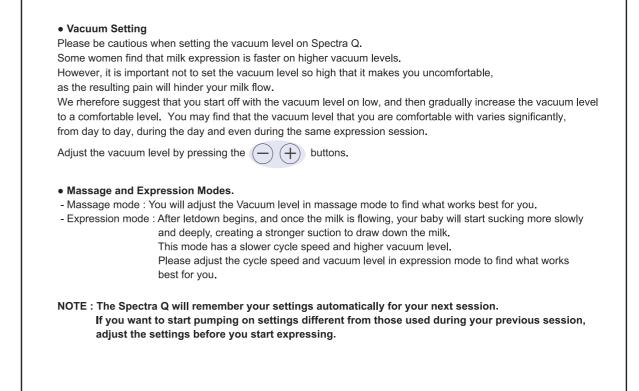

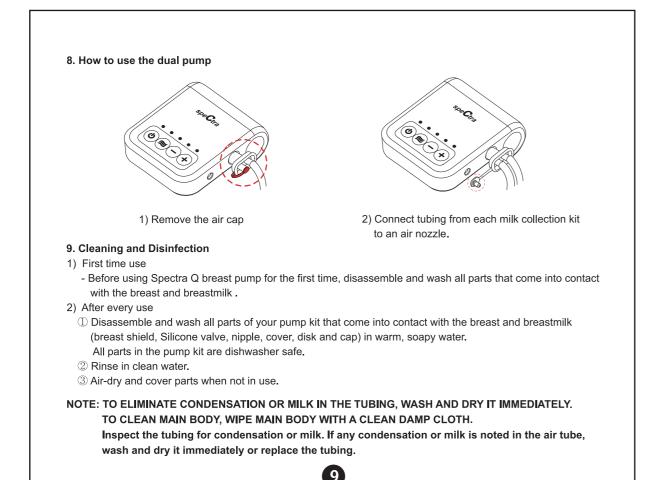

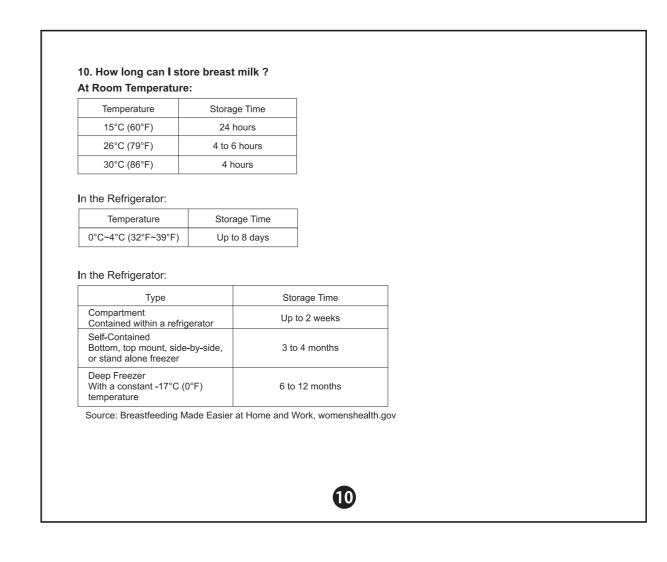

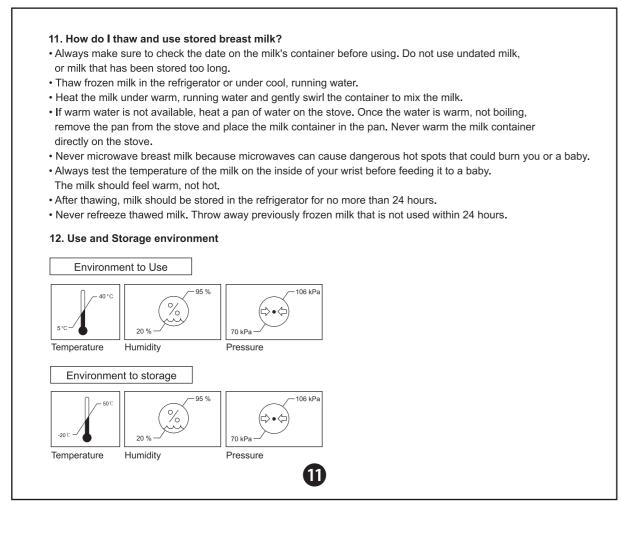

Condition	Possible Causes	Checks	Solutions
No Power	Adaptor	Check if the power cord is not connected or it has damaged.	Plug into the outlet. If it has damaged, Contact manufacturer or service center or where you purchased
	Air tube	Check the tubing is connected to the main body.	Connect the air tube to the main body.
No Suction	Valve	Check if they are connected to breast shield properly.	Disassemble and reassemble them properly.
	Air cap	Check if the air cap is closed.	Close the air cap.
Low Suction	Vacuum Level	Check if there is a low vacuum level on the vacuum regulator valve or if there is an abnormal noise.	Contact the location where you purchased the product or the manufacturer.
	Defective assembly kit	Check the connection of the kit.	Disassemble and reassemble them.
	Breast shield	Check if there is problem with the breast shield.	Purchase and replace the breast shield.
	Valve	Check if there is damaged in valve head.	Replace the valve.
Pain	Too high suction	Check the suction level.	Set to the lowest suction level and consult your lactation consultant or physician.
		12	



Mobile Phone Address

Telephone

This equipment needs to be installed and put into service in accordance with the information provided in the user manual [IEC/EN 60601-1-11:2010 Clause 12.3a] Wireless communications equipment such as wireless home network devices, mobile phones, cordless telephones and their base stations, walkie-talkies can affect this equipment and should be kept at least a distance 1.0m away from the equipment. [IEC/EN 60601.1.11:2010 Clause 12.3b] This equipment has been tested and found to comply with the limits for medical devices in IEC 60601-1-2:2007. These limits are designed to provide reasonable protection against harmful interference in a typical medical installation. This equipment generates, uses and can radiate radio frequency energy and if not installed and used in accordance with the instructions, may cause harmful interference to other devices in the vicinity. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to other devices, which can be determined by turning the equipment off and on, the user is encourage to try to correct the interference by one or moer of the following measures. Reorient of relocate the receiving device. Increase the separation between the equipment. Connect the equipment into an outlet on a circuit different from that to which the other device(s) are connected. Consult the manufacturer or field service technician for help.	40 5110
with the information provided in the user manual [IEC/EN 60601-1-11:2010 Clause 12.3a] Wireless communications equipment such as wireless home network devices, mobile phones, cordless telephones and their base stations, walkie-talkies can affect this equipment and should be kept at least a distance 1.0m away from the equipment. [IEC/EN 60601.1.11:2010 Clause 12.3b] This equipment has been tested and found to comply with the limits for medical devices in IEC 60601-1-2:2007. These limits are designed to provide reasonable protection against harmful interference in a typical medical installation. This equipment generates, uses and can radiate radio frequency energy and if not installed and used in accordance with the instructions, may cause harmful interference to other devices in the vicinity. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to other devices, which can be determined by turning the equipment off and on, the user is encourage to try to correct the interference by one or moer of the following measures. Reorient of relocate the receiving device. Increase the separation between the equipment. Connect the equipment into an outlet on a circuit different from that to which the other device(s) are connected.	
Wireless communications equipment such as wireless home network devices, mobile phones, cordless telephones and their base stations, walkie-talkies can affect this equipment and should be kept at least a distance 1.0m away from the equipment. [IEC/EN 60601.1.11:2010 Clause 12.3b] This equipment has been tested and found to comply with the limits for medical devices in IEC 60601-1-2:2007. These limits are designed to provide reasonable protection against harmful interference in a typical medical installation. This equipment generates, uses and can radiate radio frequency energy and if not installed and used in accordance with the instructions, may cause harmful interference to other devices in the vicinity. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to other devices, which can be determined by turning the equipment off and on, the user is encourage to try to correct the interference by one or moer of the following measures. - Reorient of relocate the receiving device. - Increase the separation between the equipment. - Connect the equipment into an outlet on a circuit different from that to which the other device(s) are connected.	···
cordless telephones and their base stations, walkie-talkies can affect this equipment and should be kept at least a distance 1.0m away from the equipment. [IEC/EN 60601.1.11:2010 Clause 12.3b] This equipment has been tested and found to comply with the limits for medical devices in IEC 60601-1-2:2007. These limits are designed to provide reasonable protection against harmful interference in a typical medical installation. This equipment generates, uses and can radiate radio frequency energy and if not installed and used in accordance with the instructions, may cause harmful interference to other devices in the vicinity. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to other devices, which can be determined by turning the equipment off and on, the user is encourage to try to correct the interference by one or moer of the following measures. - Reorient of relocate the receiving device. - Increase the separation between the equipment. - Connect the equipment into an outlet on a circuit different from that to which the other device(s) are connected.	
These limits are designed to provide reasonable protection against harmful interference in a typical medical installation. This equipment generates, uses and can radiate radio frequency energy and if not installed and used in accordance with the instructions, may cause harmful interference to other devices in the vicinity. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to other devices, which can be determined by turning the equipment off and on, the user is encourage to try to correct the interference by one or moer of the following measures. - Reorient of relocate the receiving device. - Increase the separation between the equipment. - Connect the equipment into an outlet on a circuit different from that to which the other device(s) are connected.	cordless telephones and their base stations, walkie-talkies can affect this equipment and should be kept at least a
This equipment generates, uses and can radiate radio frequency energy and if not installed and used in accordance with the instructions, may cause harmful interference to other devices in the vicinity. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to other devices, which can be determined by turning the equipment off and on, the user is encourage to try to correct the interference by one or moer of the following measures. Reorient of relocate the receiving device. Increase the separation between the equipment. Connect the equipment into an outlet on a circuit different from that to which the other device(s) are connected.	This equipment has been tested and found to comply with the limits for medical devices in IEC 60601-1-2:2007.
with the instructions, may cause harmful interference to other devices in the vicinity. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to other devices, which can be determined by turning the equipment off and on, the user is encourage to try to correct the interference by one or moer of the following measures. - Reorient of relocate the receiving device. - Increase the separation between the equipment. - Connect the equipment into an outlet on a circuit different from that to which the other device(s) are connected.	These limits are designed to provide reasonable protection against harmful interference in a typical medical installation.
However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to other devices, which can be determined by turning the equipment off and on, the user is encourage to try to correct the interference by one or moer of the following measures. - Reorient of relocate the receiving device. - Increase the separation between the equipment. - Connect the equipment into an outlet on a circuit different from that to which the other device(s) are connected.	
If this equipment does cause harmful interference to other devices, which can be determined by turning the equipment off and on, the user is encourage to try to correct the interference by one or moer of the following measures. Reorient of relocate the receiving device. Increase the separation between the equipment. Connect the equipment into an outlet on a circuit different from that to which the other device(s) are connected.	
which can be determined by turning the equipment off and on, the user is encourage to try to correct the interference by one or moer of the following measures. Reorient of relocate the receiving device. Increase the separation between the equipment. Connect the equipment into an outlet on a circuit different from that to which the other device(s) are connected.	
interference by one or moer of the following measures. - Reorient of relocate the receiving device. - Increase the separation between the equipment. - Connect the equipment into an outlet on a circuit different from that to which the other device(s) are connected.	
 Reorient of relocate the receiving device. Increase the separation between the equipment. Connect the equipment into an outlet on a circuit different from that to which the other device(s) are connected. 	
 Increase the separation between the equipment. Connect the equipment into an outlet on a circuit different from that to which the other device(s) are connected. 	,
- Connect the equipment into an outlet on a circuit different from that to which the other device(s) are connected.	
	·
	Consult the manufacturer or field service technician for help.