



ARGO

ELECTRIC TOILET LIFT

Instruction Manual



Phone

(212) 366-5483



Contact

Info@ClimbingSteps.com

www.MobilePatientLift.com



Address

6601 Lyons Rd, Suite C10,
Coconut Creek, FL 33073



MOBILE PATIENTLIFT



Table of Contents

1.0	Introduction
	1.1 - Indication for Use
	1.2 - General Description / Intended Use
	1.3 - Disclaimer
	1.4 - Unpacking the Device
2.0	Symbols and Definitions Used in the Manual
	2.1 - Warning/Cautions
	2.2 - Safety Precautions
3.0	Diagram of Lift
4.0	ArGo Toilet Lift Features
5.0	Assembling Details
6.0	Installation Details
7.0	Charging the ArGo Toilet Lift
8.0	Operation Details
9.0	Technical Specifications
10.0	Care and Cleaning Instructions
11.0	FAQs
12.0	Troubleshooting
13.0	Limited Warranty
14.0	Device Label

1.0 Introduction

Congratulations on choosing the ArGo Toilet Lift! We understand that maintaining independence in the bathroom is a priority, and our lift is designed to make using the toilet safe, comfortable, and dignified. This manual will guide you through the entire setup process, from unpacking the lift to its proper installation and operation. Please take the time to read through these instructions carefully to ensure a smooth and successful installation.



Improper usage of this device can cause injury. The ArGo Toilet Lift must only be operated as described in this manual. Do not modify the ArGo Toilet Lift as modifications can result in unpredictable performance and result in injury.

NOTE: This manual should remain with the ArGo Toilet Lift at all times.

For customer service or technical assistance,
please contact us via email Info@ClimbingSteps.com

1.1 Indications for Use

The ArGo Toilet Lift empowers individuals with limited mobility to maintain independence in the bathroom. It tackles the challenges of safely sitting down and standing up when using the toilet, promoting a dignified and comfortable experience. This lift is a perfect solution for those who find traditional methods difficult, allowing them to use the bathroom with greater ease, independence and confidence.



DO NOT use this lift to transport occupants
who may have cervical, spinal, or fracture injuries.

1.2 General Description / Intended Use

The ArGo Toilet Lift is designed for both safety and user comfort. Its smooth lifting mechanism allows for effortless transfers on and off the toilet. However, user safety is paramount. To ensure a secure and comfortable experience, always ensure the user is properly positioned in the lift before operating. It's important that anyone using and/or assisting with the lift reads this manual thoroughly to become familiar with proper operation procedures.

1.3 Disclaimer

This user manual contains general instructions and guidelines for the use, operation, and care of this product. These instructions are not all-inclusive. The safe and proper use of this product is solely at the discretion of the user. Safety information is included as a service to the user. All other safety measures taken by the user should be within and under consideration of applicable regulations.

1.4 Unpacking the Device

Unpack your brand new ArGo Toilet Lift, remove all the shipping and packing materials, and check all the items for proper operation. If anything is missing or noted not to be correct, or any type of damage is present due to shipping, please contact Mobile PatientLift.

Items Included:

- 1 x ArGo Toilet Lift Base
- 1 x Right Handle (with switch)
- 1 x Left Handle
- 1 x Battery
- 1 x Charger
- 1 x Wheel Set
- 1 x Adjustable Leg Set
- 1 x Installation Kit
- 1 x Instruction Manual



2.0 Symbols and Definitions Used in this Manual



Consult instructions for use.



Serial Number of the device.



Date of Manufacture.



Product should not be disposed of with your other household waste.



Check sign explains the items that you should comply with upon operation, repair and maintenance of this device.



Do not lubricate the belts or tracks of this device.



Mechanical moving parts.

2.1 Warning / Caution

These words carry special meanings and should be carefully reviewed.



This symbol alerts the reader about a situation which, if not avoided, could result in death or serious injury. It may also describe potential serious adverse reactions and safety hazards.



This symbol alerts the reader of a potentially hazardous situation which, if not avoided, may result in minor or moderate injury to the user or patient or damage the product or other property. This includes special care necessary for the safe and effective use of the device and the care necessary to avoid damage to a device that may occur as a result of use or misuse.


NOTE: This provides special information to make maintenance easier or important instructions clearer.

2.2 Safety Precautions



1. Read this entire manual carefully before using the ArGo Toilet Lift. Ensure you understand all the instructions for safe operation and maintenance.
2. Follow the provided installation instructions precisely to ensure the lift is securely mounted on your toilet.
3. Never exceed the lift's weight capacity as specified in the manual. Overloading can damage the lift and compromise safety.
4. If a user cannot maintain an upright seated position independently, a caregiver or supervisor should be present to assist during transfers.
5. Maintain a clean seat before each use. Regularly inspect the lift for missing or damaged parts, and never operate it if something is amiss.
6. Always sit down slowly and steadily on the lift to prevent injury and avoid stressing the lift mechanism.
7. While the lift is operating, avoid placing hands, feet, or any other objects near moving parts to prevent accidental injury.
8. Standing or Kneeling is Prohibited: The lift is designed for seated transfers only. Never stand or kneel on the lift platform.
9. The ArGo Toilet Lift is designed for bathroom use. Avoid using it for any other purpose.
10. Never leave children unattended while using the ArGo Toilet Lift.

3.0 Diagram of Lift

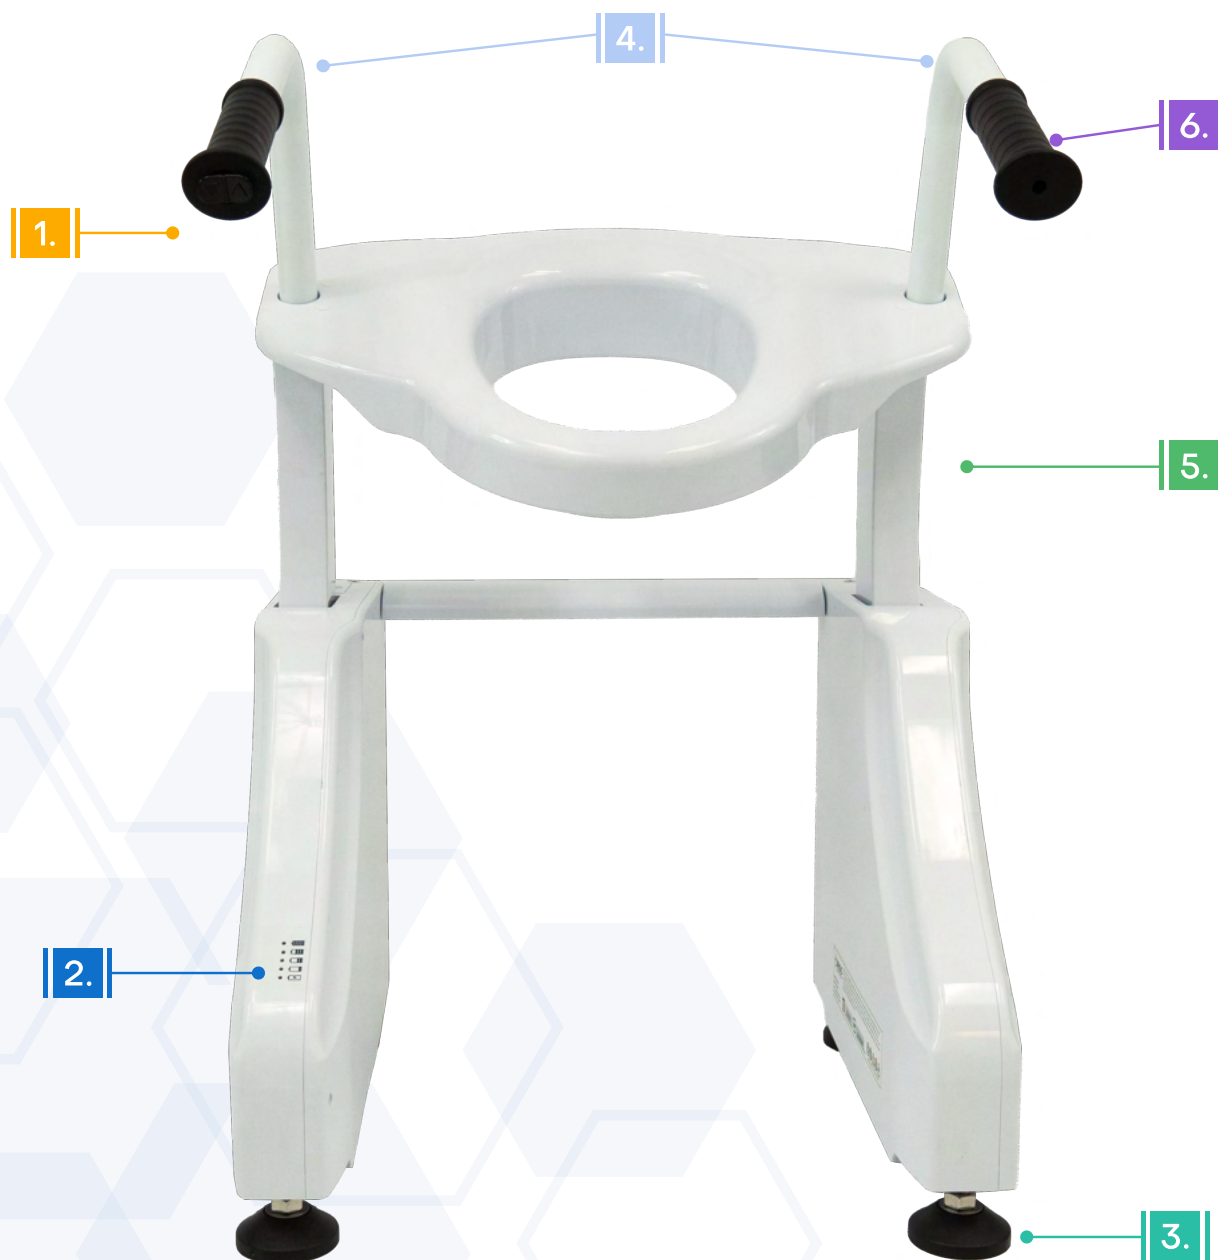

1. Easy Operation Button

2. Battery Indicator Light

3. Height Adjustable Legs

4. Support handles

5. Adjustable Seat Height

6. Ergonomic Grip

4.0 ArGo Toilet Lift Features



Effortless Transfers: The ArGo's electric lift provides a smooth and gentle rise and descent, making transfers on and off the toilet effortless.



Universal Design: The ArGo's adjustable height ensures compatibility with almost any toilet shape and height, offering a versatile solution for various bathroom configurations.



High Lift Support: The ArGo boasts a 13-inch lift, ideal for those who need extra assistance regaining a standing position after using the toilet.



Secure and Stable Support: Ergonomically angled handles provide additional stability and support during transfers, enhancing user confidence.



Battery Powered Convenience: The ArGo features a rechargeable battery, allowing for use in bathrooms without a nearby electrical outlet.



Plug-In Option for Unlimited Lifts: For added peace of mind, the ArGo offers the option to plug it in for continuous use without worrying about battery life.



Easy to Use Controls: A simple push-button operation makes the ArGo effortless to use, promoting independence in the bathroom.



Comfortable and Adjustable Seat: The ArGo's ergonomic seat provides comfort during use and adjusts to your desired height for optimal positioning.

5.0 Assembling Details



Step 1

Unpack the components from the packaging and ensure all necessary parts are included. Organize them in a clear workspace to avoid confusion during the assembly process.



Step 2

Take the right handle, which has an electrical connector, and carefully align the notches on the plugs. Once connected, twist the threaded collar to secure the connection.

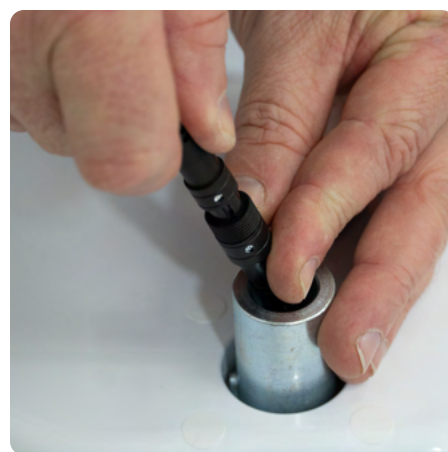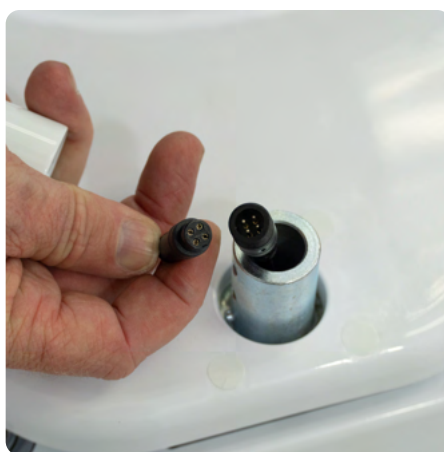

Step 3

Both handles should fit onto the posts located on the base of the lift. Check that the screw holes on the handles align with the corresponding holes on the base for proper attachment.



Step 4

Insert the provided screws through the aligned holes in the handles and the posts. Tighten the screws using an allen wrench to ensure that both handles are firmly secured to the base.



Step 5

Install the adjustable feet into the bottom of the lift by screwing them in. This will allow you to make height adjustments to accommodate the specific toilet height.



Step 6

Adjust the lift height by turning the feet to raise or lower the lift to the desired height. Ensure the rear support area of the lift is slightly higher ($\frac{1}{8}$ " to $\frac{1}{4}$ ") than the toilet rim for proper alignment.



Optional Step

If you need the lift to be mobile, you can replace the adjustable feet with the optional wheel set. This allows for easier movement of the lift between bathrooms or different locations.



6.0 Installation Details

STEP 1

Use a flathead screwdriver and a pair of pliers to remove the bolts and nuts located beneath the toilet that secure the seat. Once the nuts are loosened and removed, lift the toilet seat off the bowl to make space for the new lift installation.



STEP 2

Raise the lift using its control to allow better access. Slide the plastic cover off the rear support and install the brackets by guiding the bolts into the slots, using an allen wrench for assistance if needed.



STEP 3

After the brackets are aligned and installed, tighten the bolts securely to ensure the lift is stable. Once everything is securely in place, slide the rear support cover back over the crossbar to complete the installation.



7.0 Charging the ArGo Toilet Lift

Your battery should arrive with some charge. However, it is recommended to **fully charge it** before first use. Make sure to plug the power adapter directly into a power outlet. When the power is connected, the indicator light on the adapter will turn on.



Charging Methods

- **Method 1: Remove and Charge**
 - a. Raise the lift halfway.
 - b. Pull up on the silver handle to remove the battery from the lift.
 - c. Plug the battery into the charger/power supply.
- **Method 2: Charge in Place**
 - a. If the battery is low and cannot raise the lift enough to remove it, plug the charger/power supply into the rear of the lift.



Failing to recharge when the battery reaches a low status will cause battery failure, **requiring a battery replacement.**



Ensure your ArGo Toilet Lift is plugged into a GFCI-protected outlet. Avoid mixing water and electricity to ensure safe operation.

Charging Your Argo Toilet Lift

To keep your Argo Toilet Lift in top shape, follow these simple charging steps:

1. **Charge Only Until Full:** Plug in the unit until the battery indicator light shows it's fully charged. Once the light indicates a full charge, unplug the unit to prevent overcharging.
2. **Avoid Full Discharge:** Be mindful not to let the battery go completely dead, as this can lead to the need for a replacement battery.

By following these steps, you'll help extend the life of your battery and keep your unit ready to use!

8.0 Operation Details



1.

Stand in front of the lift and use the buttons on the right handle to lower the seat. Once the lift reaches a comfortable height, sit down slowly as the seat continues to lower you into position.




2.

While seated, complete your usual routine comfortably. The lift remains stationary while in use, providing a stable platform for support.



3.

After using the toilet, press the button on the right handle to raise the lift. As the seat lifts you, place your feet firmly on the ground and use the handles for balance until you are in a fully standing position.

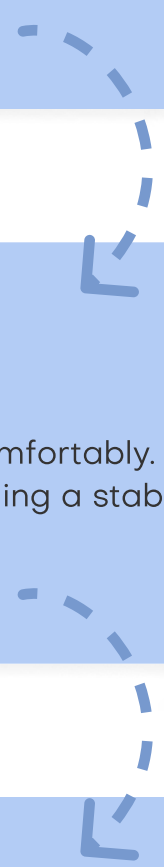

9.0 Technical Specifications

- A** Lift Height: 17"
- B** Lift Width: 24"
- C** Lift Depth: 21"
- D** Adjustable Height: 0" - 14"
- E** Base Inner Width: 16"
- F** Adj. Leg Height: 3"
- G** Handle Height: 9"
- H** Handle Length: 13"
- I** Seat Depth: 16"
- J** Inside Bowl Width: 11"
- K** Inside Bowl Depth: 9"
- L** Full Height: 37"



10.0 Care and Cleaning Instructions

Regularly clean the ArGo Toilet Lift to prevent dirt and debris buildup. Use a mild detergent and water to clean the surfaces of the lift.



To clean the surfaces of the ArGo Toilet Lift, create a mild detergent solution, wipe down all surfaces with a damp cloth or sponge, and dry thoroughly.



Do not scratch or scrape the surface of the product with hard objects to prevent material damage.



Do not use products that have bleach or phenolic cleaners.



Check the height adjustment of the lift to ensure it is still set at the desired level. If necessary, adjust the feet of the lift to maintain the proper height.



Inspect the handles periodically to ensure they are securely attached. If any screws are loose, tighten them using the provided allen wrench.



Inspect the toilet brackets and bolts to ensure they are securely attached to the lift and the toilet. If any bolts are loose, tighten them using the allen wrench.



In a medical setting, we recommend you disinfect the lift between riders with basic disinfectant for patient and operator safety.



If any issues or defects are noticed, contact Climbing Steps, Inc. for warranty service and repairs.



11.0 FAQs

Q

Is the ArGo Toilet Lift compatible with different types of toilets?

The ArGo Toilet Lift is suitable for a variety of toilet types, as long as the toilet is less than 21" wide and the rim is between 14" and 18" tall. This makes it versatile and adaptable to different bathroom setups.

A**Q**

How portable is the ArGo Toilet Lift?

For ease of use, the ArGo includes four optional wheels that allow users to use the lift in multiple locations, providing convenience and flexibility. This adaptability is particularly advantageous for medical facilities seeking versatile equipment for patient care.

A**Q**

Can the ArGo Toilet Lift be adjusted to accommodate different toilet heights?

Yes, unlike some other toilet lifts and lift assist devices, the ArGo Toilet Lift is adjustable to accommodate different heights. It has adjustable feet that can increase or decrease the height between 14" and 18", allowing for customization based on the toilet bowl height.

A**Q**

Are there any specific clearance or space requirements for using the ArGo Toilet Lift?

Yes, the ArGo Toilet Lift requires the toilet to be less than 21" wide and have a rim height between 14" and 18" for proper operation. It is important to ensure the toilet meets these requirements to ensure compatibility with the lift.

A

12.0 Troubleshooting

If you have any questions about the bridge bath lift, please call us for customer service assistance. The device label will also show the serial number and the date manufactured.

Problem	Cause	Solution
The ArGo Toilet Lift is not lifting or lowering.	The device is not properly plugged in or the battery is not charged.	Ensure the power cord is securely plugged into a working electrical outlet or check that the battery is fully charged. If using the battery, switch to the plug-in option to test if the battery needs replacement.
The lift moves slowly or stops during operation.	The lift is overloaded beyond its weight capacity or there is an obstruction.	Check to ensure the user's weight does not exceed the lift's capacity and remove any obstructions from under or around the lift.
The lift makes unusual noises during operation.	Components may be loose.	Inspect the lift for any loose parts and tighten as necessary.
The lift seat is not adjusting to the desired height	The adjustment mechanism is jammed or malfunctioning.	Check for any debris or foreign objects obstructing the mechanism. Clean and inspect the adjustment controls.

If any of the problems above persist, contact customer support for further assistance or consider professional servicing. For any additional questions, please contact us.

13.0 Limited Warranty

Thank you for your interest in the products and services of Climbing Steps, Inc. Your safety, comfort, and satisfaction are at the heart of everything we do. For the Argo Toilet Lift, Climbing Steps, Inc. extends the following warranty coverage, reflecting our commitment to quality and your satisfaction:

What does this Limited Warranty cover?	<ul style="list-style-type: none"> · Electronics: Enjoy peace of mind with a 6-month warranty against defects in materials and workmanship. · Welds: Our Lifetime Warranty on welds demonstrates our commitment to lasting quality and your safety.
What will we do to correct problems?	In the event of a defect, Climbing Steps, Inc. will repair or replace the affected product or part with either new or refurbished items, at no cost to you. Our aim is to ensure your complete satisfaction and to keep your equipment running flawlessly.
How long does the coverage last?	The Warranty Period offers a 180-day warranty on all products or parts from the date of purchase. Should a product or part be repaired or replaced, the new item will carry the remainder of the original product's warranty or 180 days from the date of repair or replacement, whichever is longer.
What does this Limited Warranty not cover?	This Warranty does not cover issues resulting from abnormal conditions, misuse, accidents, alterations, unauthorized repairs, or other damage not caused by defects in material or workmanship. The seat pads are recognized as subject to wear and tear, these components are crafted for endurance but not covered by the limited warranty.
What do you have to do?	If you require warranty service, please reach out to us for an evaluation of the issue and guidance on the best resolution. Our dedicated team is here to ensure your experience with our products is outstanding.

For any questions or to initiate a warranty claim, please contact us:

Email: (212) 366-5483

Phone: Info@ClimbingSteps.com

14.0 Device Label



The ArGo toilet lift is designed for individuals who experience difficulty or discomfort when bending or standing up from the toilet, such as those with limited mobility, joint pain, or balance issues. Its primary function is to provide a safe and effortless way to transition from standing to sitting and vice versa with the push of a button. This device is particularly beneficial for those who want to maintain their independence and privacy in the bathroom, offering a versatile solution that accommodates various toilet shapes and heights while ensuring stability and comfort.



Manufactured by: **Mobile Patient Lift** 6601 Lyons Rd, Suite C10, Coconut Creek, FL 33073



Please See Manual for Device Symbol Definitions

*Label may look different on the device.

Distributed by:

Mobile Patient Lift
 6601 Lyons Rd, Suite C10,
 Coconut Creek, FL 33073
 +1 (212) 366-5483

Manual Published Date

09/19/24

Have more questions? Contact us!

Email: Info@ClimbingSteps.com
Web: www.MobilePatientLift.com
Phone: +1 (212) 366-5483

Mail:
Mobile Patient Lift
6601 Lyons Rd, Suite C10,
Coconut Creek, FL 33073

Scan with your smartphone camera to view more information about the
Argo Toilet Lift!



or visit:
www.MobilePatientLift.com



MOBILE PATIENTLIFT

ARGO

www.MobilePatientLift.com