


C-600
Water quality tester



PAYOT

Usage


- Turn on the device;
- Remove the protective cap;
- Put the electrode in the solution;
- Stir gently and wait for the reading to stabilize; Read the value;
- Rinse the electrode with distilled water; and dry it with filter paper.
- Turn off the device and put on the protective cover.
- Keep it dry.

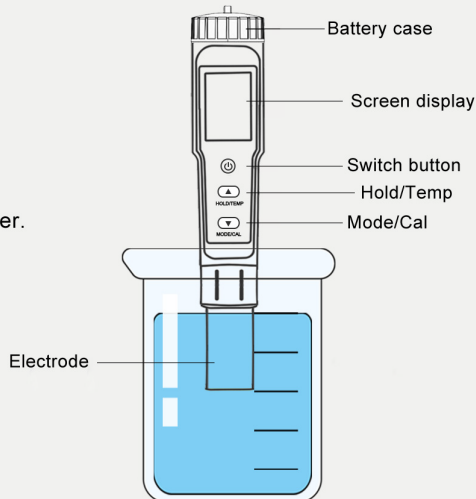

SPECIFICATIONS

C-600 pH/EC/TDS/Salt/Orp/S.G/Temp Meter			
	Range	Accuracy	Resolution
pH	0.00-14.00 pH	±0.05 pH	0.01 pH
EC	0-9990µS/cm; 10.01-19.99 mS/cm; 20.1-400.0 mS/cm	±2% F.S.	1µS/cm; 10µS/cm; 0.01mS/cm; 0.1mS/cm
TDS	0-999ppm; 1000-9990ppm; 10.1-200.0 ppt	±2% F.S.	1 ppm; 10ppm; 0.1ppt
Salt	0.01-25.00 %; 0-999 ppm; 1000-9990 ppm; 10.1-200.0 ppt	±2% F.S.	0.01 %; 1ppm; 10ppm; 0.1ppt
S.G	1.000-1.222		
ORP	-999mV~+999mV	15 mV	1 mV
Temp.	0.1°C-60.0°C; 32.1°F-140.0°F	±0.5°C	0.1°C; 0.1°F
Calibration	pH	3 points: 6.86/4.00/9.18	
	EC/TDS/Salt	1413µS/cm; 12.88 mS/cm; 111.8 mS/cm	
	ORP	256 mV	
ATC Temp.	0.1°C-60.0°C	Environment	0.1°C-60.0°C RH: max 90%
Waterproof	IP67	TDS Factor	0.5
Battery	3*1.5V (LR44) low battery indicator	Electrode	Replaceable
Dimensions/Weight	183*37*37mm (7.20*1.46*1.46in)/ 90g	Backlight	optional

TEMPERATURE (°C/°F)

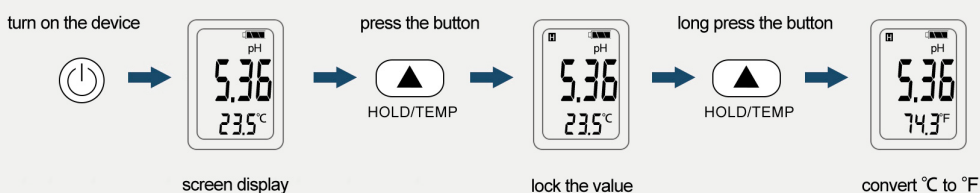

Note: The device has a memory function, the startup mode is last time shutdown mode.

MODE (pH/EC/TDS)

