



PRODUCT CATALOG
BONE LEVEL

AVP MEDICAL TECHNOLOGY

EXCLUSIVE EUROPEAN DEALER OF BIOINFINITY

avpmedtech.com



bioinfinityimplants.com



Avrupa Implant
İkitelli OSB HESKOP
M5 Blok No:82 34490
Basaksehir / Istanbul, Turkiye
Phone : +90 212 670 13 00 (pbx)
info@bioinfinityimplants.com

Rev. No: BPCENG-R003

EC REP mdi Europa GmbH

Langenhagener Str. 71 D-30855
Langenhagen - Germany
Phone: +49 511 39089530
E-mail: info@mdi-europa.com

avrupa implant is an  company
UMY MEDICAL

INTRODUCTION

An Uyg Uysal company, Avrupa Implant was established to manufacture high value-added products in various fields to the dental industry, particularly for Dental Implants.

Avrupa Implant, the main field of activity of which is Dental Implant systems, aims to produce scientific and technological R&D projects together with universities, improve itself and develop the industry, rise to the leading position in its field, and provide value and contribution to Turkiye in this sense, by following the technological developments closely.

Uyg Uysal, which was established in 1976, has gained experience in dental industry since 1999 as well as experience in dental implants, the success of which has been proven in the national and international arena, since 2001.

BioInfinity Dental Implant System, which was brought to life by the production experience of experts who have served in the medical-dental industry with Uyg Uysal for years, is taking firm steps further every day towards becoming a leading Implant brand with the innovative R&D studies executed in the light of scientific developments, with its professional manufacturing and quality control infrastructure, and strong sales, technical support and service networks.

Avrupa Implant owns essential knowledge and infrastructure needed to do more qualified and cost effective production in line with the needs of the sector as well as the expectations of the dentists in the dynamic developing dental sector.

Avrupa Implant has adopted achieving success in Turkiye and abroad as a principle with its corporate identity, experience and sense of quality by strictly adhering to the principles of Total Quality Management at every stage of the chain from product design to after-sales support.

BioInfinity Dental Implant System offers you and your patients a wide comfort in your clinic with its hybrid design, reverse buttress thread, mini thread on the platform part, OptimOss surface, ConFix connection, platform switch, concave abutment design, surgical and prosthetic stage color coding, torque ratchet that does not require calibrate and its more prosthetic superstructure options suitable for every indication.


There are many reasons to choose BioInfinity!

We hope you will enjoy reviewing our BioInfinity Bone Level product catalog...

Kind regards,



Fatih Uysal
Vice President, Sales and Marketing

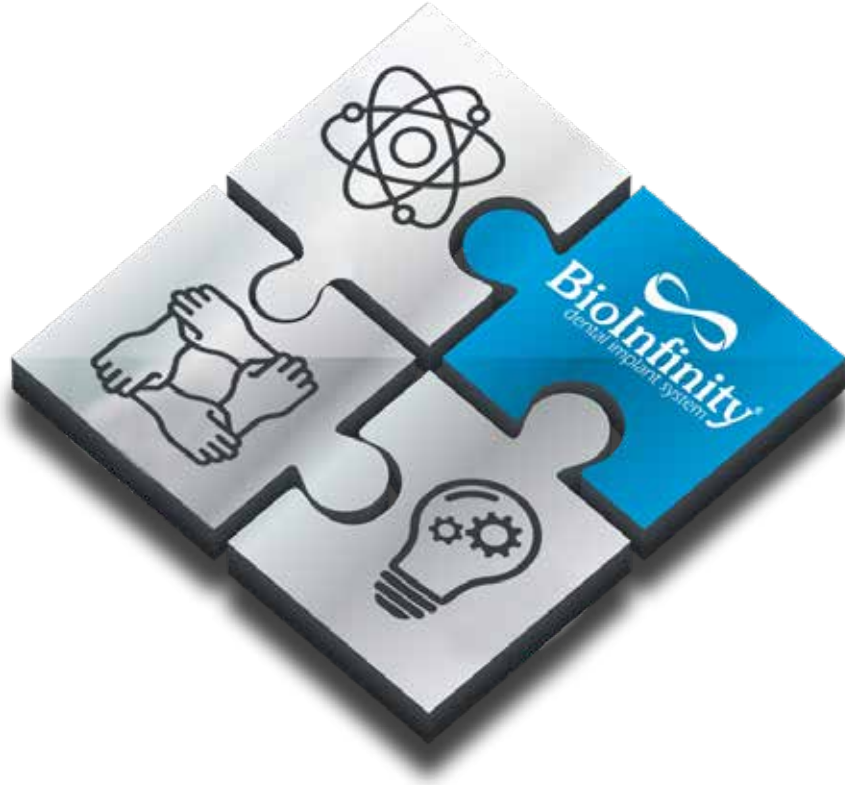

VISION

We adopt as a mission to achieve the leading position in the dental industry with our innovative works in line with the needs and expectations of dentists and patients by making a difference with the services and products we offer, and to represent Turkiye in the best way on national and international basis with the breakthroughs, adopting modern science, technology and humanely and moral values.

MISSION

As Avrupa Implant, we aim to increase the living quality of patients by giving priority to dentist and patient satisfaction from design of the products we produce within the framework of high quality standards to after-sales support.



QUALITY POLICY

As Avrupa Implant, human health is our main policy. We have adopted the principle of improving the living quality of patients by following the scientific and technological developments and providing failure-free, cost-effective and reliable products and services by improving our products in accordance with the needs and expectations of dentists and patients.

Our mission, commitment and policy is to continue our activities in accordance with human health and awareness of quality, laws and regulations, improving our processes with our entrepreneurial and innovative staff by keeping dentist and patient satisfaction as the utmost priority as well as increasing the efficiency of our quality management system.

CONTENT

1.....	Introduction	35.....	Torque Guide
2.....	Vision, Mission	36.....	Healing Abutment
3.....	Quality Policy	37.....	Transfer Coping, Lab Analog, Lab Abutment Screw
5.....	Quality Control	39.....	Straight Abutment
6.....	Clean Room	40.....	Angled Esthetic Abutment
7.....	Packaging	41.....	Temporary Abutment Titanium / PEEK, Abutment Holder
9/11.....	Bone Level Implant System	42.....	BioBall™ System
12/13.....	OptimOss™ Surface	44.....	BioLoc™ System
14.....	Hybrid Design	46/47.....	Multi Unit System, Bone Profiler Drill
15.....	Platform Switch	48.....	UMC - Uysal Milling Center
16.....	Mini Thread	49.....	TiBase Abutment, Custom Castable Abutment, Pre-milled Abutment
17.....	Reverse Buttress Thread	49.....	Scanbody, Digital Analog
18.....	ConFix™ Connection	50.....	Abutment Try-in Kit
19.....	Concentric Production	51.....	Washing and Sterilization
20.....	Concave Abutment	52.....	Osstell
21.....	Color Coding	53.....	Surgical Equipment
25/28.....	Surgical Kit	54.....	Advanced Implantology Academy
29.....	Drill Protocol	55.....	Symbols
30/31.....	Bone Level Short Implant System, Sinus Closing Screw	56/58.....	Product List





QUALITY CONTROL

In order to achieve the required standards and quality in the final product, BioInfinity Dental Implant System components are carefully examined by our quality control department with high precision technological devices throughout the entire production process.



CLEAN ROOM

BioInfinity Dental Implant System components are packaged in a clean room conforming to ISO Class 7 environmental requirements. Our clean room holds the criteria determined in international standards and is subject to validation periodically in order to keep the number of particles and microorganisms under control.

<http://ifu.avrupaimplants.com>



GS1
Singular Barcode



PACKAGING

Double sterile packaging method is used in the packaging of BioInfinity dental implants.

The risk of contamination of the Implant stored in the titanium tube is minimized.


The Implant package also includes a closing screw.

The 'peel and stick' type of labels on the Implant package contain the relevant product information and surgical and prosthetic color coding. This label should be affixed to the patient's clinical record file for future reference to product information.

In addition, the labels contain the unique barcode stipulated there is a singular barcode required on the labels.



You can access the user's manuals for the products via the electronic user manual card (e-IFU) included in the product package or directly via our website (<http://ifu.avrupaimplants.com>).



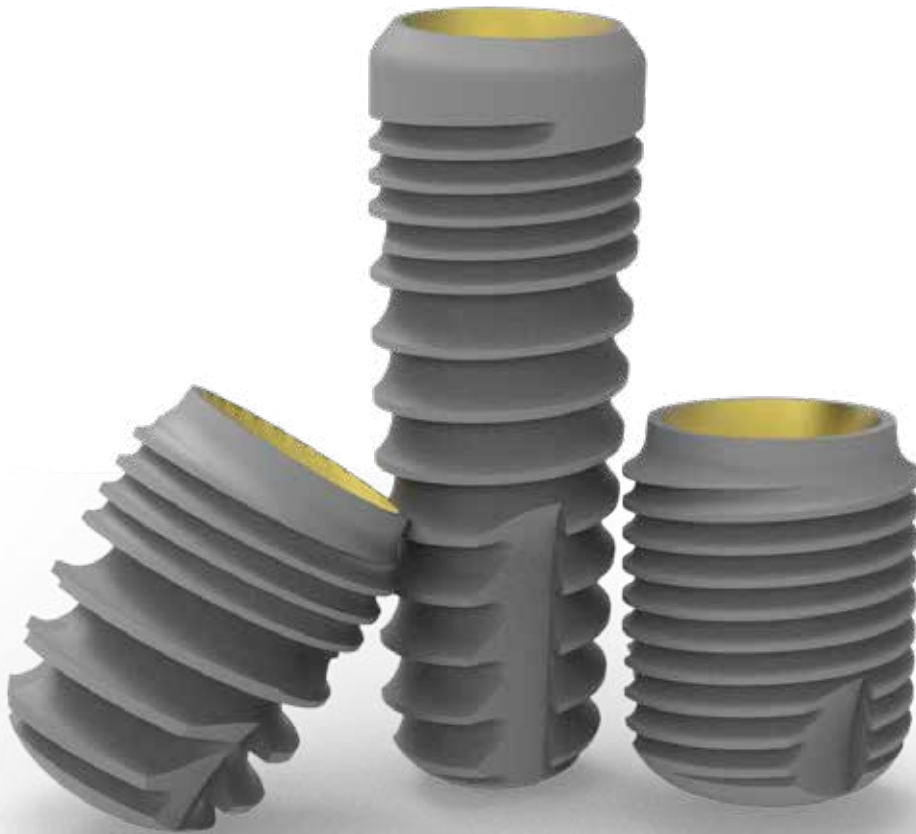


BONE LEVEL IMPLANT SYSTEM


BONE LEVEL IMPLANT SYSTEM

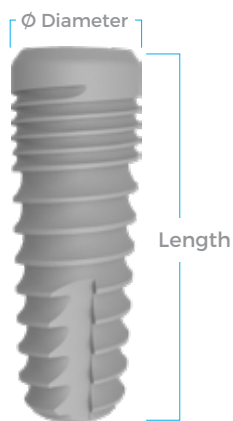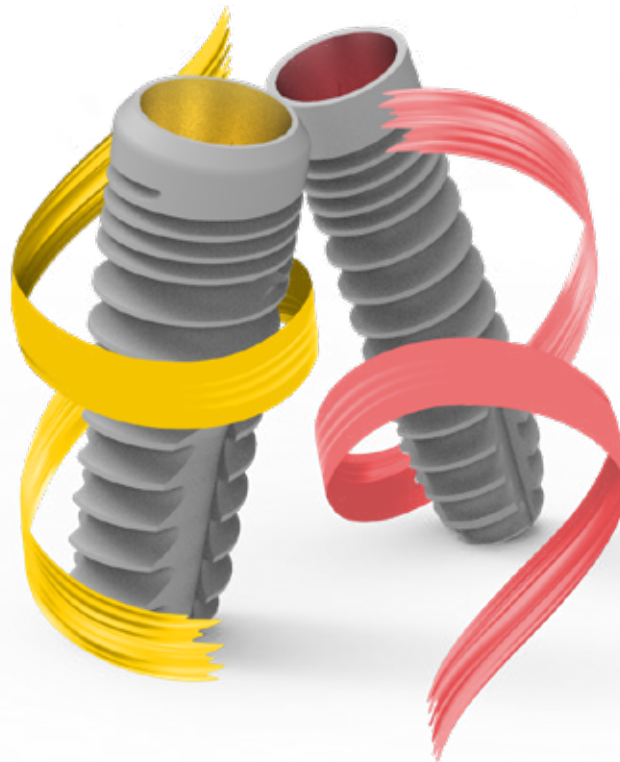


		Prosthetic Platform		BONE LEVEL		
		Junior	Standard			
		J	S			
		Ø 3.2	Ø 3.7	Ø 4.2	Ø 4.7	Ø 5.2
Length	8 mm		•	•	•	•
	10 mm	•	•	•	•	•
	12 mm	•	•	•	•	•
	14 mm	•	•	•	•	•
	16 mm	•	•	•	•	

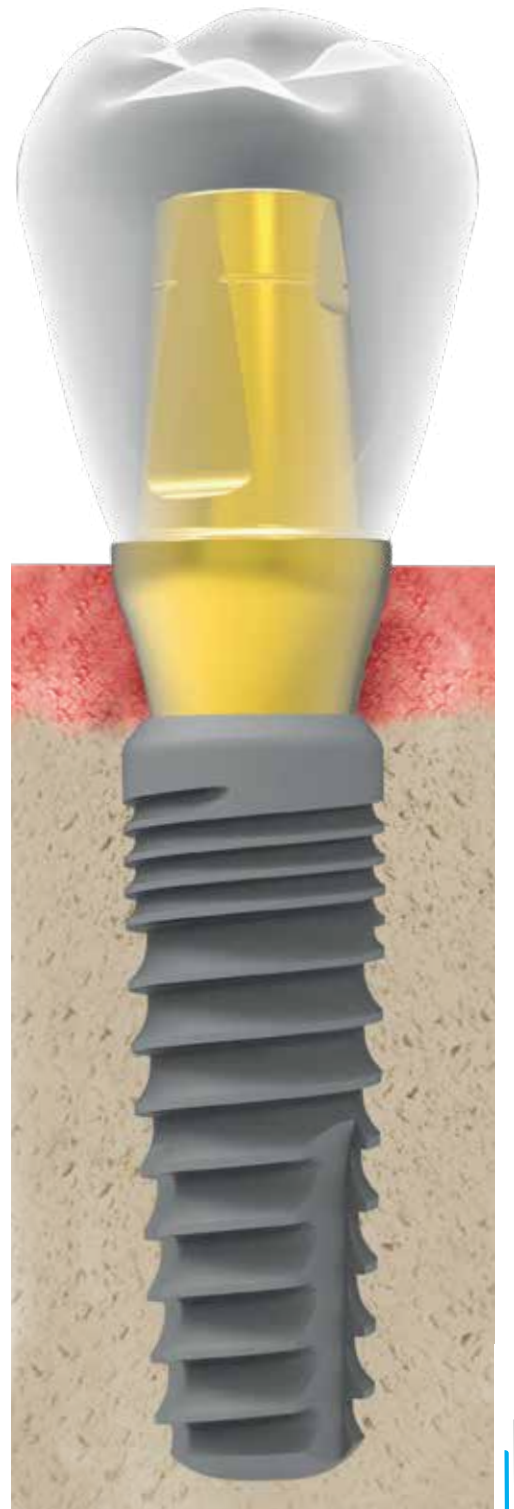


OptimOss™ Surface



Mini Thread




Concentric Production



Hybrid Design



Reverse Buttress Thread




Concave Abutment



Platform Switch



ConFix™ Connection




Color Coding




BONE LEVEL

OPTIMOSSTM SURFACE


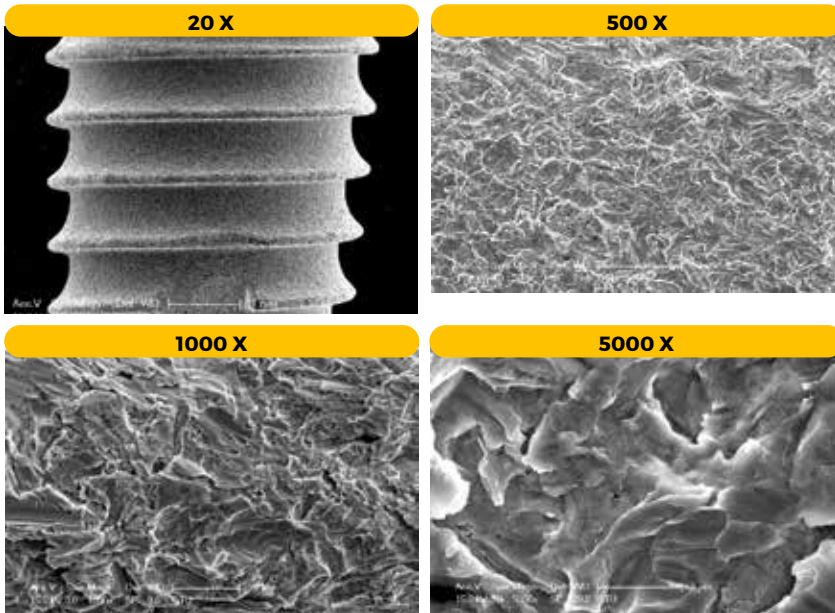


Surface technical knowledge of BioInfinity dental implants is based on surface technology transferred from the United States.



Our biocompatible, osteoconductive and resorbable BCP (Biphasic Calcium Phosphate) roughened surface contributes positively to osseointegration.

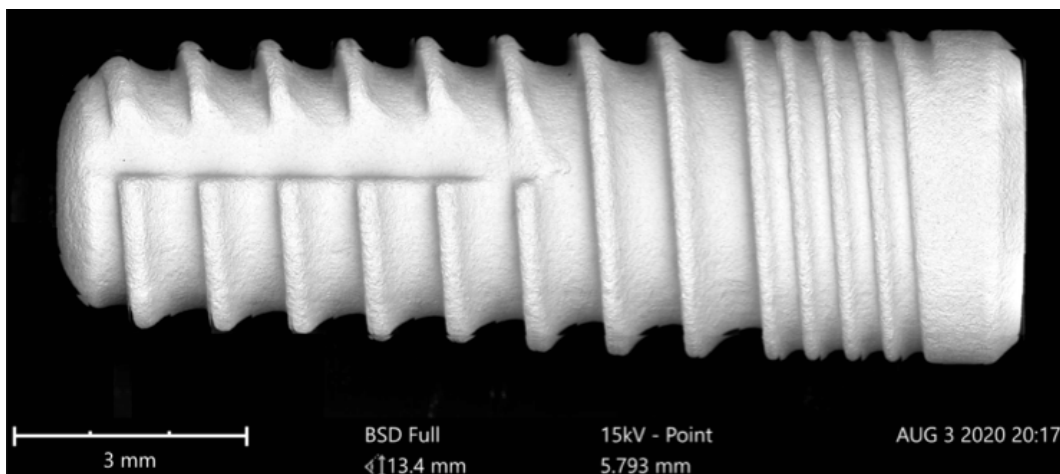

BioInfinity implant image is taken from Clean Implant "Implant Study 2017-2019" Report.

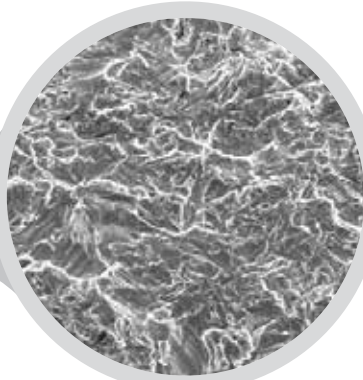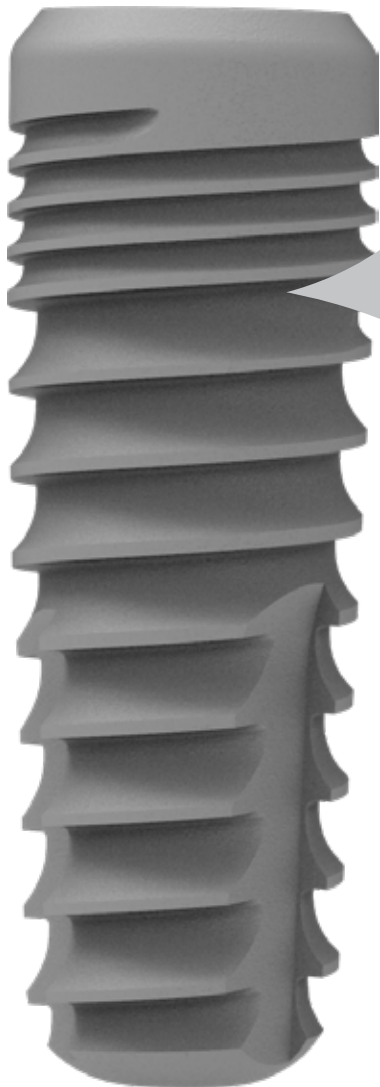

Histologic cross-sectional image of osseointegration at 12 weeks*

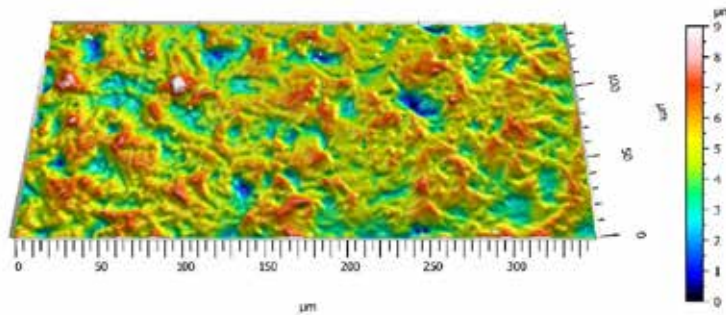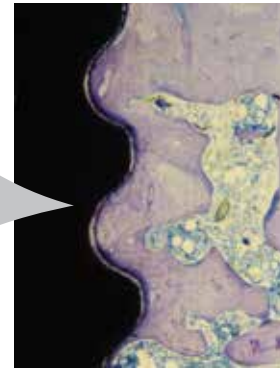

ISO 25178		
Höhen-Parameter		
Sa	1.589671	um




It is frequently suggested in the literature that dental implants with moderate surface roughness contribute positively to osseointegration.

Scientific studies performed in İstanbul Technical University have shown that BioInfinity dental implants have moderate surface roughness (Sa / 1-2 μm) and homogeneous surface morphology.

BioInfinity dental implants with roughness measurement after surface treatment are guaranteed to have the desired roughness value.

*Dundar Serkan, et al. "Comparison of Osseointegration of Five Different Surfaced Titanium Implants." The Journal of Craniofacial Surgery 29.7 (2018): 1991-1995.


**Salimov Fariz, et al. "The effects of repeated usage of Implant drills on cortical bone temperature, primary/secondary stability and bone healing: A preclinical in vivo micro-CT study" © 2020 John Wiley & Sons A/S. Published by John Wiley & Sons Ltd., Clin Oral Impl Res. 2020;00:1-7. DOI: 10.1111/clr.13603

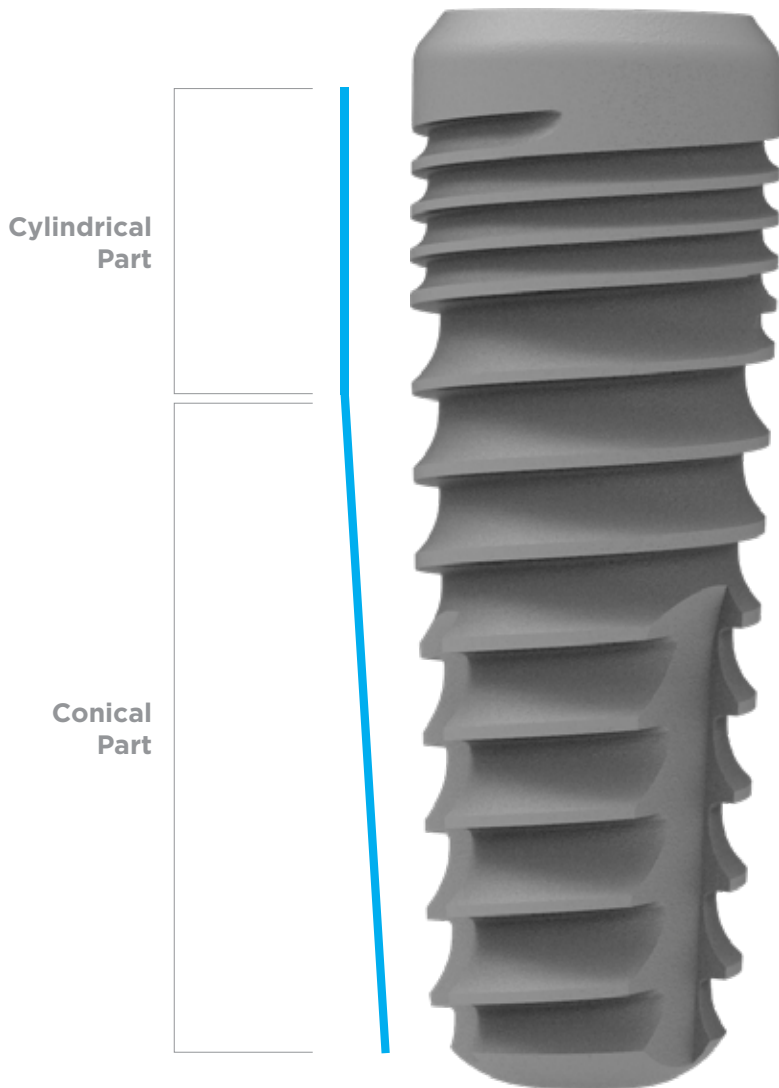

HYBRID DESIGN

Implants with conical designs can be placed in the jawbone faster, reducing the Implantation time. Implants with cylindrical design provide more surface area and contribute positively to osseointegration.

BioInfinity dental implants have a hybrid design with an ideal combination of conical and cylindrical forms. With hybrid design, the Implant placement time is reduced, the Implant engages to the jawbone with minimum stress and maximum primary stability is achieved.

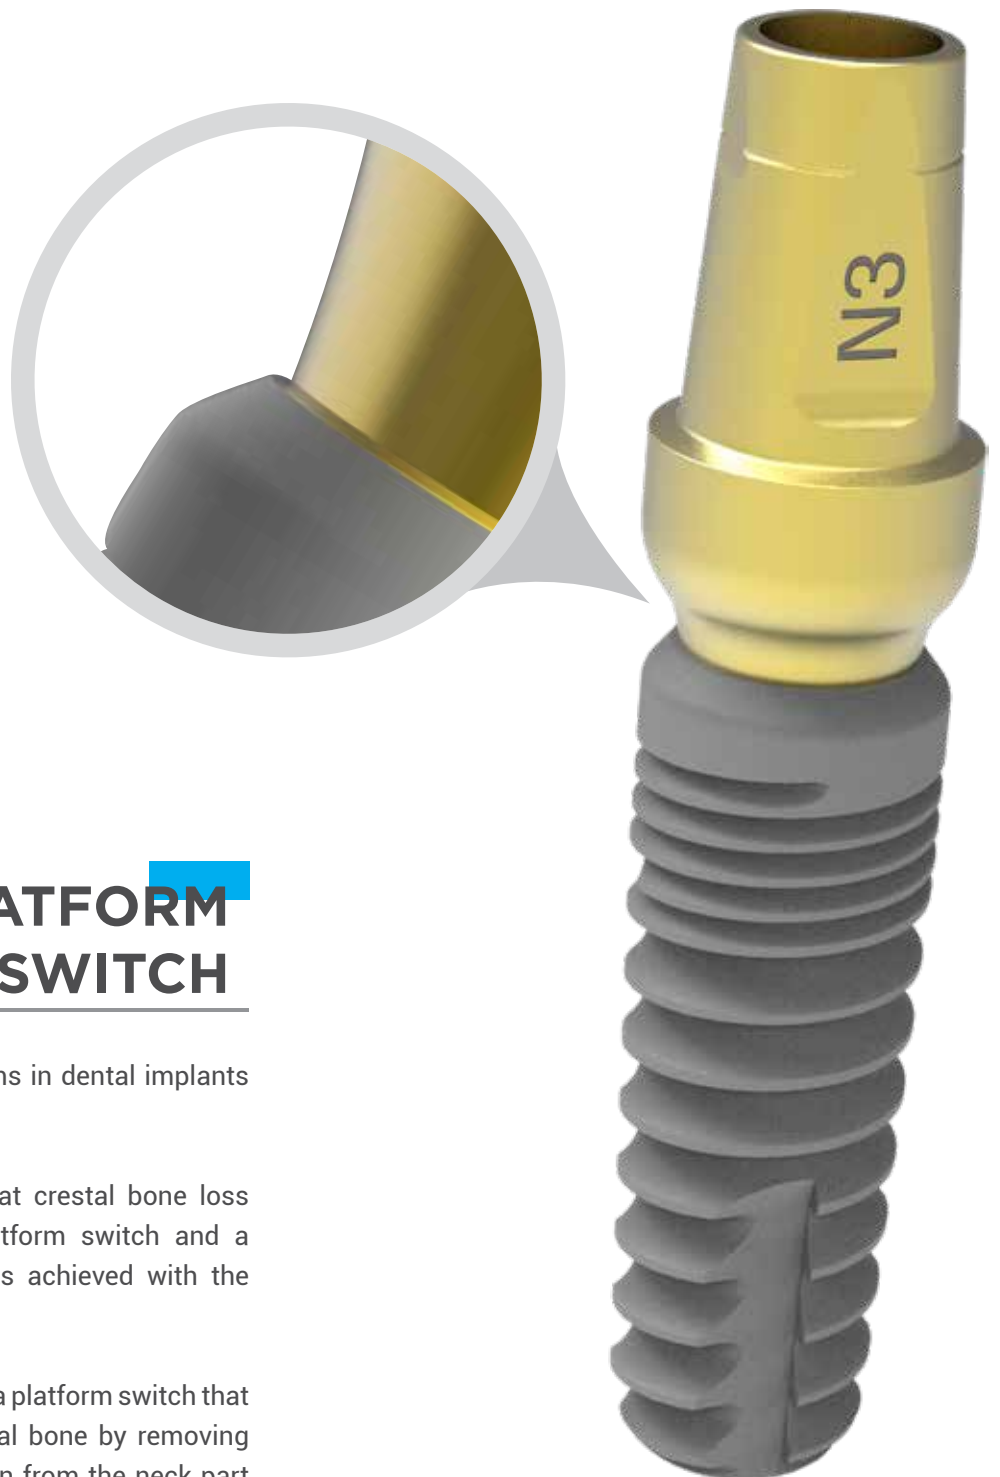

PLATFORM SWITCH

One of the most common problems in dental implants is crestal bone loss.


Scientific studies have shown that crestal bone loss is less in the Implants with platform switch and a successful esthetic appearance is achieved with the gingival papilla being preserved.

BioInfinity dental implants feature a platform switch that minimizes resorption in the crestal bone by removing the implant - abutment connection from the neck part of the implant.

MINI THREAD

The mini threads on the neck of BioInfinity dental implant ensure the protection of marginal bone and soft tissue.

The optimal load distribution provided by the mini threads reduces the marginal bone loss.


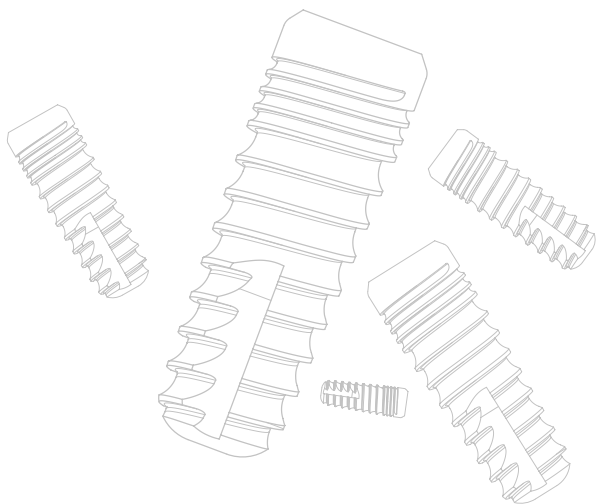


REVERSE BUTTRESS THREAD

BioInfinity dental implants feature a wide, self-cutting, reverse buttress thread design.


With reverse buttress wide grooves;

- Minimal stress occurs between the bone and the Implant while the Implant is placed in the jaw bone, since the Implant is placed by cutting instead of rubbing.
- The surface area is increased, thus providing a positive contribution to osseointegration.
- Maximum primary from stability is achieved from by the not only the apex but also the grooves.
- High resistance is shown against tensile forces, leading to immediate loading.
- Advantage of a more secured use is provided on the sinus base.

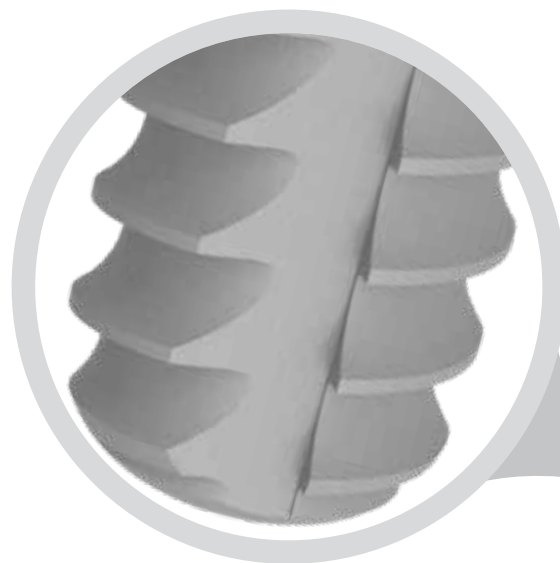

According to finite element analysis studies, it has been observed that single thread implants give better results when it comes to Implant stability.

* Ma, P., Liu, H.C., Li, D.H., Lin, S., Shi, Z. & Peng, Q.J. (2007) influence of helix angle and density on primary stability of immediately loaded Dental Implants: Three-dimensional finite element analysis. Zhonghua Kou Qiang Yi Xue Za Zhi 42: 618-621.

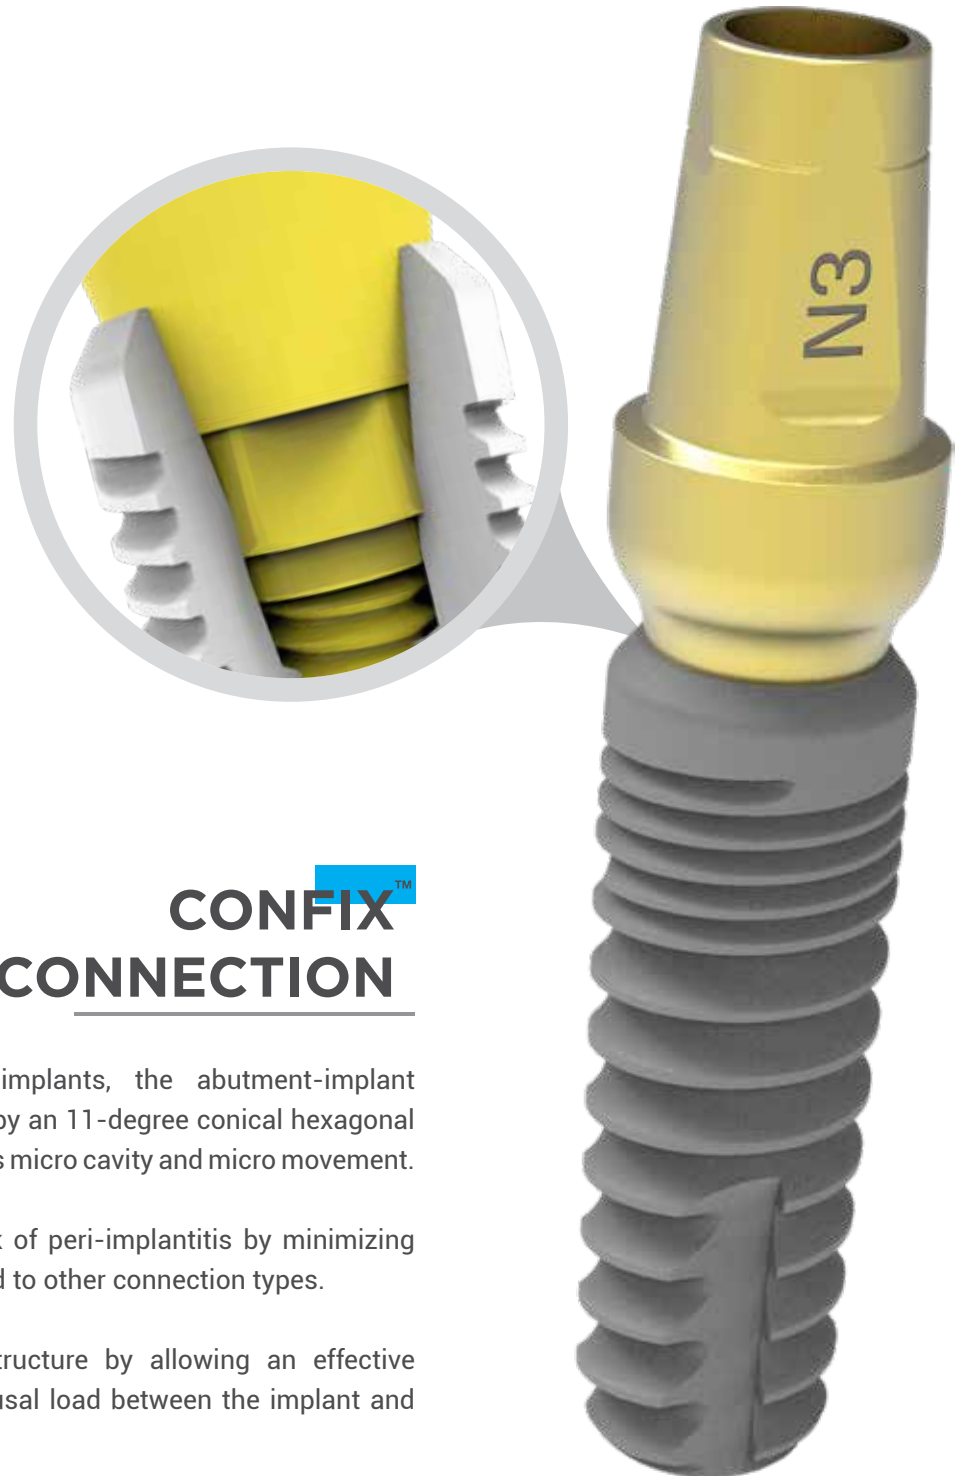


CONFIX[™] CONNECTION

In BioInfinity dental implants, the abutment-implant connection is provided by an 11-degree conical hexagonal connection that prevents micro cavity and micro movement.

ConFix reduces the risk of peri-implantitis by minimizing micro leakage compared to other connection types.

ConFix protects the structure by allowing an effective distribution of the occlusal load between the implant and the abutment.

ConFix provides sufficient surface area between the implant and abutment to resist lateral movements and protects the abutment screw against shear forces. The conical hexagonal structure minimizes screw loosening by preventing rotation of abutment.

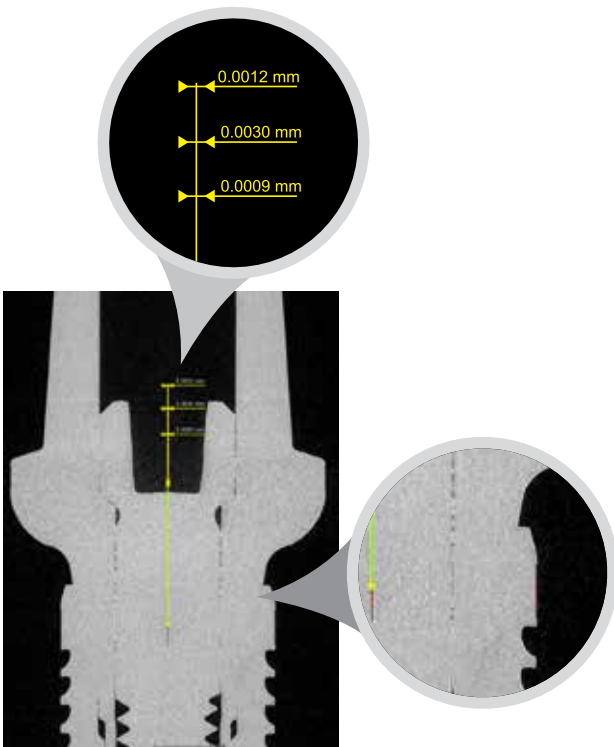


CT (Computerized Tomography) image of the torqued implant - abutment connection with 25 Ncm

CONCENTRIC PRODUCTION

Scientific studies show that most of the loads on the implant are concentrated on the abutment screw, which provides the implant-abutment connection. When the reasons for the failure of dental implants are examined, it is seen that the most common problem is screw-implant breakage. The reason for this is the inhomogeneous load distribution due to the lack of concentricity in the implant - abutment connection.

Concentricity between implant and abutment in BioInfinity dental implants has been achieved as a result of R&D studies and improvements in production, and the difference between centers has been minimized. In our quality control department, concentricity is guaranteed in BioInfinity dental implants with high precision technological devices.

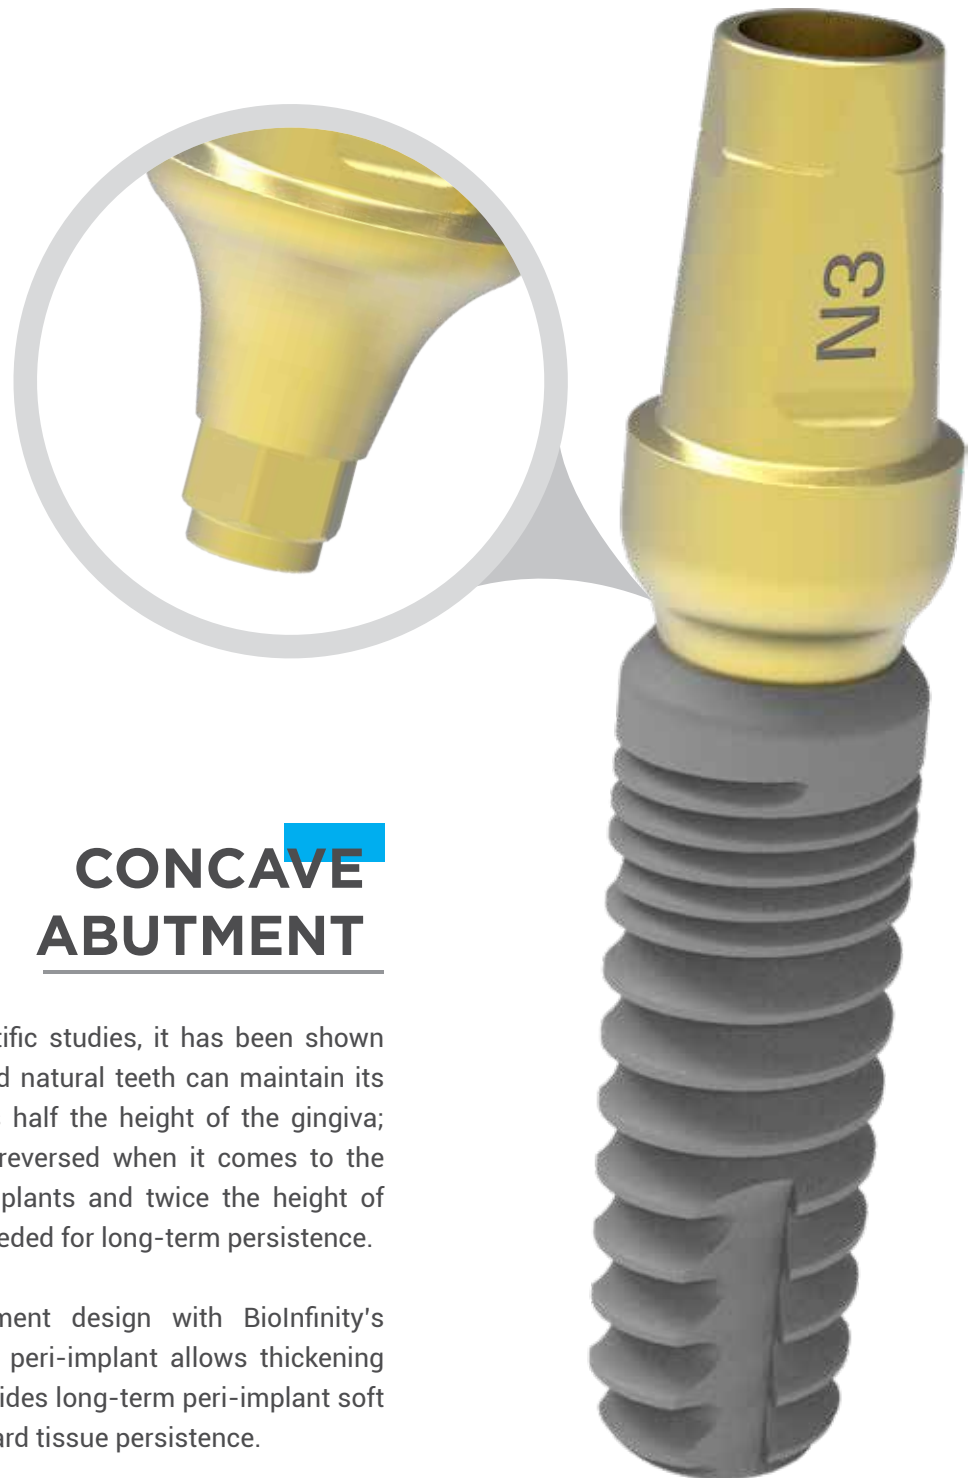

CONCAVE ABUTMENT

As the result of scientific studies, it has been shown that the gingiva around natural teeth can maintain its health even when it is half the height of the gingiva; however, this ratio is reversed when it comes to the gingiva around the implants and twice the height of gingiva thickness is needed for long-term persistence.

Thanks to the abutment design with BioInfinity's concave outlet profile, peri-implant allows thickening of the gingiva and provides long-term peri-implant soft tissue, and therefore hard tissue persistence.


In addition, BioInfinity's cemented abutments with different gingiva heights for each indication make it possible to avoid the risk of flood cement residues, which are the primary cause of peri-implantitis.








COLOR CODING

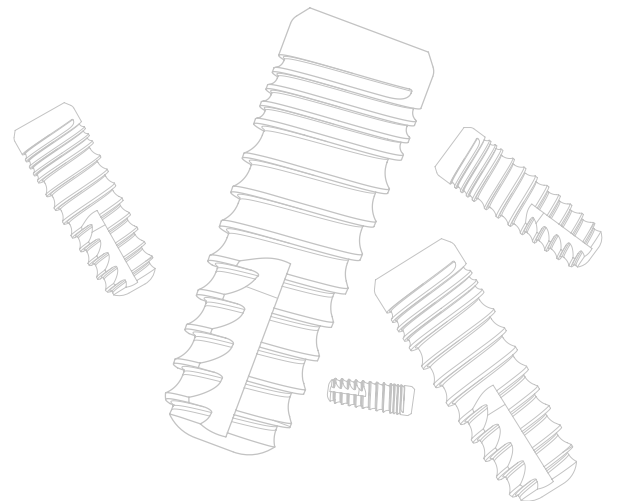



























All components on BioInfinity Dental Implant System have color coding.

Color coding provides simple, fast and reliable application in surgical and prosthetic applications.




	J	S			
Prosthetic Color Code	Junior	Standard			
Surgical Color Code	Ø 3.2	Ø 3.7	Ø 4.2	Ø 4.7	Ø 5.2
BONE LEVEL					

BONE LEVEL IMPLANT SYSTEM

Length	8 mm	10 mm	12 mm	14 mm	16 mm
					
		BR3210	BR3212	BR3214	BR3216
					
	BR3708	BR3710	BR3712	BR3714	BR3716
					
	BR4208	BR4210	BR4212	BR4214	BR4216
					
	BR4708	BR4710	BR4712	BR4714	BR4716
					
	BR5208	BR5210	BR5212	BR5214	

Closing Screw



* Implants are packaged with a closing screw
* Ti-Gr 23 (Ti6Al4V ELI)



CNC / MACHINING CENTER



BONE LEVEL IMPLANT SYSTEM

SURGICAL



Bone Level Surgical Kit

	Starter	Pilot	Junior Platform					Standard Platform	Hex Drivers
Fissure	8 mm	PD							
FD	SD2208								12HDS-S
Round	10 mm	Drill	3.2	3.7	4.2	4.7	5.2		
RD	SD2210	SD32	CD37	CD42	CD47	CD52			12HDL-L
Lindemann	12 mm	Depth Gauge	Depth Gauge	Depth Gauge	Depth Gauge	Depth Gauge			
LD	SD2212	DG32	DG37	DG42	DG47	DG52			12HDR-S
Drill Extender	14 mm	Counter Sink	Counter Sink	Counter Sink	Counter Sink	Counter Sink			
DE	SD2214	CS32	CS37	CS42	CS47	CS52			12HDR-L
Hand Wrench	16 mm	Tap	Tap	Tap	Tap	Tap			
TAPHW	SD2216	TAP32	TAP37	TAP42	TAP47	TAP52			
Pin 0°	Pin 17°	Spare							
PP2228	BMU17PP								
Pin 0°	Pin 30°	Spare							
PP2228	BMU30PP								

BSK2000



The color coding of the implant diameters are available on drills, depth gauges, counter sinks and taps




8, 10, 12 and 14 mm starter drills have stopper, 16mm ones don't stopper


Junior (J) | **Standard** (S)



The color coding of the implant drivers is the same as the prosthetic platforms of the implants



The fact that either one of the 6 channels on the implant drivers corresponds to the buccal provides more optimal positioning of the angled abutments

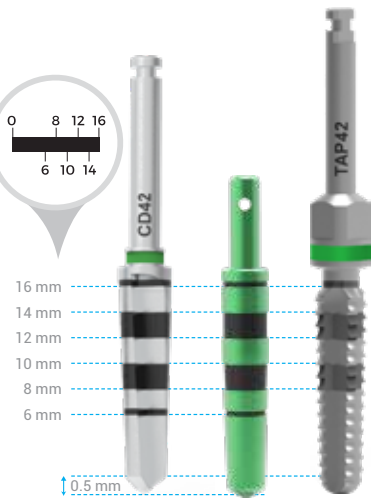

Drill length is 0.5mm longer than implant length

The laser lines on the drills and taps are designed to ensure secure application



Implant Handle

Product Code | SPH1000

Designed for implant placement in the upper jaw anterior region




Surgical and Prosthetic Torque Ratchet

Product Code | SPTR

Starter Drill



Final Drill

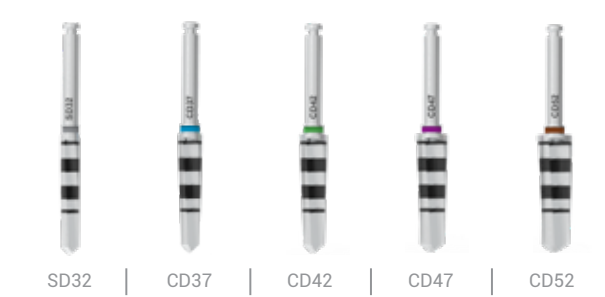

Depth Gauge




Counter Sink




Tap




Drill

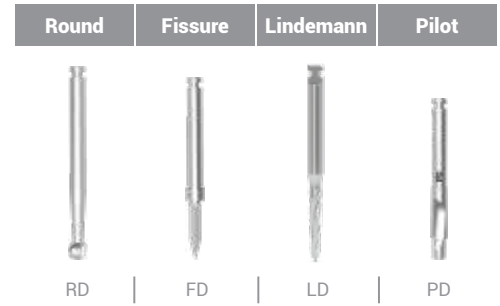


Implant Driver

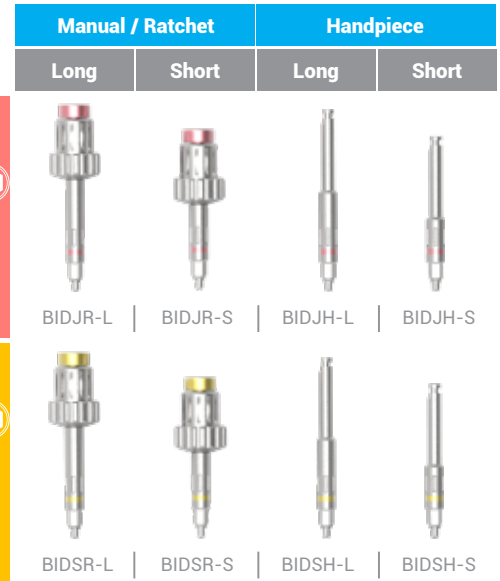


Hex Driver

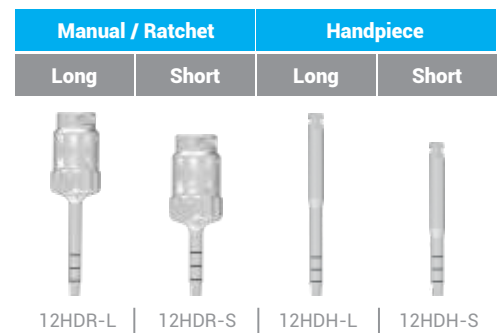


Pin

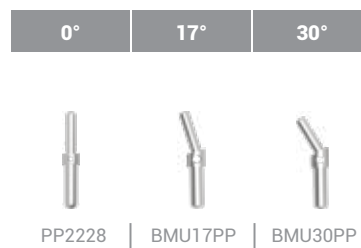



Other

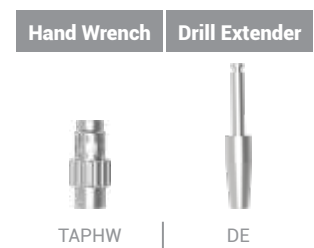

DRILL PROTOCOL

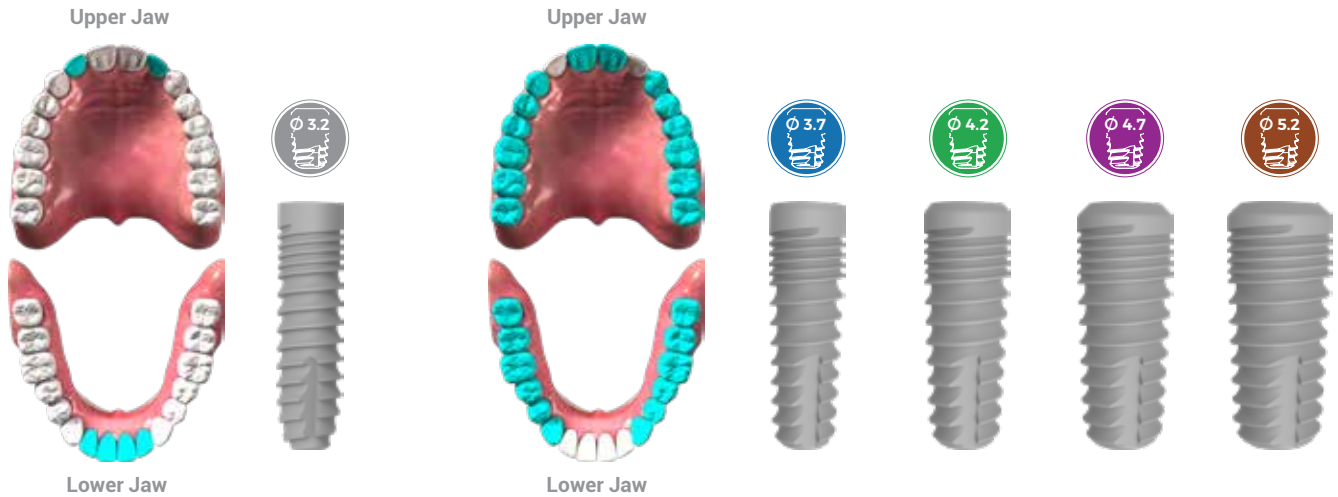

* It is recommended to use Ø 3.2 implant in the upper jaw lateral, lower jaw central and lateral

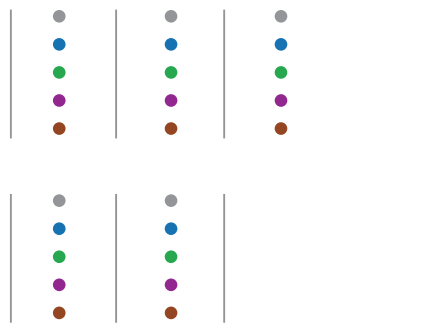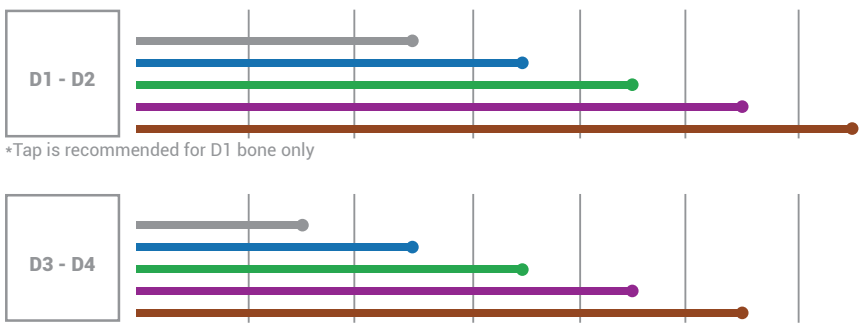

*Tap is recommended for D1 bone only

BONE LEVEL SHORT IMPLANT SYSTEM






BONE LEVEL SHORT HARD

Standard **S**

Ø 4.2	Ø 4.7	Ø 5.2
-------	-------	-------

6 mm




		
BR4206H	BR4706H	BR5206H

BONE LEVEL SHORT SOFT

Standard **S**

Ø 4.2	Ø 4.7	Ø 5.2
-------	-------	-------

6 mm

		
BR4206S	BR4706S	BR5206S



Surgical Kit Short

Product Code | BSSKIT



Drill Protocol Short Implant										
	Starter Drill	Pilot Drill	3.2 Drill	3.7 Drill	4.2 Drill	4.2 Drill Short	4.7 Drill	4.7 Drill Short	5.2 Drill	5.2 Drill Short
	SD2206	PD	SD32	CD37	CD42	SSD42	CD47	SSD47	CD52	SSD52
Ø 4.2	•	•	•	•	•	•				
Ø 4.7	•	•	•	•	•		•	•		
Ø 5.2	•	•	•	•	•		•		•	•

Tap is recommended for D1 bone only



BSCS0 | BSCS1

* Designed to the implant placement on the sinus floor in safety
* Ti-Gr 23 (Ti6Al4V ELI)

SINUS CLOSING SCREW



QUALITY CONTROL CENTER




BONE LEVEL IMPLANT SYSTEM

PROSTHESIS




Prosthetic Color	Junior (J)		Standard (S)	
Emergence Profile	Narrow (N)	Narrow (N)	Regular (R)	Wide (W)
Emergence Profile Ø	Ø 4.0	Ø 4.5	Ø 5.5	Ø 6.5

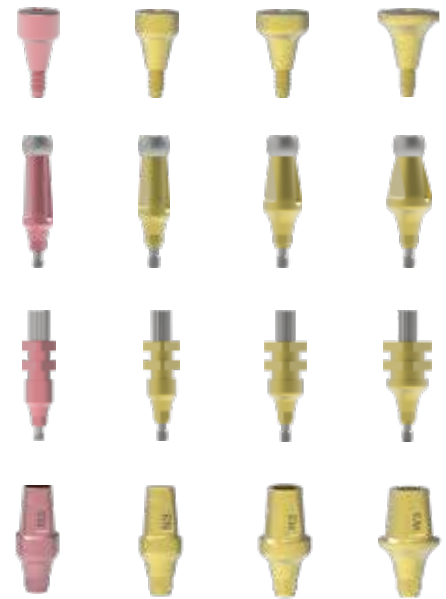


It is necessary to use a healing abutment and transfer coping with an emergence profile the same as abutment you prefer




Color coding and laser marking in prosthetic parts provide simple, fast and reliable application in prosthetic applications

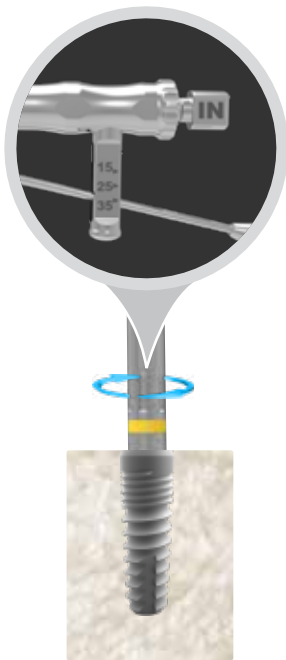

Implant Placement
≤ 35 Ncm

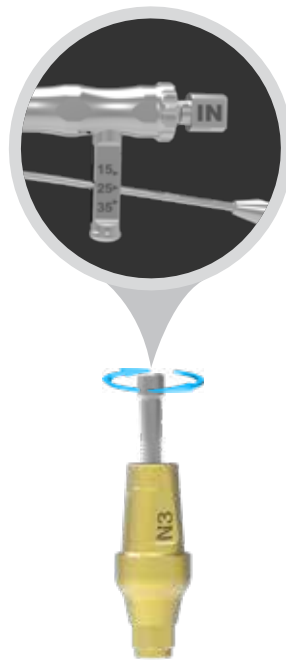

Implant Level Final Restorations
25 Ncm

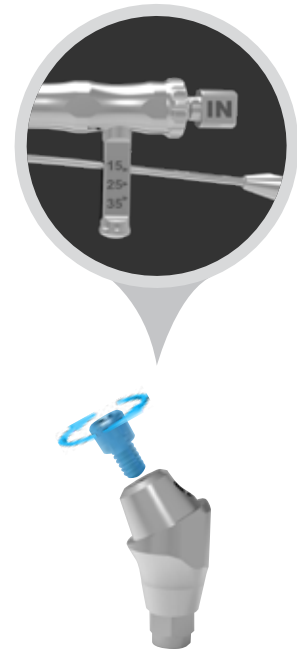


Abutment Level Final Restorations
15 Ncm


Torque Guide	
Application	Torque Value*
Implant Placement	≤ 35 Ncm
Healing Abutment	Manually (5 - 10 Ncm)
Temporary Restorations	15 Ncm
Implant Level Final Restorations	25 Ncm
Abutment Level Final Restorations	15 Ncm

*Recommended torque values



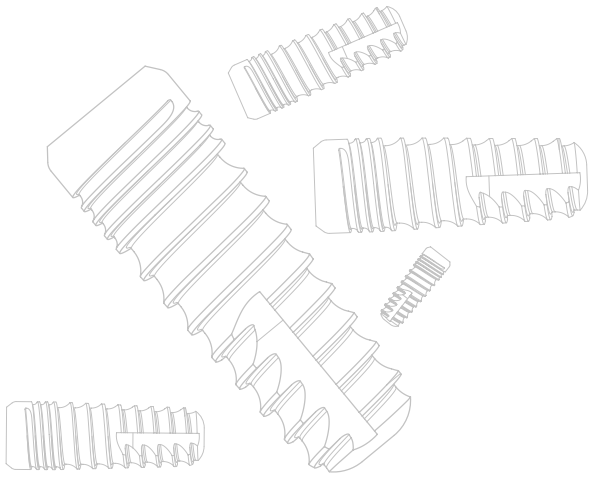

HEALING ABUTMENT



The laser marks on the hex drivers are designed to select the appropriate height of healing abutments



Gingival Height	1 mm	2 mm	3 mm	4 mm	5 mm	7 mm
Narrow	BHAJN1	BHAJN2	BHAJN3	BHAJN4	BHAJN5	BHAJN7
Narrow	BHASN1	BHASN2	BHASN3	BHASN4	BHASN5	BHASN7
Regular	BHASR2	BHASR3	BHASR4	BHASR5	BHASR7	
Wide		BHASW3	BHASW4	BHASW5	BHASW7	

* Ti-Gr 23 (Ti6Al4V ELI)
* Torque value: Manually (5 - 10 Ncm)


TRANSFER COPING

Closed Tray




- * Closed tray technique is used to take impression at implant level
- * It is packaged with BTCScJ for junior platforms and with BTCScS transfer coping screw for standard platform
- * Ti-Gr 23 (Ti6Al4V ELI)
- * Screw torque value: Manually (5 - 10 Ncm)

Open Tray

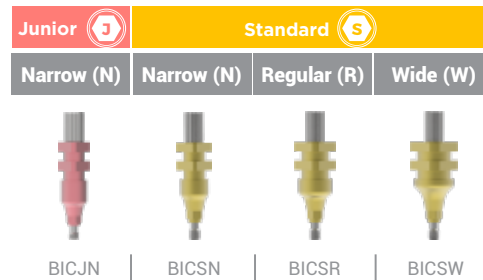

- * Open tray technique is used to take impression at implant level
- * It is packaged with BICScJ for junior platforms and with BICScS transfer coping screw for standard platform
- * Ti-Gr 23 (Ti6Al4V ELI)
- * Screw torque value: Manually (5 - 10 Ncm)


Lab Analog



- * Ti-Gr 23 (Ti6Al4V ELI)

LAB ANALOG

Lab Abutment Screw



- * Ti-Gr 23 (Ti6Al4V ELI)

LAB ABUTMENT SCREW
























LABORATORY

STRAIGHT ABUTMENT



Straight Abutment


Gingival Height	1 mm	2 mm	3 mm	4 mm	5 mm	
Narrow 						
	BSAJN1	BSAJN2	BSAJN3	BSAJN4	BSAJN5	
	Narrow 					
		BSASN1	BSASN2	BSASN3	BSASN4	BSASN5
		Regular 				
BSASR2			BSASR3	BSASR4	BSASR5	
Wide 						
			BSASW3	BSASW4	BSASW5	

- * Used to create a cement-retained, single or multiple-unit prostheses
- * Packaged with an abutment screw, BASJ for junior platform and BASS for standard platform
- * Ti-Gr 23 (Ti6Al4V ELI)
- * Screw torque value: 25 Ncm

ANGLED ESTHETIC ABUTMENT

Angled Esthetic Abutment 15°

Gingival Height	1/2 mm	2/3 mm	3/4 mm	4/5 mm
-----------------	--------	--------	--------	--------

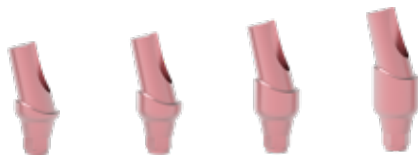

Narrow



BAEJ15N12 | BAEJ15N23 | BAEJ15N34 | BAEJ15N45



Narrow



BAES15N12 | BAES15N23 | BAES15N34 | BAES15N45



Regular



BAES15R23 | BAES15R34 | BAES15R45



Wide



BAES15W34 | BAES15W45

Angled Esthetic Abutment 25°

1/2 mm	2/3 mm	3/4 mm	4/5 mm
--------	--------	--------	--------



BAES25N12 | BAES25N23 | BAES25N34 | BAES25N45




BAES25R23 | BAES25R34 | BAES25R45



BAES25W34 | BAES25W45

- * Used to create a cement-retained, single or multiple-unit prostheses
- * Packaged with an abutment screw, BASJ for junior platform and BASS for standard platform
- * Ti-Gr 23 (Ti6Al4V ELI)
- * Screw torque value: 25 Ncm

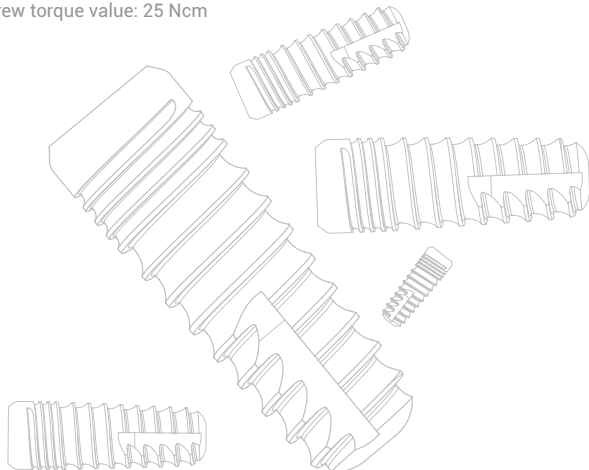

Abutment Screw

Junior



Standard



BASJ





BASS

- * Ti-Gr 23 (Ti6Al4V ELI)
- * Screw torque value: 25 Ncm

TEMPORARY ABUTMENT

Temporary Abutment - Titanium

Junior (J)		Standard (S)				
Narrow (N)		Narrow (N)		Regular (R)		Wide (W)
1 mm	3 mm	1 mm	3 mm	2 mm	4 mm	3 mm

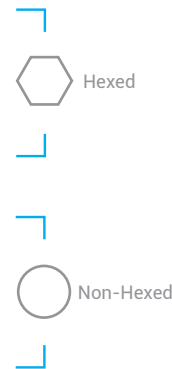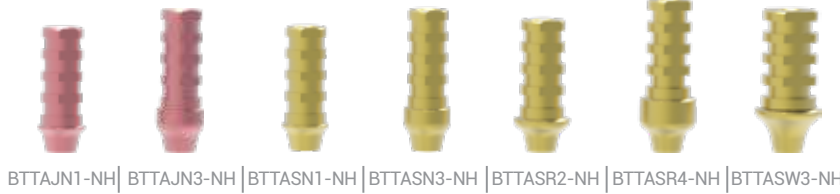

- * Use hexed abutments for single-unit, screw-retained or cement-retained, custom abutment restorations
- * Use non-hexed abutment for multiple unit, screw-retained restorations
- * Packaged with an abutment screw, BASJ for junior platform and BASS for standard platform
- * Ti-Gr 23 (Ti6Al4V ELI)
- * Screw torque value: 25 Ncm




Abutment Holder

Product Code | BTAH

Designed to modification of the temporary abutment

Temporary Abutment - PEEK



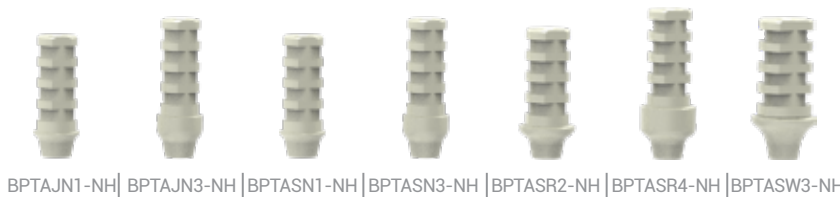









Junior (J)		Standard (S)				
Narrow (N)		Narrow (N)		Regular (R)		Wide (W)
1 mm	3 mm	1 mm	3 mm	2 mm	4 mm	3 mm




- * Use for fabrication of cement or screw-retained provisional restorations (up to 30 days)
- * Use hexed abutments for single-unit, screw-retained or cement-retained, custom abutment restorations
- * Use non-hexed abutment for multiple unit, screw-retained restorations
- * Packaged with an abutment screw, BASJ for junior platform and BASS for standard platform
- * Ti-Gr 23 (Ti6Al4V ELI)
- * Screw torque value: 25 Ncm

**BIOBALL™
SYSTEM**

BioBall™ Abutment

Gingival Height	1 mm	2 mm	3 mm	4 mm	5 mm
					
Junior 	BBAJN1	BBAJN2	BBAJN3	BBAJN4	BBAJN5
					
Standard 	BBASN1	BBASN2	BBASN3	BBASN4	BBASN5

- * Use for retention of implant supported overdentures
- * Packaged with BioBall Set
- * Ti-Gr 23 (Ti6Al4V ELI)
- * Torque value: 25 Ncm

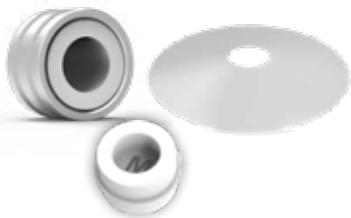

BioBall Set

Product Code | BBSET

- * Includes; Metal Housing (with L BioBall insert), Protective Disc, M BioBall PEEK insert







BioBall Lab Analog

Product Code | BBLA

- * Ti-Gr 23 (Ti6Al4V ELI)

BioBall™ PEEK Insert

L	S	M	H
For Lab	Soft Retention	Medium Retention	High Retention
	600 gram	1000 gram	1400 gram
			
BBL4	BBS4	BBM4	BBH4

- * 4 per package
- * Medical Grade PEEK

BioMatrix™

Overdenture Solutions

BioBall™ PEEK inserts

compatible with
Ø2.5 mm ball abutment of
all implant brands



RHEIN83

 Rhein83



Ball Abutment Set

Product Code | BBASET

Includes; Inox Housing, Black nylon insert,
Pink nylon insert, Clear nylon insert, Protective disc

Ball Abutment Nylon Insert

Black	Pink	Clear
For Lab	900 gram	1300 gram
		
BBANI-B	BBANI-P	BBANI-C

BIOLOC™
SYSTEM



BioLoc™ Abutment

Gingival Height	1 mm	2 mm	3 mm	4 mm	5 mm	6 mm	Angled 1.5 mm	Angled 3 mm
-----------------	------	------	------	------	------	------	---------------	-------------



Junior

BLOAJ1 | BLOAJ2 | BLOAJ3 | BLOAJ4 | BLOAJ5 | BLOAJ6 | BLOAS15J1.5 | BLOAS15J3



Standard

BLOAS1 | BLOAS2 | BLOAS3 | BLOAS4 | BLOAS5 | BLOAS6 | BLOAS15S1.5 | BLOAS15S3

- * Use with overdentures or partial dentures retained whole or in part by dental implants in the mandible or maxilla
- * Packaged BioLoc angled abutment with an abutment screw, BASJ for junior platform and BASS for standard platform
- * TiN coated
- * Ti-Gr 23 (Ti6Al4V ELI)
- * Torque value: 25 Ncm



Hex Driver is used to carry and torque the BioLoc abutment, no special driver is needed!



BioLoc Set

Product Code | BLSET

- * Includes; Metal Housing (with L BioLoc insert), Protective disc, S-M-H BioLoc PEEK inserts



BioLoc Set Mini

Product Code | BLSET-ECO

- * Includes; Metal Housing (with L BioLoc insert), Protective disc, M BioLoc PEEK insert

BioLoc™ Parts

Transfer Coping	Lab Analog
-----------------	------------



BLOT | BLOLA

BioLoc™ PEEK Insert

L	S	M	H
---	---	---	---

For Lab Soft Retention Medium Retention High Retention
700 gram 1400 gram 2300 gram




BLL4 | BLS4 | BLM4 | BLH4

- * 4 per package
- * Medical Grade PEEK


Insert Handle



Product Code | KMT002



For insertion



For remove

BioMatrix™ Overdenture Solutions

BioLoc™ PEEK inserts

compatible with Locator* abutments of all implant brands



*Locator is a trademark of Zest IP Holdings, LLC

KERATOR



Kerator Abutment & Kit

Gingival Height	Junior (J)	Standard (S)
1 mm	AT401	IS401
2 mm	AT402	IS402
3 mm	AT403	IS403
4 mm	AT404	IS404
5 mm	AT405	IS405
6 mm	AT406	IS406
Angled 1.5 mm	AT4AN1.5	IS4AN1.5
Angled 3 mm	AT4AN3	IS4AN3

Includes; Kerator Abutment,
Metal Housing (with black insert),
Protective disc,
Pink, Blue, Red nylon inserts


Kerator Nylon Insert (20°)

Blue	Pink	White
544 gr. 1.2 lbs	1088 gr. 2.4 lbs	1814 gr. 4 lbs
CPB	CPP	CPW

Kerator Nylon Insert - Angled (40°)

Yellow	Red	Orange	Green
0 gr. 0 lbs	362 gr. 0.8 lbs	816 gr. 1.8 lbs	1451 gr. 3.2 lbs
CPY	CPR	CPO	CPG

MULTI UNIT SYSTEM

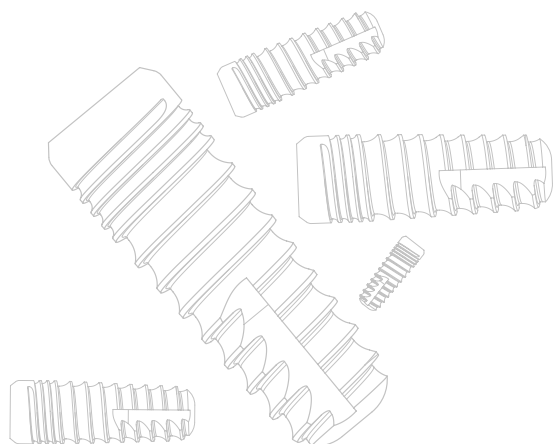

Multi Unit Straight Abutment

Gingival Height	1 mm	3 mm	5 mm
-----------------	------	------	------

Junior



BMUAJ1 | BMUAJ3

Standard



BMUAS1 | BMUAS3 | BMUAS5

- * Used for multiple-unit restorations including; screw-retained restorations at the abutment level, cast alloy bar for overdentures and fixed/hybrid restorations
- * Packaged with BMUACC
- * Ti-Gr 23 (Ti6Al4V ELI)
- * Torque value: with hex adapter 25 Ncm



Cover Cap

Product Code | BMUACC

Torque value:
Manually (5 - 10 Ncm)

Multi Unit Angled Abutment 17°

Gingival Height	2 mm	3 mm	4 mm
-----------------	------	------	------

Junior



BMUA17J2 | BMUA17J3

Standard



BMUA17S2 | BMUA17S3 | BMUA17S4

Multi Unit Angled Abutment 30°

3 mm	4 mm	5 mm
------	------	------



BMUA30S3 | BMUA30S4 | BMUA30S5

- * Used for multiple-unit restorations including; screw-retained restorations at the abutment level, cast alloy bar for overdentures and fixed/hybrid restorations
- * Packaged with BMUACC
- * Packaged with an abutment screw, BASJ for junior platform and BASS for standard platform
- * Ti-Gr 23 (Ti6Al4V ELI)
- * Screw torque value: with hex driver 25 Ncm

Multi Unit Coping



Plastic Coping

Product Code | BMUCP-NH

- * Use for fabricating metal-reinforced acrylic prostheses or bar overdentures
- * May be trimmed for height
- * Packaged with BMUACS
- * Acetal Resin



Passive Fit Coping

exocad

Product Code | BMUCPF

- * Use for fabricating metal-reinforced acrylic prostheses or bar overdentures, cemented using the passive-fit technique
- * May be trimmed for height
- * Packaged with passive fit part and BMUACS
- * Ti-Gr 23 (Ti6Al4V ELI) + Acetal Resin



Titanium Coping

Product Code | BMUCT-NH

- * Use for fabricating acrylic temporary and final prostheses
- * May be trimmed for height
- * Packaged with BMUACS
- * Ti-Gr 23 (Ti6Al4V ELI)



Coping Screw

Product Code | BMUACS

- *Torque value:
Manually or 15 Ncm

Multi Unit Parts

**Transfer Coping
Open Tray**



BMUAOT-NH

**Transfer Coping
Closed Tray**



BMUACT-NH

Lab Analog



BMULA-NH



- * Torque value: Manually (5 - 10 Ncm)
- * Ti-Gr 23 (Ti6Al4V ELI)

Hex Adapter

Product Code | BMUHA



- * Used to carry and torque straight multi unit abutment

Abutment Driver

Product Code | BMUAD



- * Used to carry straight/angled multi unit abutment

Bone Profiler Drill

Junior

Standard



BFDJ

BFDS

- * Designed to drilling of the crestal bone for optimal placement of multi unit angled abutment
- * Screw the guide into the implant and align the profiling bur for precise bone removal
- * Stainless Steel



CUSTOMIZED SOLUTIONS

In the rapidly expanding digital dentistry, choosing the right solution partners for customized prosthetic solutions is of vital for the long-term success of clinics.

UMC is a design and production center providing service for the clinics and laboratories using BioInfinity.



CUSTOMIZED SOLUTIONS

exocad

TiBase Abutment



Junior 		Standard 	
Hexed	Non- Hexed	Hexed	Non- Hexed



BTBAJN1-H | BTBAJN1-NH | BTBASN1-H | BTBASN1-NH

- * Use hexed for single-unit, screw retained or cement-retained, CAD/CAM hybrid zirconia restorations.
- * Use non-hexed for multiple-unit, screw retained or cement-retained, CAD/CAM hybrid zirconia restorations.
- * Packaged with an abutment screw, BASJ for junior platform and BASS for standard platform.
- * Ti-Gr 23 (Ti6Al4V ELI)
- * Screw torque value: 25 Ncm

Custom Castable Abutment

Junior 		Standard 	
Hexed	Non- Hexed	Hexed	Non- Hexed



BCCAJ-H | BCCAJ-NH | BCCAS-H | BCCAS-NH

- * Use hexed abutments for single-unit, screw-retained or cement-retained, custom abutment restorations.
- * Use non-hexed abutment for multiple-unit, screw-retained restorations
- * Packaged with an abutment screw, BASJ for junior platform and BASS for standard platform.
- * Acetal Resin
- * Screw torque value: 25 Ncm

Pre-milled Abutment

Junior 	Standard 
--	--



BPMAJ | BPMAS

- * Used for customized cementretained restorations
- * Packaged with an abutment screw BASJ for junior platform and BASS for standard platform.
- * Ti-Gr 23 (Ti6Al4V ELI)
- * Screw torque value: 25 Ncm

Scanbody

Junior 	Standard 	Multi Unit
--	--	------------



BSBJ | BSBS | BMUSB

- * Designed for intraoral scanner and lab model scanner
- * Packaged with an abutment screw, BASJ for junior platform, BASS for standard platform and BMUACS for multi unit abutment.
- * Ti-Gr 23 (Ti6Al4V ELI)

Digital Analog


Junior 	Standard 	Multi Unit
--	--	------------





BDAJ | BDAS | BMUDA

- * Designed to be used in 3D printers for digital model
- * Packaged with BDASc
- * Ti-Gr 23 (Ti6Al4V ELI)

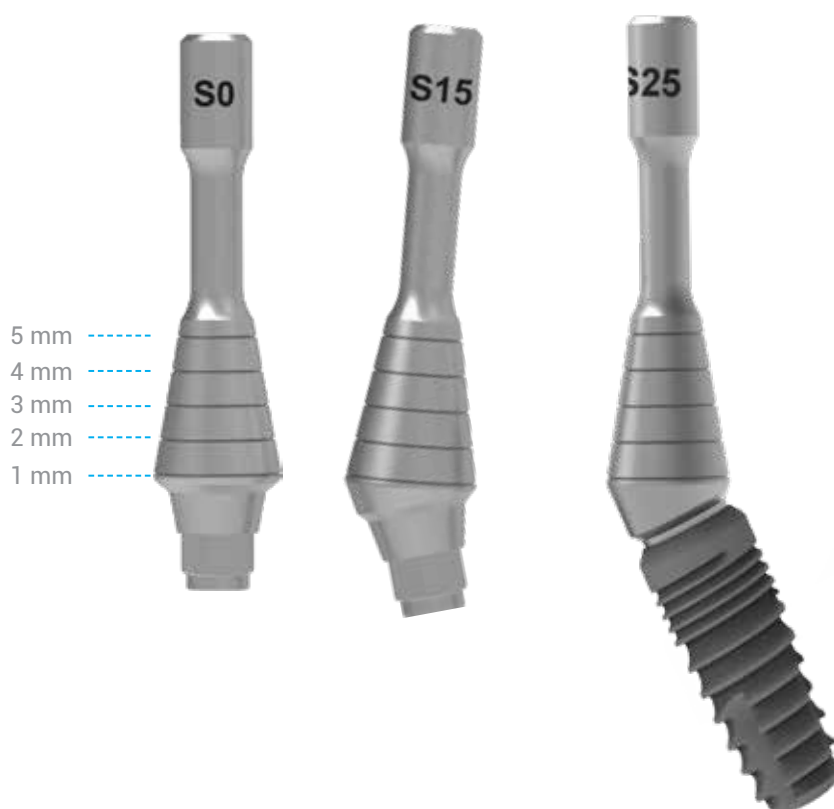ABUTMENT TRY-IN KIT



Abutment Try-in Kit

Angled of Abutment	Junior 	Standard 
0°	TRYJ0	TRYS0
15°	TRYJ15	TRYS15
25°	-	TRYS25
17°	TRYJ17	TRYS17
30°	-	TRYS30

Product Code | TRYKIT

* Designed to determine the appropriate gingival height and abutment angle in an ideal superstructure planning
 * Ti-Gr 23 (Ti6Al4V ELI)

WASHING AND STERILIZATION



Things to be considered during the use of the surgical kit;

Our surgical instruments are delivered as non-sterile. They must necessarily be cleaned, disinfected and sterilized before use.

Rapid sterilization methods must not be allowed. Hot air sterilization, radiation sterilization, plasma sterilization, formaldehyde or ethylene oxide sterilization methods must be avoided. Surgical instruments must not be exposed to temperatures higher than 134°C (273°F).

Surgical instruments must never be cleaned with a metal brush or steel wool. Instruments made from different materials must never be placed in liquid bath at the same time as they create a risk of galvanic corrosion.

It is recommended to use a water-soluble, non-toxic, biodegradable and slightly alkaline cleaning agent. The use of cleaning or disinfecting products containing chlorine (bleach, tap water, etc.), oxalic acid or hydrogen peroxide must not be preferred as they will damage the surgical instruments and cause oxidation.

When using the drills, it is recommended to observe the rotational speeds (rpm) in the instructions manual and in the catalogue. In order to avoid possible stress and necrosis on the bone, it is recommended to replace the drill at every 25th use.

Suggested sterilization parameters

Dynamic air discharge (pre-vacuum vapor cycle)

Exposure temperature: 134°C

Exposure time: 4 minutes

Minimum drying time;

For wrapped devices: 15 minutes

For devices inside container: 30 minutes

Exposure temperature: 121°C

Exposure time: 20 minutes

Minimum drying time;

For wrapped devices: 15 minutes

For devices inside container: 30 minutes



OSSTELL


Osstell helps you assess the condition of osseointegration by determining the Implant stability in an objective and noninvasive way without jeopardizing the healing process. Osstell notifies you when an Implant is ready to load.

You can measure the ISQ value of BioInfinity dental implants with Osstell as well.




Osstell

Osstell IDx	Osstell ISQ
101000	100500

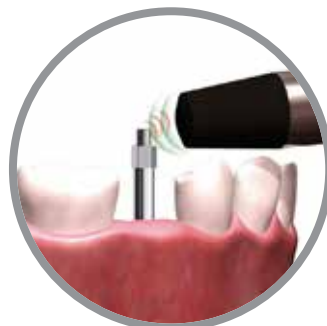

Smartpeg






SURGICAL EQUIPMENTS



Ultrasonic Piezo Surgery
200300

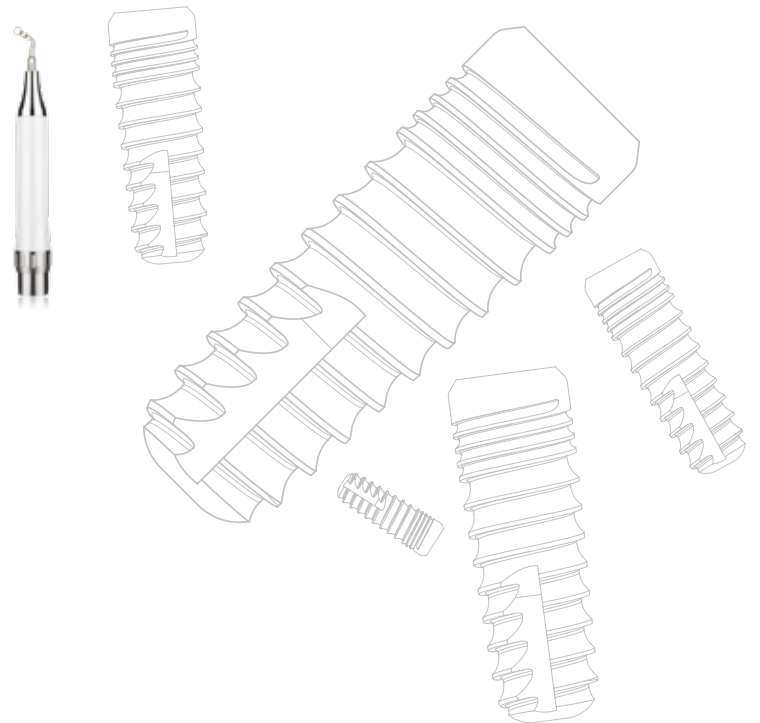

Implant Motor
XCube
200200



Implant Motor
Traus
200100



ADVANCED
IMPLANTOLOGY
ACADEMY
























BASIC AND ADVANCED IMPLANTOLOGY

COURSE • SEMINAR • SYMPOSIUM

SYMBOLS



Explanation of the symbols on labels and packages

Symbol	Explanation	Symbol	Explanation	Symbol	Explanation
	Manufacturer		Temperature limitation		Junior platform
	CE conformity mark and notified body number		Electronic instruction manual		Standard platform
	Catalog number		Sterilized using irradiation		Ø 3.2 implant
	Serial number		Non-sterile		Ø 3.7 implant
	Do not re-use		Do not re-sterilize		Ø 4.2 implant
	Keep dry		Do not use if package is damaged		Ø 4.7 implant
	Expiration date		Keep away from sunlight		Ø 5.2 implant
	Medical Device		Single steril barrier system with protective packaging inside		

PRODUCT LIST

Implant

Product Code	Product Name	Page No
BR3210.....	Implant 3.2x10 mm.....	22
BR3212.....	Implant 3.2x12 mm.....	22
BR3214.....	Implant 3.2x14 mm.....	22
BR3216.....	Implant 3.2x16 mm.....	22
BR3708.....	Implant 3.7x08 mm.....	22
BR3710.....	Implant 3.7x10 mm.....	22
BR3712.....	Implant 3.7x12 mm.....	22
BR3714.....	Implant 3.7x14 mm.....	22
BR3716.....	Implant 3.7x16 mm.....	22
BR4208.....	Implant 4.2x08 mm.....	22
BR4210.....	Implant 4.2x10 mm.....	22
BR4212.....	Implant 4.2x12 mm.....	22
BR4214.....	Implant 4.2x14 mm.....	22
BR4216.....	Implant 4.2x16 mm.....	22
BR4708.....	Implant 4.7x08 mm.....	22
BR4710.....	Implant 4.7x10 mm.....	22
BR4712.....	Implant 4.7x12 mm.....	22
BR4714.....	Implant 4.7x14 mm.....	22
BR4716.....	Implant 4.7x16 mm.....	22
BR5208.....	Implant 5.2x08 mm.....	22
BR5210.....	Implant 5.2x10 mm.....	22
BR5212.....	Implant 5.2x12 mm.....	22
BR5214.....	Implant 5.2x14 mm.....	22
BR4206H.....	Short Implant 4.2x06 mm (Hard).....	30
BR4206S.....	Short Implant 4.2x06 mm (Soft).....	30
BR4706H.....	Short Implant 4.7x06 mm (Hard).....	30
BR4706S.....	Short Implant 4.7x06 mm (Soft).....	30
BR5206H.....	Short Implant 5.2x06 mm (Hard).....	30
BR5206S.....	Short Implant 5.2x06 mm (Soft).....	30

Junior / Standard Platform

Product Code	Product Name	Page Number
BCSJ.....	Closing Screw Junior.....	22
BCSS.....	Closing Screw Standard.....	22
BSCS0.....	Sinus Closing Screw Junior 0 mm.....	31
BSCS1.....	Sinus Closing Screw Standard 1 mm.....	31
BHAJN1.....	Healing Abutment Junior Narrow 1 mm.....	36
BHAJN2.....	Healing Abutment Junior Narrow 2 mm.....	36
BHAJN3.....	Healing Abutment Junior Narrow 3 mm.....	36
BHAJN4.....	Healing Abutment Junior Narrow 4 mm.....	36
BHAJN5.....	Healing Abutment Junior Narrow 5 mm.....	36
BHAJN7.....	Healing Abutment Junior Narrow 7 mm.....	36
BHASN1.....	Healing Abutment Standard Narrow 1 mm.....	36
BHASN2.....	Healing Abutment Standard Narrow 2 mm.....	36
BHASN3.....	Healing Abutment Standard Narrow 3 mm.....	36
BHASN4.....	Healing Abutment Standard Narrow 4 mm.....	36
BHASN5.....	Healing Abutment Standard Narrow 5 mm.....	36
BHASN7.....	Healing Abutment Standard Narrow 7 mm.....	36
BHASR2.....	Healing Abutment Standard Regular 2 mm.....	36
BHASR3.....	Healing Abutment Standard Regular 3 mm.....	36
BHASR4.....	Healing Abutment Standard Regular 4 mm.....	36
BHASR5.....	Healing Abutment Standard Regular 5 mm.....	36
BHASR7.....	Healing Abutment Standard Regular 7 mm.....	36
BHASW3.....	Healing Abutment Standard Wide 3 mm.....	36
BHASW4.....	Healing Abutment Standard Wide 4 mm.....	36
BHASW5.....	Healing Abutment Standard Wide 5 mm.....	36
BHASW7.....	Healing Abutment Standard Wide 7 mm.....	36
BASJ-LAB.....	Lab Abutment Screw Junior.....	37

BASS-LAB.....	Lab Abutment Screw Standard.....	37
BLAJ.....	Lab Analog Junior.....	37
BLAS.....	Lab Analog Standard.....	37
BICJN.....	Transfer Coping Junior Narrow (Open Tray).....	37
BTCJN.....	Transfer Coping Junior Narrow (Closed Tray).....	37
BICScJ.....	Transfer Coping Screw Junior (Open Tray).....	37
BTCScJ.....	Transfer Coping Screw Junior (Closed Tray).....	37
BICSN.....	Transfer Coping Standard Narrow (Open Tray).....	37
BTCSN.....	Transfer Coping Standard Narrow (Closed Tray).....	37
BICSR.....	Transfer Coping Standard Regular (Open Tray).....	37
BTC SR.....	Transfer Coping Standard Regular (Closed Tray).....	37
BICSW.....	Transfer Coping Standard Wide (Open Tray).....	37
BTC SW.....	Transfer Coping Standard Wide (Closed Tray).....	37
BICScS.....	Transfer Coping Screw Standard (Open Tray).....	37
BTCScS.....	Transfer Coping Screw Standard (Closed Tray).....	37
BSAJN1.....	Straight Abutment Junior Narrow 1 mm.....	39
BSAJN2.....	Straight Abutment Junior Narrow 2 mm.....	39
BSAJN3.....	Straight Abutment Junior Narrow 3 mm.....	39
BSAJN4.....	Straight Abutment Junior Narrow 4 mm.....	39
BSAJN5.....	Straight Abutment Junior Narrow 5 mm.....	39
BSASN1.....	Straight Abutment Standard Narrow 1 mm.....	39
BSASN2.....	Straight Abutment Standard Narrow 2 mm.....	39
BSASN3.....	Straight Abutment Standard Narrow 3 mm.....	39
BSASN4.....	Straight Abutment Standard Narrow 4 mm.....	39
BSASN5.....	Straight Abutment Standard Narrow 5 mm.....	39
BSASR2.....	Straight Abutment Standard Regular 2 mm.....	39
BSASR3.....	Straight Abutment Standard Regular 3 mm.....	39
BSASR4.....	Straight Abutment Standard Regular 4 mm.....	39
BSASR5.....	Straight Abutment Standard Regular 5 mm.....	39
BSASW3.....	Straight Abutment Standard Wide 3 mm.....	39
BSASW4.....	Straight Abutment Standard Wide 4 mm.....	39
BSASW5.....	Straight Abutment Standard Wide 5 mm.....	39
BASJ.....	Abutment Screw Junior.....	40
BASS.....	Abutment Screw Standard.....	40
BAEJ15N12.....	15° Angled Esthetic Abutment Junior Narrow 1-2 mm.....	40
BAEJ15N23.....	15° Angled Esthetic Abutment Junior Narrow 2-3 mm.....	40
BAEJ15N34.....	15° Angled Esthetic Abutment Junior Narrow 3-4 mm.....	40
BAEJ15N45.....	15° Angled Esthetic Abutment Junior Narrow 4-5 mm.....	40
BAES15N12.....	15° Angled Esthetic Abutment Standard Narrow 1-2 mm.....	40
BAES15N23.....	15° Angled Esthetic Abutment Standard Narrow 2-3 mm.....	40
BAES15N34.....	15° Angled Esthetic Abutment Standard Narrow 3-4 mm.....	40
BAES15N45.....	15° Angled Esthetic Abutment Standard Narrow 4-5 mm.....	40
BAES15R23.....	15° Angled Esthetic Abutment Standard Regular 2-3 mm.....	40
BAES15R34.....	15° Angled Esthetic Abutment Standard Regular 3-4 mm.....	40
BAES15R45.....	15° Angled Esthetic Abutment Standard Regular 4-5 mm.....	40
BAES15W34.....	15° Angled Esthetic Abutment Standard Wide 3-4 mm.....	40
BAES15W45.....	15° Angled Esthetic Abutment Standard Wide 4-5 mm.....	40
BAES25N12.....	25° Angled Esthetic Abutment Standard Narrow 1-2 mm.....	40
BAES25N23.....	25° Angled Esthetic Abutment Standard Narrow 2-3 mm.....	40
BAES25N34.....	25° Angled Esthetic Abutment Standard Narrow 3-4 mm.....	40
BAES25N45.....	25° Angled Esthetic Abutment Standard Narrow 4-5 mm.....	40
BAES25R23.....	25° Angled Esthetic Abutment Standard Regular 2-3 mm.....	40

BAES25R34.....	25° Angled Esthetic Abutment Standard Regular 3-4 mm.....	40	BLOAJ3.....	BioLoc Abutment Junior 3 mm.....	44
BAES25R45.....	25° Angled Esthetic Abutment Standard Regular 4-5 mm.....	40	BLOAJ4.....	BioLoc Abutment Junior 4 mm.....	44
BAES25W34.....	25° Angled Esthetic Abutment Standard Wide 3-4 mm.....	40	BLOAJ5.....	BioLoc Abutment Junior 5 mm.....	44
BAES25W45.....	25° Angled Esthetic Abutment Standard Wide 4-5 mm.....	40	BLOAJ6.....	BioLoc Abutment Junior 6 mm.....	44
BTAH.....	Abutment Holder.....	41	BLOAS15J1.5.....	BioLoc Abutment Junior Angled 1.5 mm.....	44
BPTAJN1-H.....	Temporary Abutment PEEK Junior Narrow 1 mm Hexed.....	41	BLOAS15J3.....	BioLoc Abutment Junior Angled 3 mm.....	44
BPTAJN1-NH.....	Temporary Abutment PEEK Junior Narrow 1 mm Non-Hexed.....	41	BLOAS1.....	BioLoc Abutment Standard 1 mm.....	44
BPTAJN3-H.....	Temporary Abutment PEEK Junior Narrow 3 mm Hexed.....	41	BLOAS2.....	BioLoc Abutment Standard 2 mm.....	44
BPTAJN3-NH.....	Temporary Abutment PEEK Junior Narrow 3 mm Non-Hexed.....	41	BLOAS3.....	BioLoc Abutment Standard 3 mm.....	44
BTTAJN1-H.....	Temporary Abutment Titanium Junior Narrow 1 mm Hexed.....	41	BLOAS4.....	BioLoc Abutment Standard 4 mm.....	44
BTTAJN1-NH.....	Temporary Abutment Titanium Junior Narrow 1 mm Non-Hexed.....	41	BLOAS5.....	BioLoc Abutment Standard 5 mm.....	44
BTTAJN3-H.....	Temporary Abutment Titanium Junior Narrow 3 mm Hexed.....	41	BLOAS6.....	BioLoc Abutment Standard 6 mm.....	44
BTTAJN3-NH.....	Temporary Abutment Titanium Junior Narrow 3 mm Non-Hexed.....	41	BLOAS15S1.5.....	BioLoc Abutment Standard Angled 1.5 mm.....	44
BPTASN1-H.....	Temporary Abutment PEEK Standard Narrow 1 mm Hexed.....	41	BLOAS15S3.....	BioLoc Abutment Standard Angled 3 mm.....	44
BPTASN1-NH.....	Temporary Abutment PEEK Standard Narrow 1 mm Non-Hexed.....	41	CPR.....	Kerator Insert Angled Red.....	45
BPTASN3-H.....	Temporary Abutment PEEK Standard Narrow 3 mm Hexed.....	41	CPY.....	Kerator Insert Angled Yellow.....	45
BPTASN3-NH.....	Temporary Abutment PEEK Standard Narrow 3 mm Non-Hexed.....	41	CPO.....	Kerator Insert Angled Orange.....	45
BPTASR2-H.....	Temporary Abutment PEEK Standard Regular 2 mm Hexed.....	41	CPG.....	Kerator Insert Angled Green.....	45
BPTASR2-NH.....	Temporary Abutment PEEK Standard Regular 2 mm Non-Hexed.....	41	CPW.....	Kerator Insert Clear.....	45
BPTASR4-H.....	Temporary Abutment PEEK Standard Regular 4 mm Hexed.....	41	CPB.....	Kerator Insert Blue.....	45
BPTASR4-NH.....	Temporary Abutment PEEK Standard Regular 4 mm Non-Hexed.....	41	CPP.....	Kerator Insert Pink.....	45
BPTASW3-H.....	Temporary Abutment PEEK Standard Wide 3 mm Hexed.....	41	IS401.....	Kerator Abutment Standard 1 mm.....	45
BPTASW3-NH.....	Temporary Abutment PEEK Standard Wide 3 mm Non-Hexed.....	41	AT401.....	Kerator Abutment Junior 1 mm.....	45
BTTASN1-H.....	Temporary Abutment Titanium Standard Narrow 1 mm Hexed.....	41	IS402.....	Kerator Abutment Standard 2 mm.....	45
BTTASN1-NH.....	Temporary Abutment Titanium Standard Narrow 1 mm Non-Hexed.....	41	AT402.....	Kerator Abutment Junior 2 mm.....	45
BTTASN3-H.....	Temporary Abutment Titanium Standard Narrow 3 mm Hexed.....	41	IS403.....	Kerator Abutment Standard 3 mm.....	45
BTTASN3-NH.....	Temporary Abutment Titanium Standard Narrow 3 mm Non-Hexed.....	41	AT403.....	Kerator Abutment Junior 3 mm.....	45
BTTASR2-H.....	Temporary Abutment Titanium Standard Regular 2 mm Hexed.....	41	IS404.....	Kerator Abutment Standard 4 mm.....	45
BTTASR2-NH.....	Temporary Abutment Titanium Standard Regular 2 mm Non-Hexed.....	41	AT404.....	Kerator Abutment Junior 4 mm.....	45
BTTASR4-H.....	Temporary Abutment Titanium Standard Regular 4 mm Hexed.....	41	IS405.....	Kerator Abutment Standard 5 mm.....	45
BTTASR4-NH.....	Temporary Abutment Titanium Standard Regular 4 mm Non-Hexed.....	41	AT405.....	Kerator Abutment Junior 5 mm.....	45
BTTASW3-H.....	Temporary Abutment Titanium Standard Wide 3 mm Hexed.....	41	IS406.....	Kerator Abutment Standard 6 mm.....	45
BTTASW3-NH.....	Temporary Abutment Titanium Standard Wide 3 mm Non-Hexed.....	41	AT406.....	Kerator Abutment Junior 6 mm.....	45
BBLA.....	BioBall Lab Analog.....	42	IS4AN1.5.....	Kerator Abutment Standard Angled 1.5 mm.....	45
BBAJN1.....	BioBall Abutment Junior Narrow 1 mm.....	42	AT4AN1.5.....	Kerator Abutment Junior Angled 1.5 mm.....	45
BBAJN2.....	BioBall Abutment Junior Narrow 2 mm.....	42	IS4AN3.....	Kerator Abutment Standard Angled 3 mm.....	45
BBAJN3.....	BioBall Abutment Junior Narrow 3 mm.....	42	AT4AN3.....	Kerator Abutment Junior Angled 3 mm.....	45
BBAJN4.....	BioBall Abutment Junior Narrow 4 mm.....	42	BMUACC.....	Multi Unit Closing Screw.....	46
BBAJN5.....	BioBall Abutment Junior Narrow 5 mm.....	42	BMASJ.....	Multi Unit Abutment Screw Junior.....	46
BBASN1.....	BioBall Abutment Standard Narrow 1 mm.....	42	BMASS.....	Multi Unit Abutment Screw Standard.....	46
BBASN2.....	BioBall Abutment Standard Narrow 2 mm.....	42	BMUAJ1.....	Multi Unit Straight Abutment Junior 1 mm.....	46
BBASN3.....	BioBall Abutment Standard Narrow 3 mm.....	42	BMUAJ3.....	Multi Unit Straight Abutment Junior 3 mm.....	46
BBASN4.....	BioBall Abutment Standard Narrow 4 mm.....	42	BMUA17J2.....	Multi Unit 17° Angled Abutment Junior 2 mm.....	46
BBASN5.....	BioBall Abutment Standard Narrow 5 mm.....	42	BMUA17J3.....	Multi Unit 17° Angled Abutment Junior 3 mm.....	46
BBASET.....	Ball Abutment Set.....	43	BMUAS1.....	Multi Unit Straight Abutment Standard 1 mm.....	46
BBANI-P.....	Ball Abutment Insert Pink.....	43	BMUAS3.....	Multi Unit Straight Abutment Standard 3 mm.....	46
BBANI-B.....	Ball Abutment Insert Black.....	43	BMUAS5.....	Multi Unit Straight Abutment Standard 5 mm.....	46
BBANI-C.....	Ball Abutment Insert Clear.....	43	BMUA17S2.....	Multi Unit 17° Angled Abutment Standard 2 mm.....	46
BBSET.....	BioBall Set.....	42	BMUA17S3.....	Multi Unit 17° Angled Abutment Standard 3 mm.....	46
BBS4.....	BioBall Insert Soft.....	42	BMUA17S4.....	Multi Unit 17° Angled Abutment Standard 4 mm.....	46
BBL4.....	BioLoc Insert for Lab.....	42	BMUA30S3.....	Multi Unit 30° Angled Abutment Standard 3 mm.....	46
BBM4.....	BioBall Insert Medium.....	42	BMUA30S4.....	Multi Unit 30° Angled Abutment Standard 4 mm.....	46
BBH4.....	BioBall Insert High.....	42	BMUA30S5.....	Multi Unit 30° Angled Abutment Standard 5 mm.....	46
BLOLA.....	BioLoc Lab Analog.....	44	BMUHA.....	Multi Unit Hex Adapter.....	47
BLSET.....	BioLoc Set.....	44	BMUAD.....	Multi Unit Abutment Driver.....	47
BLSET-ECO.....	BioLoc Set Mini.....	44	BMUACS.....	Multi Unit Coping Screw.....	47
BLS4.....	BioLoc Insert Soft.....	44	BMULA-NH.....	Multi Unit Lab Analog Non-Hexed.....	47
BLL4.....	BioLoc Insert for Lab.....	44	BMUCPF.....	Multi Unit Passive Fit Coping Non-Hexed.....	47
BLM4.....	BioLoc Insert Medium.....	44	BMUCP-NH.....	Multi Unit Plastic Coping Non-Hexed.....	47
BLH4.....	BioLoc Insert High.....	44	BMUCT-NH.....	Multi Unit Titanium Coping Non-Hexed.....	47
BLOTC.....	BioLoc Transfer Coping.....	44	BMUAOT-NH.....	Multi Unit Transfer Coping (Open Tray) Non-Hexed.....	47
KMT002.....	BioLoc Insert Handle.....	44	BMUACT-NH.....	Multi Unit Transfer Coping (Closed Tray) Non-Hexed.....	47
BLOAJ1.....	BioLoc Abutment Junior 1 mm.....	44	BFDJ.....	Bone Profiler Drill Junior.....	47
BLOAJ2.....	BioLoc Abutment Junior 2 mm.....	44	BFDS.....	Bone Profiler Drill Standard.....	47

BCCAJ-H	Custom Castable Abutment Junior Hexed	49	BIDSH-S	Implant Driver, Standard Platform - Short (Handpiece)	28
BCCAJ-NH	Custom Castable Abutment Junior Non-Hexed	49	BIDSR-S	Implant Driver, Standard Platform - Short (Manually/Ratchet)	28
BCCAS-H	Custom Castable Abutment Standard Hex	49	BIDSH-L	Implant Driver, Standard Platform - Long (Handpiece)	28
BCCAS-NH	Custom Castable Abutment Standard Non-Hexed	49	BIDSR-L	Implant Driver, Standard Platform - Long (Manually/Ratchet)	28
BMUSB	Scan Body Multi Unit	49	LD	Lindemann Drill	28
BDAJ	Digital Analog Junior	49	PD	Pilot Drill	28
BDAS	Digital Analog Standard	49	PP2228	Pin 0°	28
BMUDA	Digital Analog Multi Unit	49	BMU17PP	Pin 17°	28
BSBJ	Scan Body Junior	49	BMU30PP	Pin 30°	28
BSBS	Scan Body Standard	49	RD	Round Drill	28
BPMAS	Pre-milled Abutment Standard	49	TAP32	Tap 3.2	28
BPMAS	Pre-milled Abutment Standard	49	TAP37	Tap 3.7	28
BTBAJNT1-H	TiBase Abutment Junior Narrow 1 mm Hex	49	TAP42	Tap 4.2	28
BTBAJNT1-NH	TiBase Abutment Junior Narrow 1 mm Non-Hex	49	TAP47	Tap 4.7	28
BTBASNT1-H	TiBase Abutment Standard Narrow 1 mm Hex	49	TAP52	Tap 5.2	28
BTBASNT1-NH	TiBase Abutment Standard Narrow 1 mm Non-Hex	49	SD2206	Starter Drill 06 mm - Short Implant	31
TRYKIT	Try-in Abutment Kit	50	BSSKIT	Surgical Kit (Short Implant)	31
TRYJ0	Try-in Abutment Junior 0°	50	SSD42	Final Drill - Short Implant 4.2	31
TRYJ15	Try-in Abutment Junior 15°	50	SSD47	Final Drill - Short Implant 4.7	31
TRYJ17	Try-in Abutment Junior 17°	50	SSD52	Final Drill - Short Implant 5.2	31
TRYS0	Try-in Abutment Standard 0°	50	STAP42	Tap - Short Implant 4.2	31
TRYS15	Try-in Abutment Standard 15°	50	STAP47	Tap - Short Implant 4.7	31
TRYS17	Try-in Abutment Standard 17°	50	STAP52	Tap - Short Implant 5.2	31
TRYS25	Try-in Abutment Standard 25°	50			
TRYS30	Try-in Abutment Standard 30°	50			

Surgical Kit

Product Code	Product Name	Page Number
BSK2000	Surgical Kit (Complete)	25
SPH1000	Implant Handle	27
SPTR	Surgical and Prosthetic Torque Ratchet	27
SD2208	Starter Drill 08 mm	28
SD2210	Starter Drill 10 mm	28
SD2212	Starter Drill 12 mm	28
SD2214	Starter Drill 14 mm	28
SD2216	Starter Drill 16 mm	28
CS32	Counter Sink 3.2	28
CS37	Counter Sink 3.7	28
CS42	Counter Sink 4.2	28
CS47	Counter Sink 4.7	28
CS52	Counter Sink 5.2	28
DG32	Depth Gauge 3.2	28
DG37	Depth Gauge 3.7	28
DG42	Depth Gauge 4.2	28
DG47	Depth Gauge 4.7	28
DG52	Depth Gauge 5.2	28
SD32	Final Drill 3.2	28
CD37	Final Drill 3.7	28
CD42	Final Drill 4.2	28
CD47	Final Drill 4.7	28
CD52	Final Drill 5.2	28
FD	Fissure Drill	28
DE	Drill Extender	28
TAPHW	Hand Wrench	28
12HDH-S	Hex Driver Short (Handpiece)	28
12HDR-S	Hex Driver Short (Manually/Ratchet)	28
12HDH-L	Hex Driver Long (Handpiece)	28
12HDR-L	Hex Driver Long (Manually/Ratchet)	28
BIDJH-S	Implant Driver, Junior Platform - Short (Handpiece)	28
BIDJR-S	Implant Driver, Junior Platform - Short (Manually/Ratchet)	28
BIDJH-L	Implant Driver, Junior Platform - Long (Handpiece)	28
BIDJR-L	Implant Driver, Junior Platform - Long (Manually/Ratchet)	28

Other

	Product Name	Sayfa No
101000	Osstell IDx	52
100500	Osstell ISQ	52
100455	SmartPeg Junior (Type 38)	52
100425	SmartPeg Standard (Type 26)	52
200100	Implant Motor - Traus	53
200200	Implant Motor - XCube	53
200300	Ultrasonic Piezo Surgery	53

AVP MEDICAL TECHNOLOGY

EXCLUSIVE EUROPEAN DEALER OF BIOINFINITY

avpmedtech.com



bioinfinityimplants.com



Avrupa Implant
İkitelli OSB HESKOP
M5 Blok No:82 34490
Basaksehir / Istanbul, Turkiye
Phone : +90 212 670 13 00 (pbx)
info@bioinfinityimplants.com

Rev. No: BPCENG-R003

EC REP mdi Europa GmbH

Langenhagener Str. 71 D-30855
Langenhagen - Germany
Phone: +49 511 39089530
E-mail: info@mdi-europa.com

avrupa implant is an  company
UMY MEDICAL