



MDS 21B ABSORBING CLAMP




- As specified in CISPR 16-1-3/ EN 55016-1-3
- Disturbance power measuring, according to CISPR 16-2-2/ EN 55016-2-2, CISPR 13/EN 55013, CISPR 14-1/EN 55014-1 and EN 50083-2
- Excellent for using as diagnostic tool and for measurements of screening attenuation of coaxial cables
- Supplied with 6 dB attenuator and RF cable

In connection with a measuring receiver according to CISPR 16-1-1, the absorbing clamp system Meyer de Stadelhofen / Lüthi (MDS) enables to measure the interference capability of radio interferers, such as domestic appliances, electric tools etc. directly; viz. by measuring the power generated by the interferer and fed to its supply cable.

The absorbing clamp measurement method (ACMM) is described in Clause 7 of CISPR 16-2-2: Specification for radio disturbance and immunity measuring apparatus and methods – Part 2-2: Methods of measurement of disturbances and immunity – Measurement of disturbance power. The absorbing clamp itself is described in CISPR 16-1-3: Radio disturbance and immunity measuring apparatus – Ancillary equipment – Disturbance power.

Example measurement set-up with table top EUT according CISPR 16-2-2

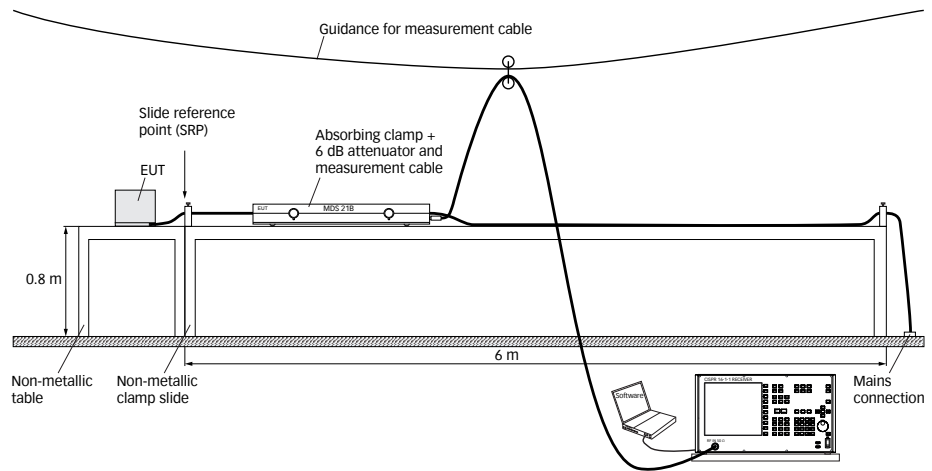

Technical specification

Frequency range:	30 MHz to 1000 MHz
Typical clamp factor:	see graph
Calibrated for receiver impedance:	50 Ω
Connector:	N, female
Max. current (f < 500 Hz):	30 A
Max. input power for immunity tests:	5 W
Diameter of appliance power cable:	up to 20 mm
Dimension (WxHxD):	610 mm x 115 mm x 80 mm
Weight:	approx. 6.3 kg
Classification:	for indoor use only
Operation:	+5 °C up to +40 °C
Relative humidity:	up to 80%



View to the EUT side of the opened MDS 21B




Advanced Test Solutions for EMC

MDS 21B ABSORBING CLAMP



View to the AE side and RF connector

Typical clamp factor in dB (pW/μV) inclusive 6 dB attenuator and 5 m cable RG223U

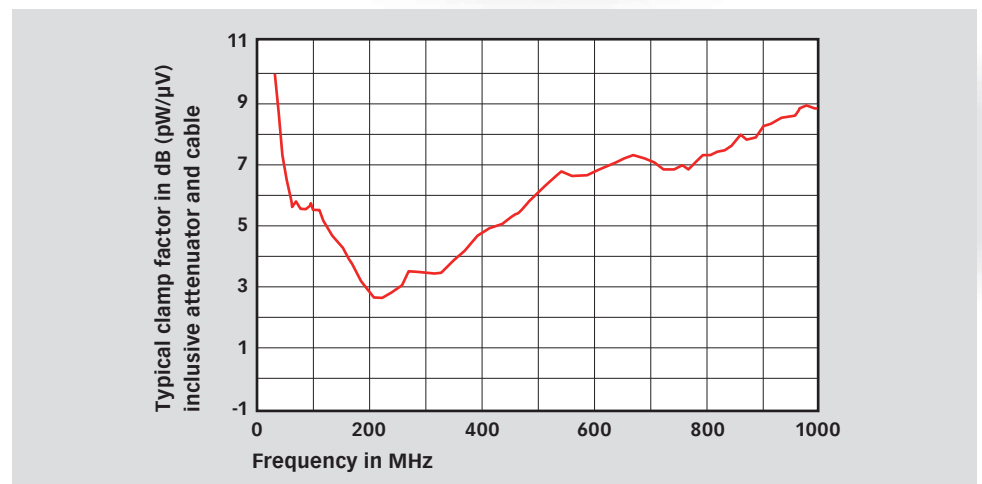

The interference output is determined by the following formula:

$$P = V + CF$$

P is the disturbance power in dB(pW)

V is the measured voltage in dB(μV)

CF is the clamp factor in dB(pW/μV)

Model no. and options

Part number	Description
257260	MDS 21B Absorbing clamp acc. CISPR 16-1-3, system Meyer de Stadelhofen / Lüthi, frequency range 30 - 1000 MHz, 50 Ohm, incl. 6 dB attenuator, RF cable N(m)-N(m) 5 m RG223U and traceable calibration (certificate according ISO17025)
238252	MBT 2 Hand-operated lane for MDS 21B

Teseq GmbH

Landsberger Str. 255 · 12623 Berlin · Germany
T +49 30 56 59 88 35 F +49 30 56 59 88 34
info.rf.cts@ametec.com www.teseq.com

© June 2017 Teseq®

Specifications subject to change without notice. Teseq® is an ISO-registered company. Its products are designed and manufactured under the strict quality and environmental requirements of the ISO 9001. This document has been carefully checked. However, Teseq® does not assume any liability for errors or inaccuracies.

82-257260 E02 June 2017