



Mission Mountain Laboratories. Inc.
 82892 US Hwy 93
 Ravalli, MT 59863
 Phone: 406-726-5227
 www.mm-labs.com



Accredited to ISO/IEC 17025:2017
 Accreditation #86228

Certificate of Analysis

Double Wood LLC
 3510 Scotts Lane #219
 Philadelphia, PA
 19129

Order ID: 2111113285
Lab Sample #: 43712703
Receive Date: 11/11/2021 12:48PM
Report ID: #9039

Sample Description: Fadogia Agrestis

Receive Condition: Good
Sample Lot #: 21SM1087 **Storage Condition:** Ambient
Serving Size: 2 capsules

<u>Chemical Analysis</u>	<u>Result</u>	<u>Specification</u>	<u>Analyst</u>	<u>Date</u>	<u>Method</u>
Cap Weight Verification	642.7 mg	Report	Emily Woodward	11/17/2021	MML160.24

<u>Identity</u>	<u>Result</u>	<u>Specification</u>	<u>Analyst</u>	<u>Date</u>	<u>Method</u>
FTIR	Conforms	Conforms	Allista Vetter	11/17/2021	MML220.02

Method References

Method # MML160.24

Reference In House Capsule Weight Method

Method # MML220.02

Desc Identification by FTIR

Instrument FTIR

Approval

Approved By:

Kimberly Nuccio
 President/Authorized Reviewer

Approved Date: 11/18/2021

Laboratory Location: 82892 US Hwy 93 N, Ravalli, MT 59863

Disclaimer: This product results are only applicable to test sample submitted. Mission Mountain Laboratory makes no claims as to the efficacy, safety, or other risks associated with any detected or non-detected levels of any compounds reported herein. This certificate shall not be reproduced except in full, without the written approval of Mission Mountain Laboratories. Quality and uncertainty data is available upon request. Testing listed above may not be included in our current PJLA scope of accreditation. Please consult PJLA Certificate# 86228 for a list of current accredited tests.




FTIR Report

Report Details

Report Location C:\pel_data\templates\standard\MML 43712703 Fadogia Agrestis Double Wood UATR
Report Creator Allista Vetter
Report Date 17 November, 2021 10:30

Compare Results

Result Spectrum

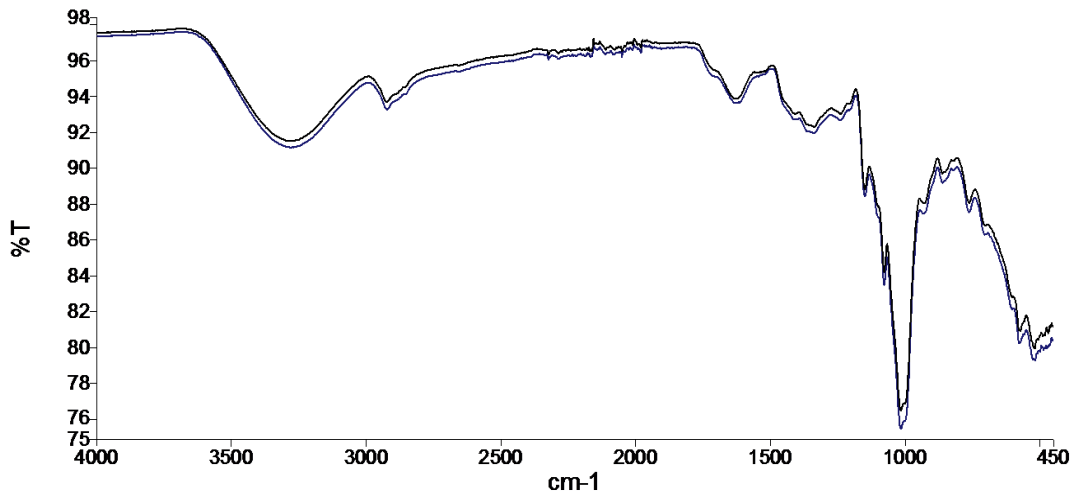

Name	Description
MML 43712703 Fadogia Agrestis Double Wood UATR	21SM1087
QC Fadogia Agrestis Double Wood UATR MML 43712703	21SM1087

Compare Summary

Name(ID)	Best Hit	Correlation	Pass / Fail
MML 43712703 Fadogia Agrestis Double Wood UATR	M:\- IDENTITY -\spectra\QC Fadogia Agrestis Double Wood UATR MML 43712703.sp	0.998777	Pass

Compare Details

Sample Name	Correlation	Pass / Fail
M:\- IDENTITY -\spectra\QC Fadogia Agrestis Double Wood UATR MML 43712703.sp	0.998777	Pass

