


Analysis of volatile chlorinated hydrocarbons

BP BOND Q

Column part number	0570235		
Phase	BP BOND Q	Detector	FID, 250°C
Column	25 m x 0.32 mm x 5 µm	Carrier gas	He
Sample	Volatile chlorinated hydrocarbons 100 ppm each	Carrier gas flow	30 mL/min
		Injection mode	Split/splitless
Initial temperature	250°C		

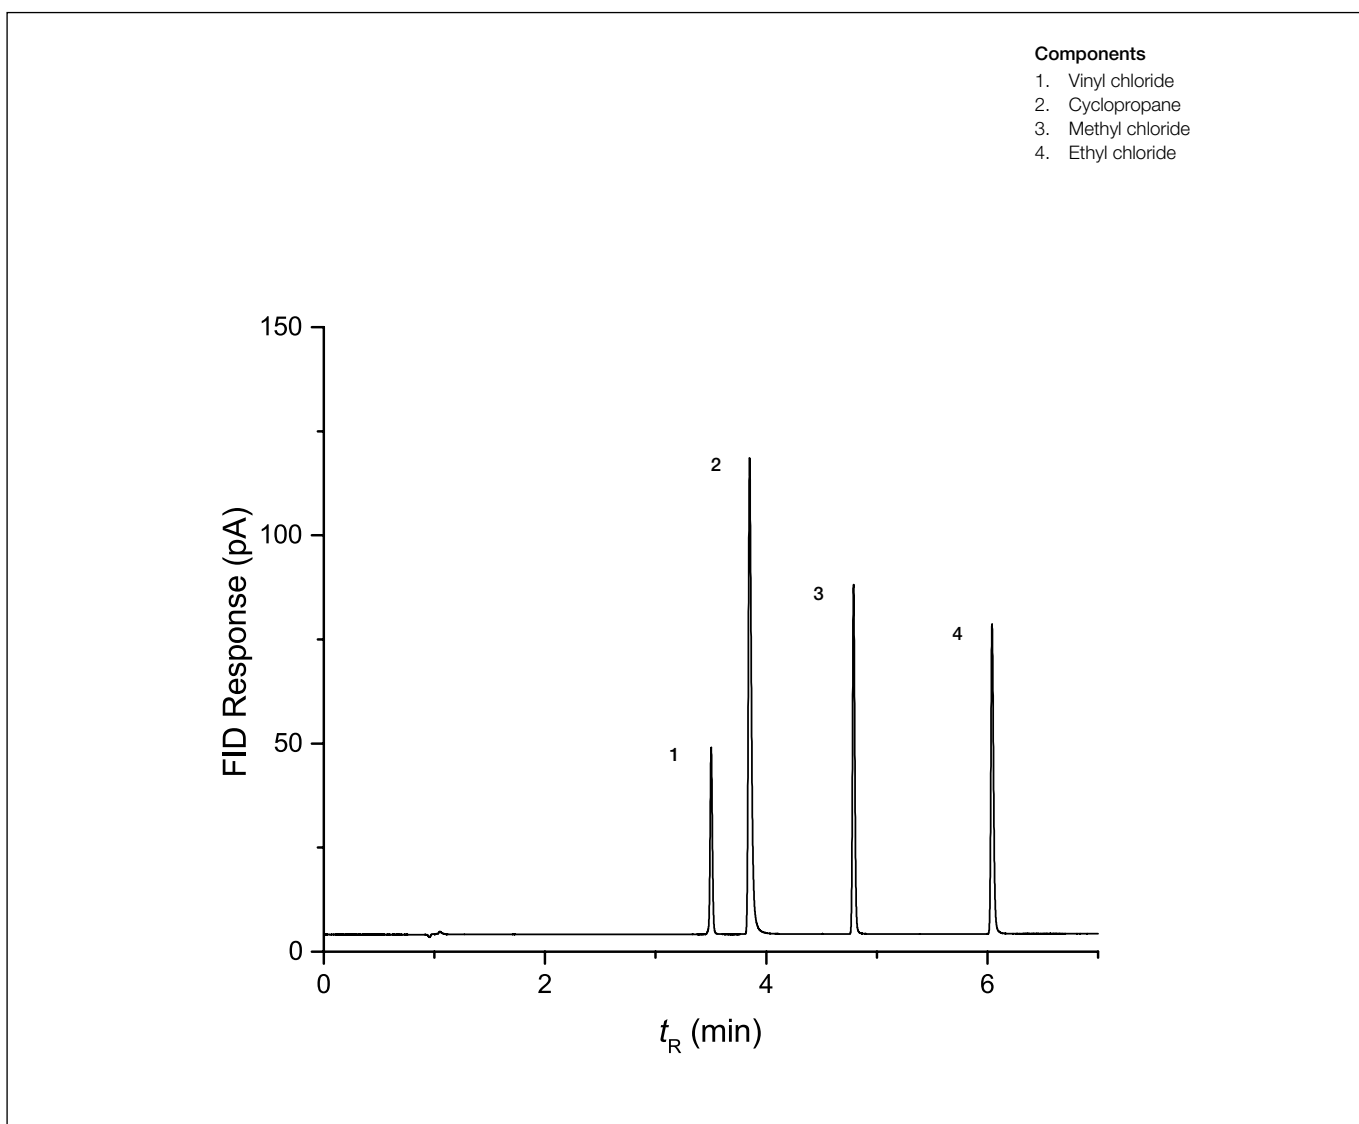

For more information visit www.trajanscimed.com or contact techsupport@trajanscimed.com