


Analysis of 15 organic acids

BP20 (WAX)

Column part number	054433		
Phase	BP20 (WAX)	Final temperature	260°C, 5 min
Column	30 m x 0.32 mm x 0.25 µm	Detector	FID
Initial temperature	70°C	Injection mode	Split
Rate	10°C/min	Carrier gas	H ₂ , 6 psi

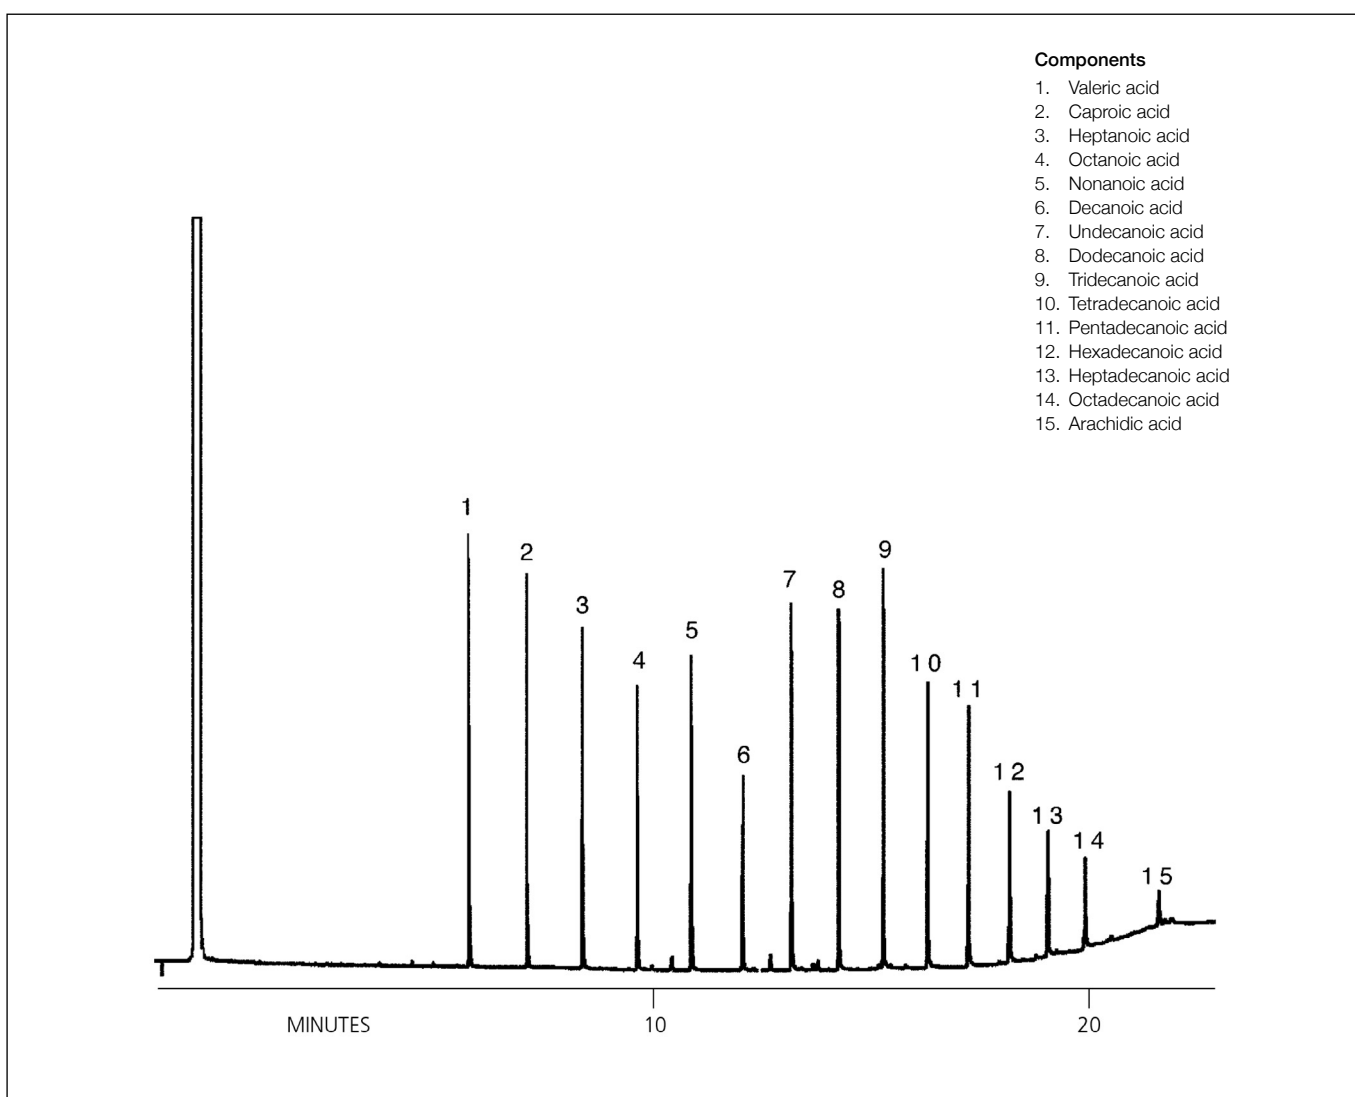

For more information visit www.trajanscimed.com or contact techsupport@trajanscimed.com