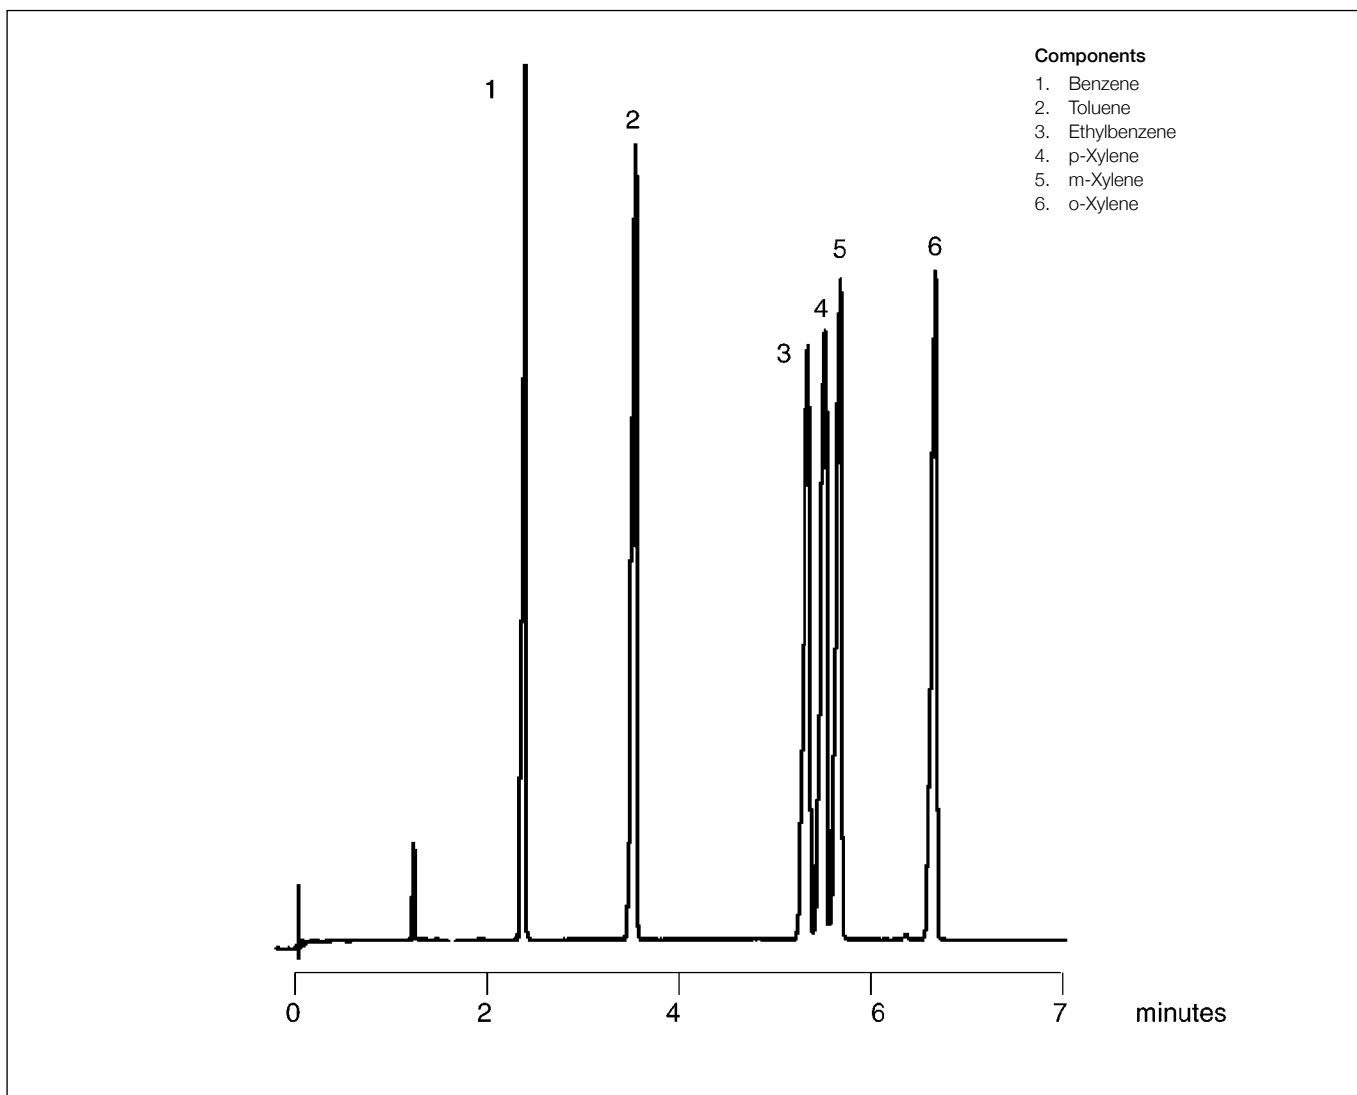


Analysis of aromatic pollutants in water

BP20 (WAX)

Column part number	054448		
Phase	BP20 (WAX)	Detector type	FID
Column	25 m x 0.53 mm x 1.0 μ m	Injection mode	Split
Initial temperature	Isothermal at 60°C	Carrier gas	H ₂


 For more information visit www.trajanscimed.com or contact techsupport@trajanscimed.com