


Analysis of polychlorinated p-dibenzodioxins


BPX5

Column Part Number	054114		
Phase	BPX5	Rate 3	5°C/min to 330°C
Column	50 m x 0.22 mm x 0.25 µm	Final temperature	330°C, 6 min
Initial temperature	80°C, 2 min	Detector	MS
Rate 1	4°C/min to 220°C	Carrier gas	He, 300 psi
Rate 2	5°C/min to 235°C, 7 min	Injection mode	Splitless, 270°C


Hexachlorodibenzodioxins

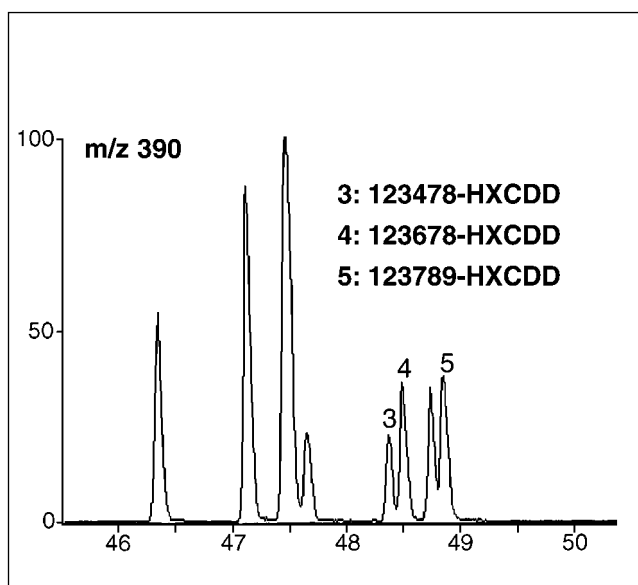


Tetrachlorodibenzodioxins

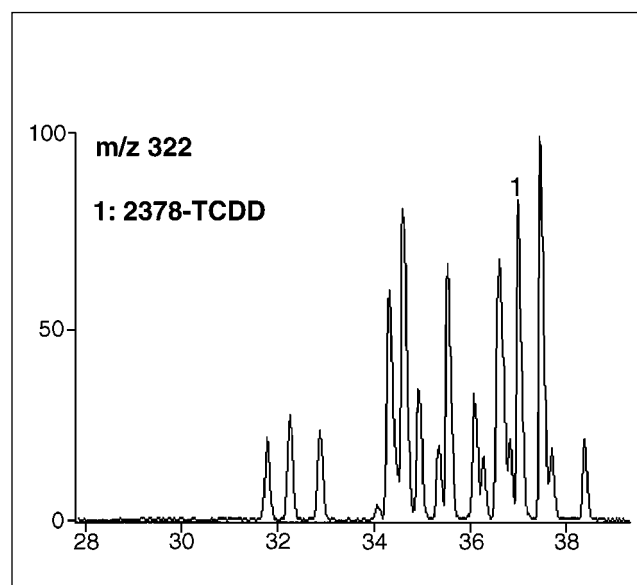

Heptachlorodibenzodioxins

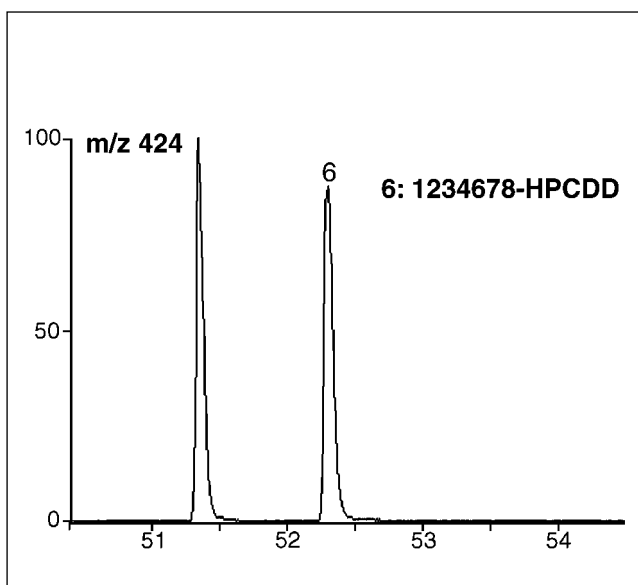

Pentachlorodibenzodioxins

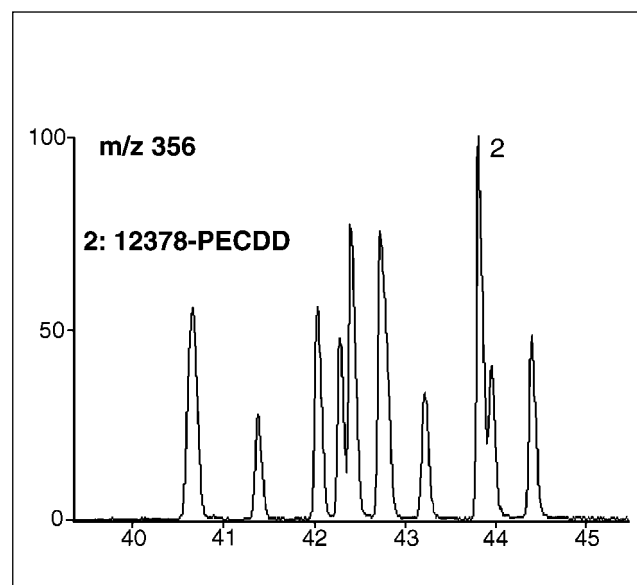


Acknowledgements: CARSO, 321 Avenue Jean Jaures, 69362 LYON CEDEX 7, FRANCE

Analysis of polychlorinated p-dibenzodioxins

BPX5

Octachlorodibenzodioxins

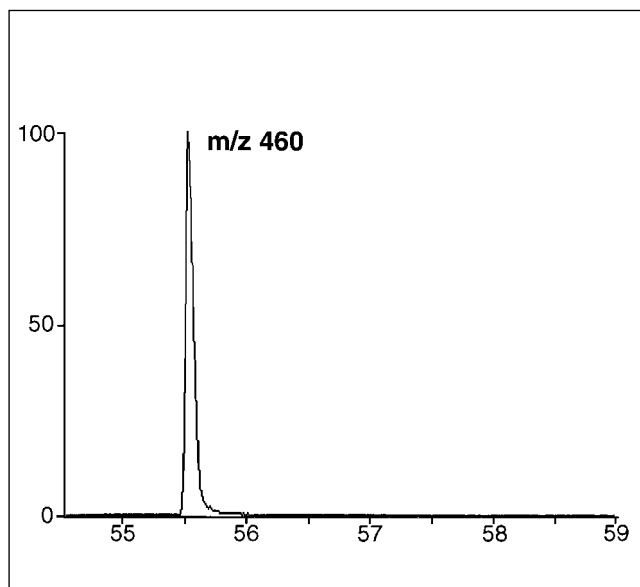

Acknowledgements: CARSO, 321 Avenue Jean Jaures, 69362 LYON CEDEX 7, FRANCE

For more information visit www.trajanscimed.com or contact techsupport@trajanscimed.com