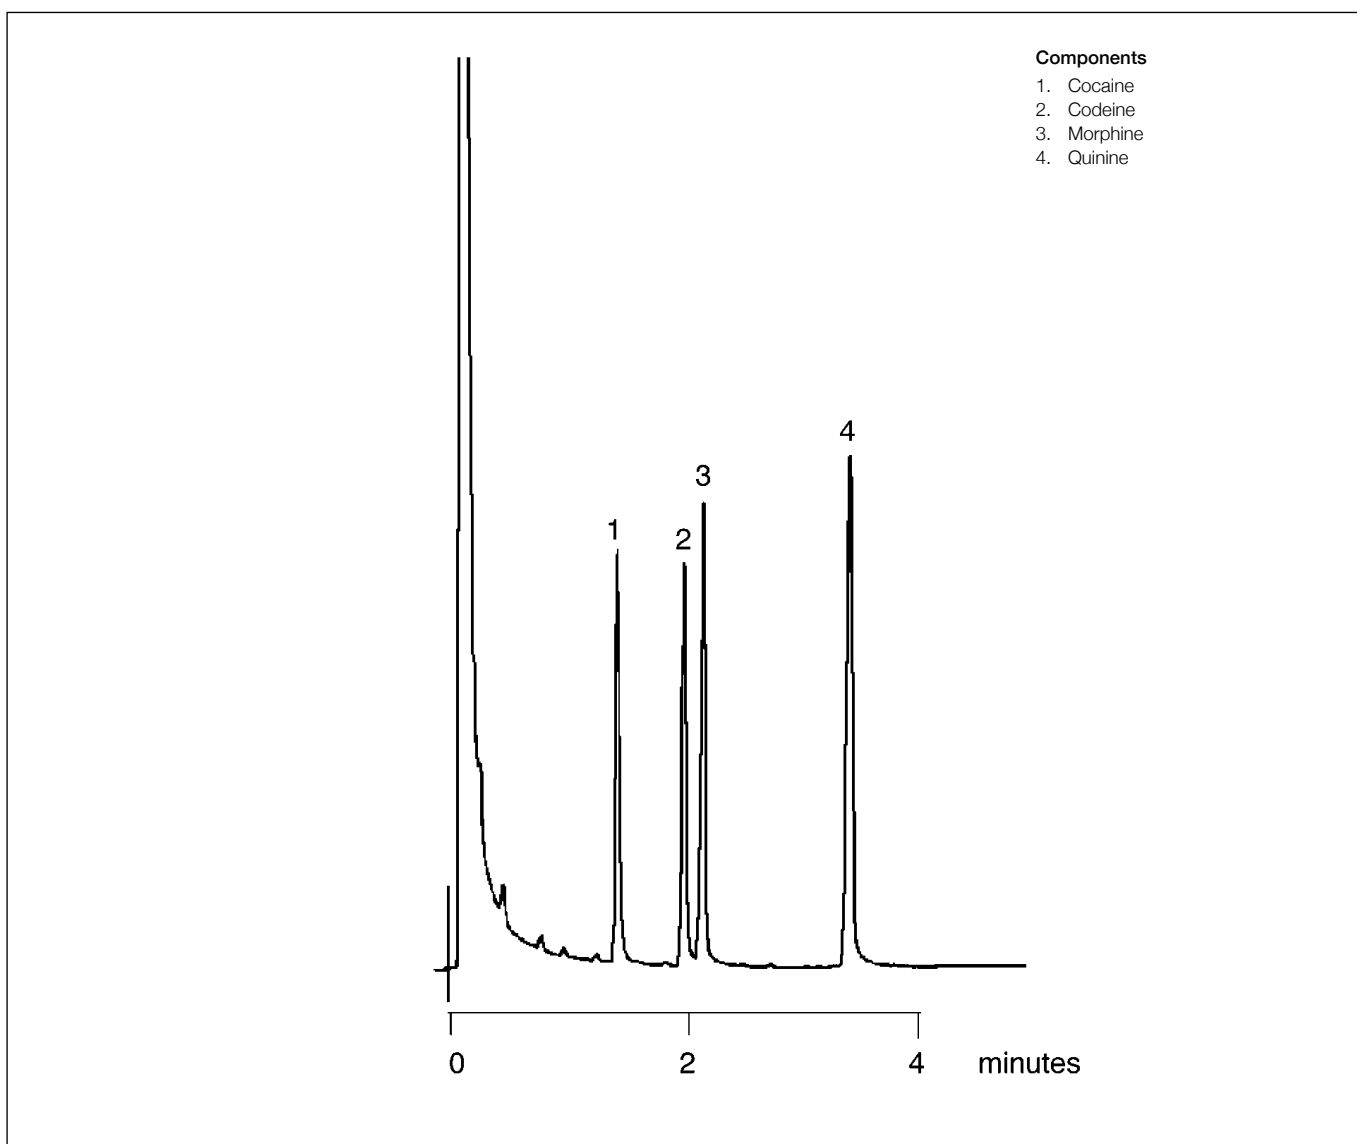


## Analysis of alkaloids

BP5

Column part number	054198		
Phase	BP5	Final temperature	300°C, 0 min
Column	25 m x 0.53 mm x 1.0 µm	Detector	FID
Initial temperature	200°C, 0 min	Injection mode	Split
Rate	25°C/min		


 For more information visit [www.trajanscimed.com](http://www.trajanscimed.com) or contact [techsupport@trajanscimed.com](mailto:techsupport@trajanscimed.com)