




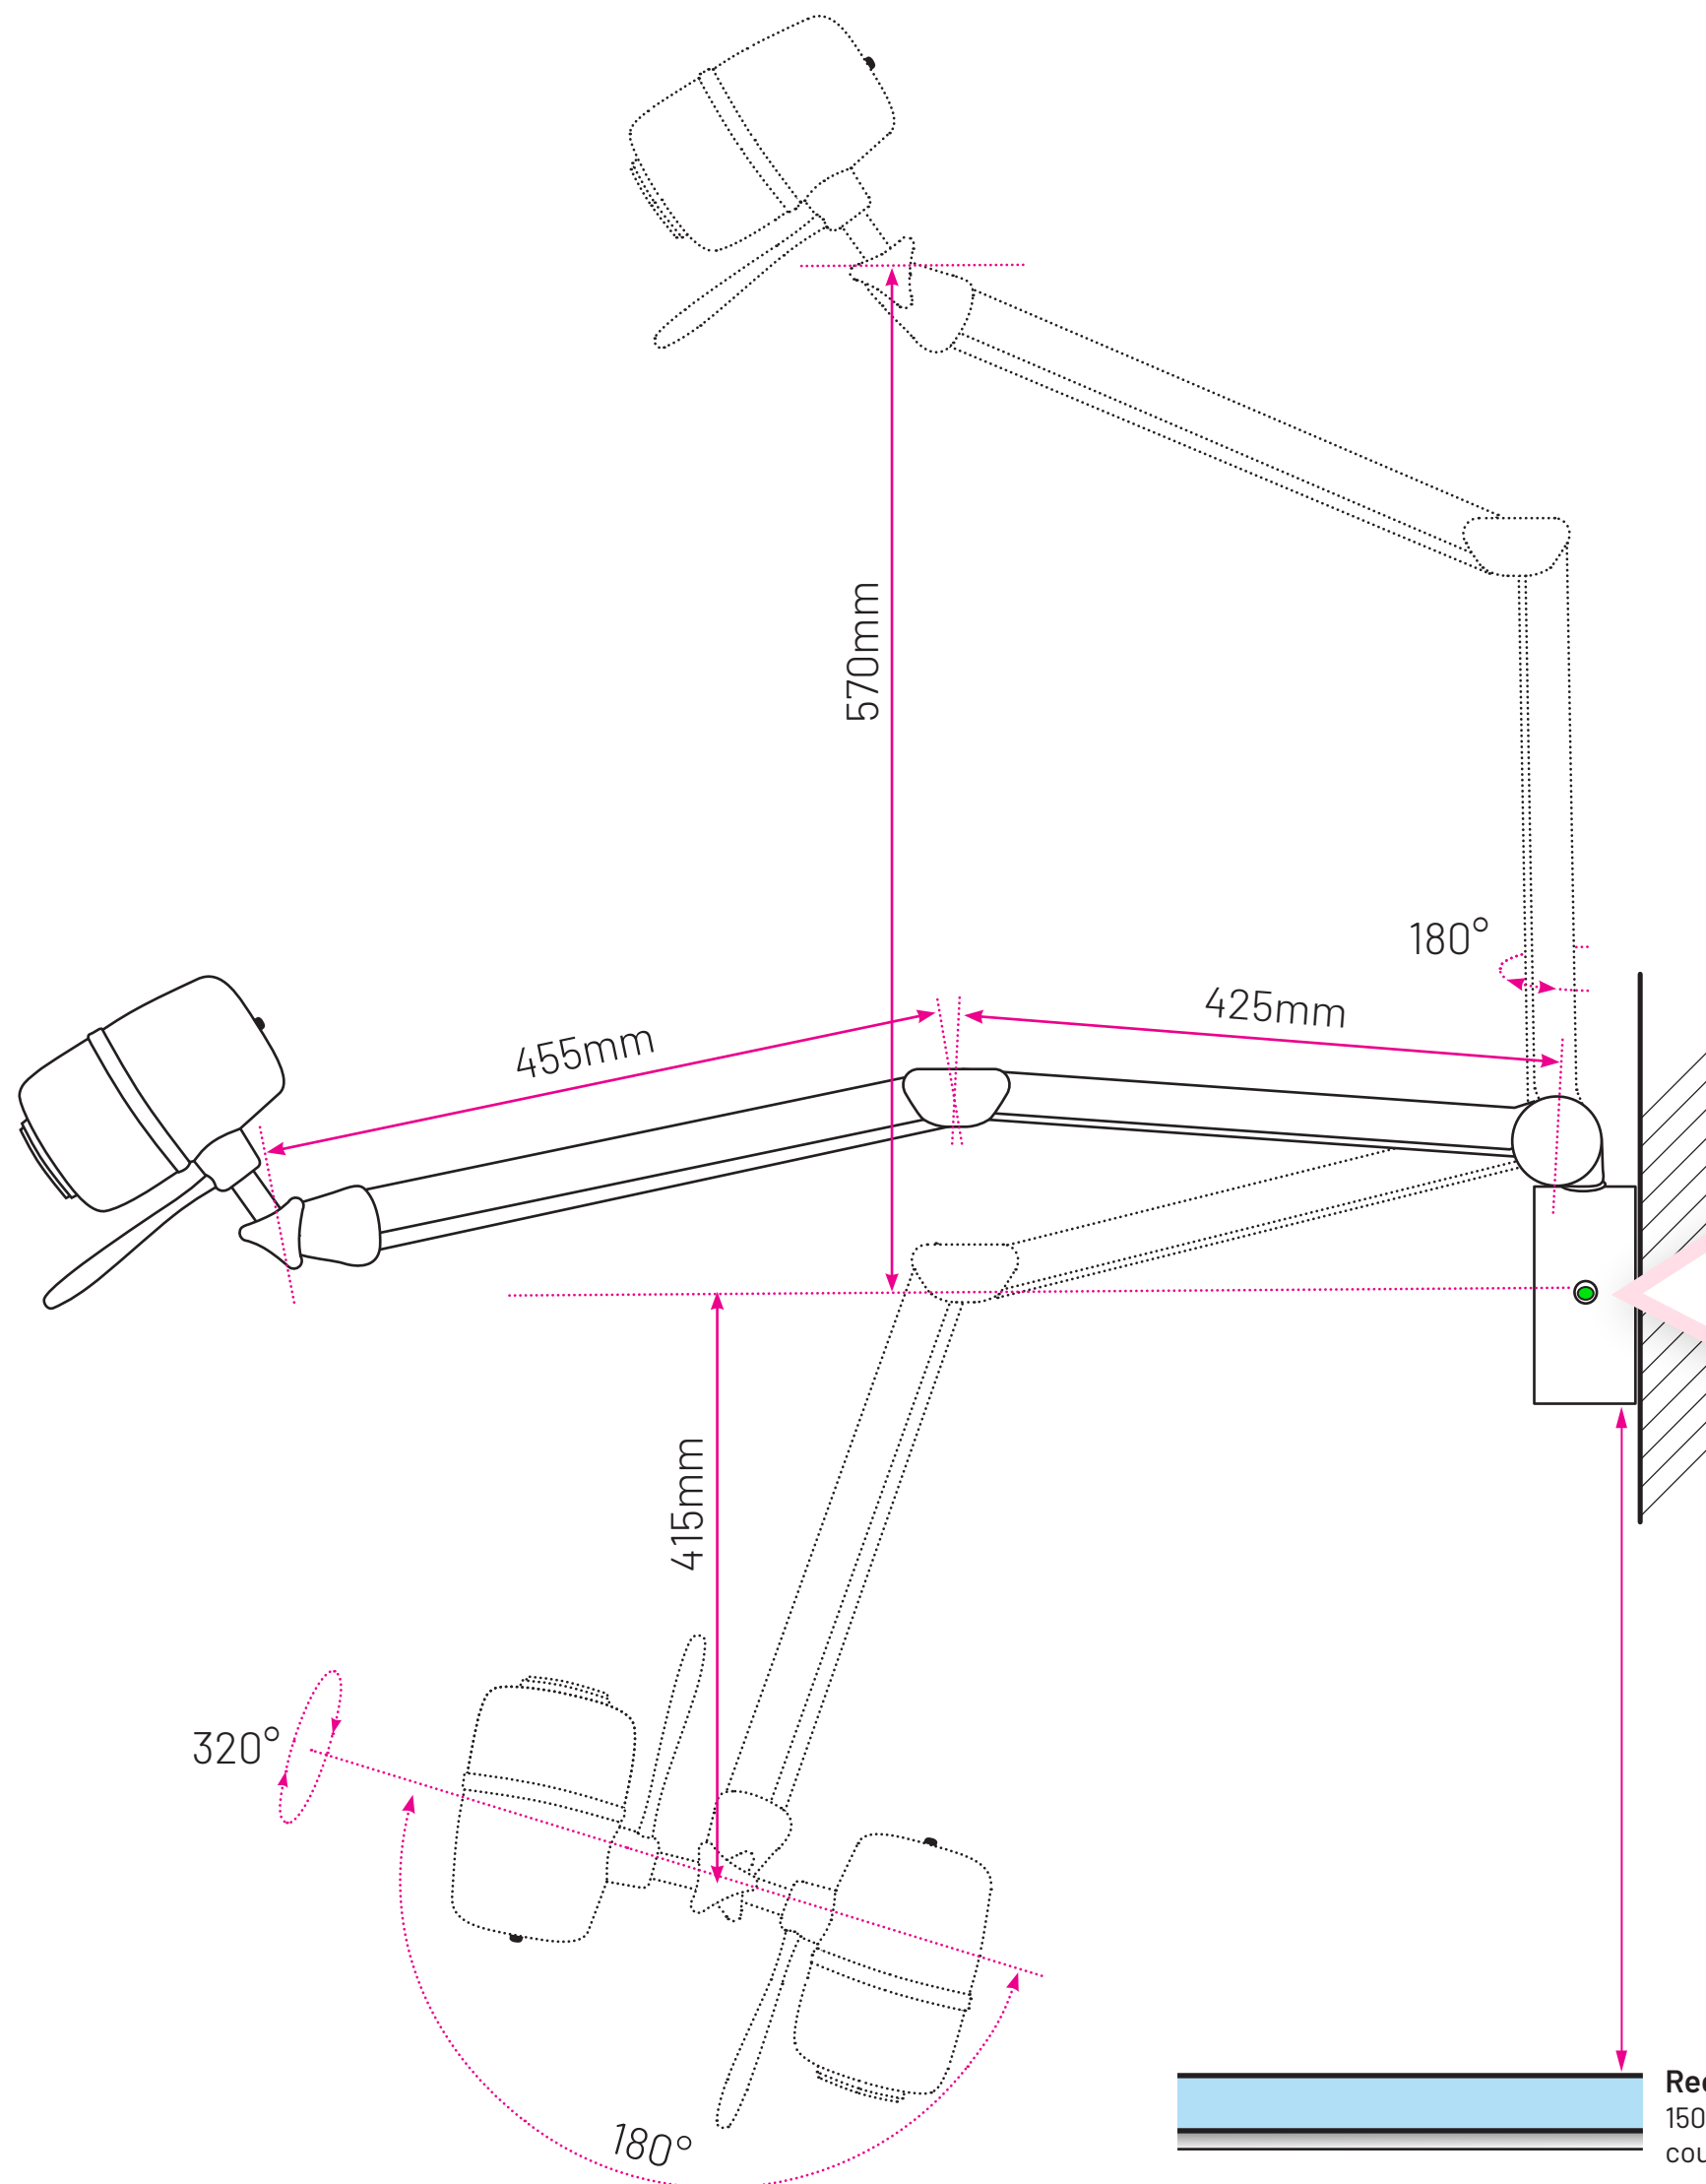

All dimensions in mm

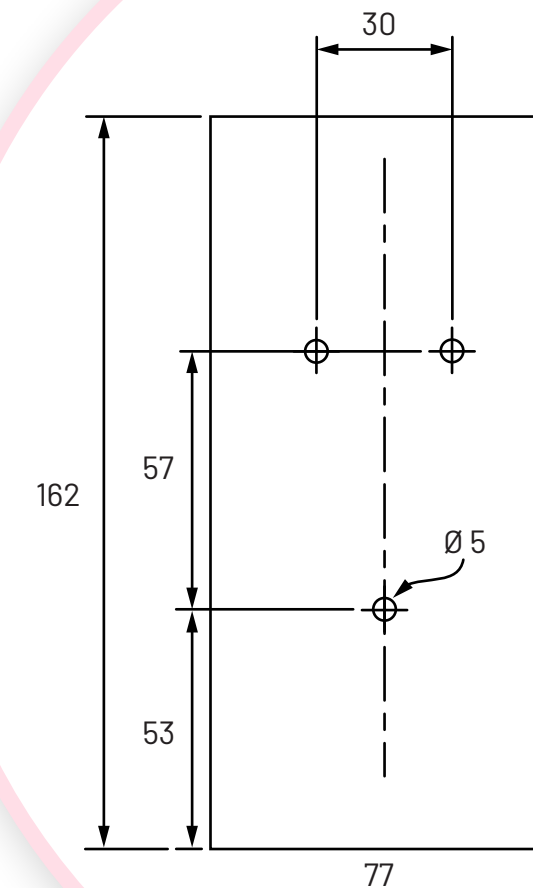

Rear view
(showing fixing points)

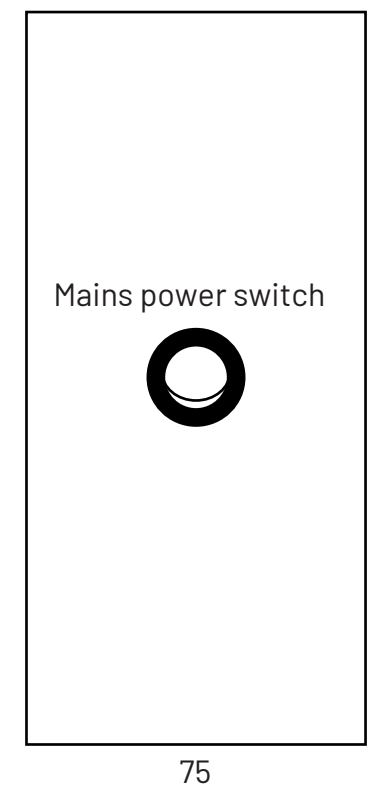

Side view

Recommended mounting height:
150 - 200mm from surface of examination
couch/table to underside of wall bracket