

# 570 IODINE FRESH TEST PROCEDURE



The 570 Iodine test procedure utilizes the **STANDARD STRIP METHOD** using the eXact iDip® 570 Smart Photometer System®. For tips on achieving best accuracy, and additional information regarding features of the eXact iDip® 570 photometer and the eXact iDip® app, please refer to the eXact iDip® Smart Guide. You can download a copy on our website at [exactidip.com](http://exactidip.com). **Test procedures can vary from test to test. Read full instructions and watch instructional video within the app.**


## YOU WILL NEED

- eXact iDip® 570 photometer
- Your smartphone/tablet with the eXact iDip® app installed
- (1) eXact® Strip Micro Iodine (Part No. 486627)
- Water sample for rinsing and testing (**NOT FOR USE WITH MARINE WATER. FRESH WATER ONLY**)

## 1 SELECT CUSTOMER

- Select **'Customers'** from the Home screen.
- Choose customer from list
  - OR** Tap **'Add customer from contacts'** and choose customer from your contacts list
  - OR** Tap **'+'** to create a new customer
- Android users: If no address is found, tap "No addresses found"
- c. Verify customer has been selected

*Note: To take full advantage of the GPS and Data Storage features, each test result must be linked to a contact. Individual users may select their contact listing.*

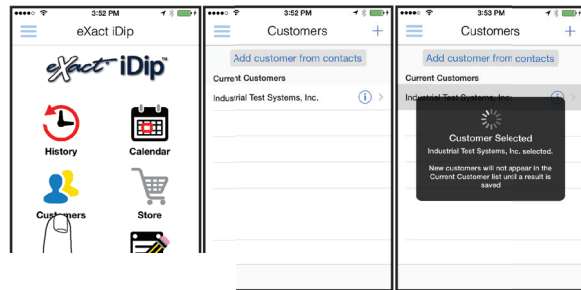

b

c


## 2 TAP ON



to power on the eXact iDip® 570

## 3 TOUCH TEST


'≡' and select 'Bluetooth Test' from the

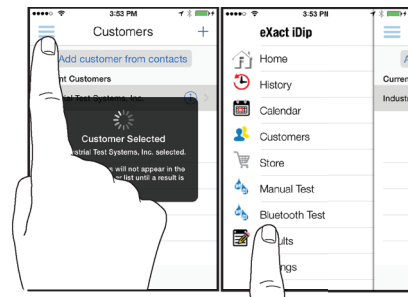

## 4 CONNECT EXACT IDIP® 570


The eXact iDip® app will automatically connect to the most recently used eXact iDip® 570 photometer. If not, select your eXact iDip® 570 from the bottom of the screen.

*Note: Always connect your eXact iDip® photometer via the Bluetooth® connection within the app. If you experience an issue connecting your device, check that your smartphone/tablet's Bluetooth® is turned on and your device is compatible.*

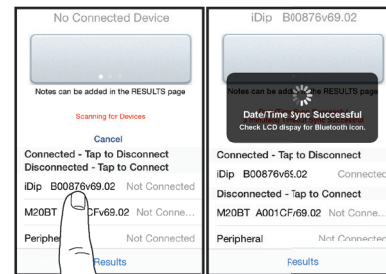

## 5 SELECT TEST

Tap **'SELECT Test'** at the top and select **570 Iodine Fresh I** (if this is not visible, purchase the test from the Store). The eXact iDip® 570 photometer and eXact iDip® app will both display the test selection for Iodine.

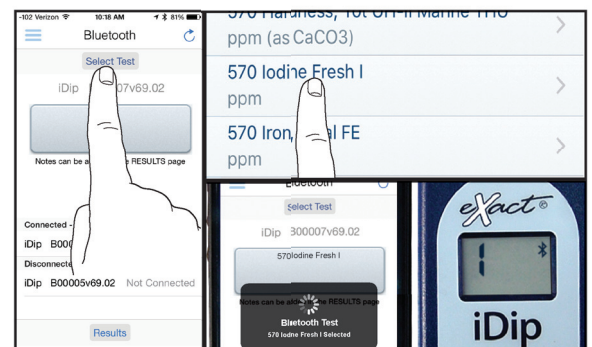

## 6 FILL CELL

Before testing, rinse CELL and clean with brush thoroughly. Finally, rinse the cell 3 times with the water sample to be tested, then **FILL** cell to capacity to begin test (refer to video in app).



**7 CAP CELL AND ZERO METE**

Place the Cell Cover onto the CELL and press the **ZERO/ON** button. The eXact iDip® 570 photometer display reads 0.00 PPM. The meter is ready for testing.

**ZERO/ON**



**8 REMOVE STRIP**

Remove one eXact® Strip Micro Iodine (Part No. 486627) and set in a dry, convenient place. Replace cap on bottle.




**9 READ**

Countdown and simultaneously **DIP** the strip into the sample, touching the bottom of the cell. Perform a circular motion (2 strokes per second) and discard the strip.



**10 CAP CELL AND READ RESULTS**

Place the Cell Cover onto the CELL and **READ** result displayed as 1.70 PPM.



**WITH BRUSH**

Remove the CELL immediately and clean with brush to thoroughly coat the CELL wall.



**TIPS**

- Due to the strip slitting process, you may find one or two strips that are noticeably smaller or larger in width than the normal strips in the bottle. These strips should be discarded. Using these strips may give unreliable results.
- Before running test unlock 570 Iodine test by purchasing in the Store.
- To obtain optimal accuracy when testing in direct sunlight, use the Cell Cover when zeroing and reading the sample.
- It is recommended to use the Cell Cleaning Brush with water to clean the CELL after each test to remove reagents which coat the CELL wall.
- DPD will stain the CELL wall if allowed to remain in the CELL. To remove staining, rinse cell thoroughly and fill with water then add two (2) drops of bleach (5%-8%) and clean with brush until stain is removed. Caution: Avoid contact of bleach with eyes and clothing.
- Be careful while dipping the strip (step 9). Do not spill the sample from the CELL.
- For a list of possible interferences with this test, see eXact iDip® Micro CL Interferences chart in your eXact iDip® Smart Guide.

**MANAGE YOUR RESULTS**

Save, send, and share results instantly using the eXact iDip® app. For step-by-step instructions, refer to the eXact iDip® Smart Guide. You can download a pdf copy on-line at [exactdip.com](http://exactdip.com).

