


TYPE A CERTIFICATE

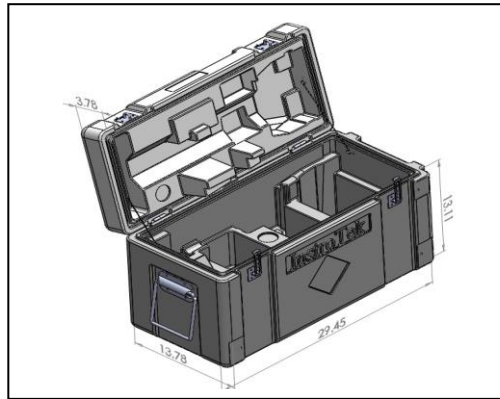

InstronTek, Inc.
One Triangle Drive
Research Triangle Park, NC 27709
Ph: (919) 875-8371

TESTING RESULTS FOR TYPE A PACKAGE

Gauge Shipping Case – Rotationally Molded Part Number 205.1043

| Gauge Type | Package Weight | Water Spray | Free Drop | Penetration | Compression | Vibration |
|------------|----------------|-------------|-----------|-------------|-------------|-----------|
| 3500 | 91 | Passed | Passed | Passed | Passed | Passed |
| 3401/3411 | 92.5 | Passed | Passed | Passed | Passed | Passed |
| 3430 | 87.5 | Passed | Passed | Passed | Passed | Passed |
| 3440 | 89 | Passed | Passed | Passed | Passed | Passed |

Water Spray – 49 CFR 173.465 (b) The structural integrity of the containers was not affected by the water spray tests.

Free Drop – 49 CFR 173.465 (c) There was no damage to the structural integrity of the package.

Penetration – 49 CFR 173.465 (e) Only cosmetic damage was the result and no structural damage was observed.

Compression – 49 CFR 173.465 (d) The shipping case withstood the weight that was placed on top of the case and passed the compression test. No visible damage occurred to the structural integrity, the latches, or to the safety features of the package.

Vibration – 49 CFR 173.410 (f) No deterioration or loosening of components was detected.