

MYCOPLASMA PNEUMONIAE ANTIBODY (IgG) TEST

Product No. 3120

IVD For *In Vitro* Diagnostic Use

INTENDED USE

ImmunoWELL Mycoplasma Pneumoniae Antibody (IgG) Test is a semi-quantitative or qualitative determination of IgG antibodies in human serum to *Mycoplasma pneumoniae* for the determination of immunological experience. The test may be used to evaluate paired sera for the presence of seroconversion and a significant increase in specific IgG and in the diagnosis of *Mycoplasma pneumoniae* infection in the adult population.

SUMMARY AND EXPLANATION

The order Mycoplasmales includes approximately 70 species, most of which are not found in humans. The genus *Mycoplasma* contains two species commonly found in man, *M. pneumoniae* and *M. genitalium*. These two species share lipid antigen specificities, and are therefore antigenically related. Two other human pathogens, *M. hominis* and *Ureaplasma urealyticum* are not serologically related to these.

Mycoplasma pneumoniae is the only known mycoplasma species that is a primary pathogen in man. Clinical manifestations can range from asymptomatic respiratory infections to severe pneumonia¹. *M. pneumoniae* accounts for 15 to 20% of total pneumonia^{2,3}. Other symptoms associated with *M. pneumoniae* infection include abnormalities of the central nervous system (meningitis, encephalitis), cardiac involvement (myocarditis, pericarditis), hemolytic anemia, arthritis, G.I. inflammations, and mucocutaneous reactions⁴. *Mycoplasma pneumoniae* is identified as a common infectious cause of Stevens - Johnson Syndrome, a well-defined systemic disease that can develop into a life-threatening illness in children⁵.

The *Mycoplasma pneumoniae* organism is sensitive to erythromycin and tetracyclines; however, it is resistant to drugs more routinely given in the treatment of acute pneumonia. Thus, a rapid and reliable diagnosis of *M. pneumoniae* infection is essential to proper patient management⁶. Culturing of *M. pneumoniae* is too difficult and slow for clinical diagnostic utility. Serology provides the primary diagnostic tool with current methods including complement fixation (CF), indirect immunofluorescence assays (IFA), immune adherence hemagglutination assay (IAHA) and enzyme immunoassay (EIA).

ASSAY PRINCIPLE

The ImmunoWELL Test utilizes an EIA microtiter plate technique for the detection of antibodies. Serum is added to antigen coated microtiter wells and allowed to react. After removal of unbound antibodies, horseradish peroxidase-conjugated antihuman IgG antibodies are allowed to react with bound antibodies. The bound peroxidase reacts with 2,2'-azino-di-[3-ethylbenzthiazoline sulfonate] (ABTS®), the chromogenic substrate, developing a color. Finally, the substrate reaction is stopped and the optical density is read with a spectrophotometric microwell reader.

REAGENTS

Reaction Wells coated with *Mycoplasma pneumoniae*, strain FH (ATCC #15531). The antigen is purified by chloroform and methanol extraction.

Specimen Diluent consisting of 0.01 M phosphate buffered saline (PBS, pH 6.2-7.6) and carrier protein containing <0.1% NaN₃

Calibrator consisting of human anti-*M. pneumoniae* prediluted 1:100 in Specimen Diluent

Positive Control consisting of human anti-*M. pneumoniae* serum containing <0.1% NaN₃

Negative Control consisting of a nonreactive serum substitute containing <0.1% NaN₃

Wash Buffer Concentrate consisting of a 20X concentrate of 0.01 M PBS (pH 6.2-7.6) and 0.05% Tween

Conjugate consisting of peroxidase-conjugated goat antihuman IgG in PBS (pH 6.2-7.6) and carrier protein containing preservatives

Substrate Buffer consisting of 0.1 M sodium citrate (pH 4.4-4.6) and 0.01% hydrogen peroxide

Substrate Concentrate 2.19% 2,2'-azino-di-[3-ethylbenzthiazoline sulfonate] (ABTS) in 0.1 M sodium citrate (pH 4.4-4.6)

Stop Solution 0.25 M Oxalic Acid

Warnings and Precautions

For *In Vitro* Diagnostic Use: ImmunoWELL reagents have been optimized for use as a system. Do not substitute other manufacturers' reagents or other ImmunoWELL Test reagents. Dilution or adulteration of these reagents may also affect the performance of the test. Do not use any kits beyond the stated expiration date. Close adherence to the test procedure will assure optimal performance. Do not shorten or lengthen stated incubation times since this may result in poor assay performance.

Some reagents contain sodium azide that may react with lead and copper plumbing to form highly explosive metal azides. On disposal, flush with a large volume of water to prevent azide build-up.

Warning - Potential Biohazardous Material: Human sera used in the preparation of this product were tested using FDA approved procedures and found non-reactive for hepatitis B surface antigen and for antibodies to HIV-1, HIV-2, and hepatitis C virus. Because no test method can offer complete assurance that infectious agents are absent, handle reagents and patient samples as if capable of transmitting disease.

Reconstitution and Storage

Kit is stored at 2-8°C. Assuming good laboratory practices are used, opened reagents remain stable as indicated by the expiration date.

Reaction wells are removed from the foil pouch and unused wells are resealed in the pouch using the integral zip-lock.

Wash Buffer (pH 6.2-7.6) is prepared by adding the contents of the Wash Buffer Concentrate (20X) bottle into 1 liter of distilled/deionized water. After reconstitution, the 1X solution is stored at 2-8°C. Discard when visibly turbid.

Note: In some instances the Wash Buffer Concentrate (20X) may develop crystals upon storage at 2-8°C. It is important that these crystals are completely redissolved before dilution of the Concentrate. This can be accomplished by warming the Concentrate to 37°C in a water bath with occasional mixing.

Color Developer is prepared by adding one (1) drop of Substrate Concentrate to 1mL of Substrate Buffer. One mL of Color Developer is sufficient for one eight-well strip. **Use within one hour.**

SPECIMEN COLLECTION AND HANDLING

ImmunoWELL Test is performed on serum. The test requires 10 µL of serum. Lipemic, hemolyzed and icteric serum have not been shown to be acceptable specimens. Serum is collected according to standard practices and may be stored at 2-8°C for up to five days. Serum may be frozen below -20°C for extended periods.

Two sera, one collected during the acute disease phase and the other collected at least one week later (convalescent), are used.

PROCEDURE

Materials Provided

Microtiter Wells in Carrier	Specimen Diluent
Positive Control	Calibrator
Negative Control	Conjugate
Wash Buffer Concentrate (20X)	Substrate Concentrate
Substrate Buffer	Package Insert
Stop Solution	

Materials Required But Not Provided

Distilled or deionized water	Test tubes
Microwell washer	Pipets
Microwell spectrophotometer (405 nm), capable of measurement to 2.00 absorbance units	

Performance Considerations

Reproducibility in the assay is largely dependent upon the consistency with which the microwells are washed. Carefully follow the recommended washing sequence as outlined in the assay procedure.

Positive and Negative Control Sera (undiluted) - These control sera are used to assure test performance.

Calibrator (prediluted 1:100) is used to standardize between run values.

Substrate Blank- All reagents, except serum, are added to the substrate blank well. This blank well is intended to baseline (zero) the microwell spectrophotometer.

Assay Procedure

1. Allow all components including diluted Wash Buffer to warm to room temperature (22-27°C).
2. Determine the total number of specimens to be run. Include one blank and duplicates of calibrator and controls in each run.
3. For each control and specimen, pipet 10 µL serum into a clean tube containing 1 mL Specimen Diluent and mix (1:100 dilution).

CAUTION: Calibrator is prediluted. Do not dilute further.

4. Determine the total number of wells to be run including blank, calibrators, controls and specimens. Well strips can be broken to the exact number needed to conserve reagent wells. Strips need to be completed with used wells to facilitate washing procedures.
5. Add 100 µL of Specimen Diluent into the first well as a substrate blank.
6. Pipet 100 µL of the prediluted calibrator and the diluted controls and specimens into each assigned well.
7. Incubate at room temperature (22-27°C) for 60±2 minutes.
8. Aspirate the samples out of the wells.
9. Wash the wells three times by completely filling the wells with Wash Buffer (see Reconstitution and Storage) and aspirating the wells completely after washes.
10. Pipet 100 µL Conjugate into all wells.
11. Incubate the wells at room temperature (22-27°C) for 30±2 minutes.
12. Aspirate the conjugate out of the wells.
13. Wash the wells three times as described in step 9.
14. Prepare fresh Color Developer (see Reconstitution and Storage).
15. Pipet 100 µL of Color Developer into each well.
16. Incubate at room temperature (22-27°C) for 30±2 minutes.
17. Add 100 µL of Stop Solution to each well.
18. Inspect the outside bottom surface of the microwells for the presence of condensation, dried buffer salts or wash solution which might interfere with the spectrophotometric reading. Carefully clean the well bottoms with a soft tissue.
19. Using the substrate blank to zero the spectrophotometer, read the optical density of each well at 405 nm within 30 minutes of completion of step 17.

NOTE: It is recommended that dual wavelength spectrophotometers use only one wavelength, 405 nm.

Quality Control

GenBio provides positive and negative controls with defined ranges. Interpretations should not be made unless the control results fall within these limits. In addition, the laboratory should act in accordance with laboratory accreditation requirements and/or individual laboratory monitoring programs.

INTERPRETATION

If either the acute or convalescent sample is classified as an IgM positive (> 950 U/mL), IgG evaluation is not required. If paired sera are available, follow the Seroconversion Method as described below. If only one specimen is available, follow the single specimen method as described below.

Calculation of Activity (U/mL)

The assigned value (U/mL) of the calibrator used in the calculation below will vary by lot number. Please verify that the lot number on the vial matches the lot number on the Package Insert Supplement to assure the proper value is used in the calculation.

In order to eliminate the effects of washing variation, instrument variability, etc., specimen values are normalized according to the following calculation:

$$A_N = (A_S \times A_{V_C}) / A_C$$

Where:

- A_N = Normalized activity of the specimen (U/mL)
- A_S = Absorbance of the specimen
- A_C = Mean absorbance of the calibrator obtained in the assay
- A_{V_C} = Assigned Value (U/mL) of the calibrator given in the Supplement

Single Specimen Method

The activity is interpreted and reported as follows:

Interpretation

<100	Result Negative, No detectable IgG antibody - Suggests no prior immunological exposure to <i>Mycoplasma pneumoniae</i> . Result does not rule out recent exposure and collection of test sample prior to development of IgG. Culture is recommended for determining current infection.
100-320	Equivocal - Immunological exposure cannot be assessed. Samples that remain equivocal after repeat testing should be retested by an alternate method, e.g., immunofluorescence assay (IFA). If results remain equivocal upon further testing, an additional sample should be taken.
>320	Positive Detectable IgG Mycoplasma antibody - Indicates presence of detectable IgG antibody. Suggests immunological exposure to <i>Mycoplasma pneumoniae</i> .

Seroconversion Method (one or both samples <200 units)

Values below 200 units are inherently imprecise and should not be used to calculate ratios. If either IgG value is below 200 units, the seroconversion method should be used. Otherwise, the ratio calculation method should be used. A significant change (seroconversion) is indicated if one sample is above 320 units and the other is below 200 units. (See Table 1)

Table 1: Seroconversion Interpretation

Acute	Convalescent	Indication
≤200	>320	Significant <i>M. pneumoniae</i> antibody rise indicating current or recent infection
≤200	≤320	No significant <i>M. pneumoniae</i> antibody change detected
>320	≤200	Significant <i>M. pneumoniae</i> antibody fall indicating recent past infection

Ratio Method (Neither sample <200 units)

A ratio is calculated by dividing the convalescent sample result by the acute sample result. Either absorbance values or activities (U/mL) may be used to calculate the ratio. Interpretations are made as described in Table 2. If both values are above 1500 units, no interpretation is possible since the assay is not reliably linear beyond 1500 units.

Table 2: Ratio Method Interpretation

<u>Ratio</u>	<u>Indication</u>
≥2.0	Significant <i>M. pneumoniae</i> antibody rise indicating current or recent infection.
≤0.5	Significant <i>M. pneumoniae</i> antibody change detected
>0.5 and <2.0	No significant <i>M. pneumoniae</i> antibody change detected

Examples of both methods are shown in Table 3.

Table 3: Examples

<u>Acute</u>	<u>Convalescent</u>	<u>Indication</u>
260	977	(Ratio – 3.8) Significant <i>M. pneumoniae</i> antibody rise indicating current or recent infection
260	384	(Ratio = 1.5) No significant <i>M. pneumoniae</i> antibody change
1893	256	(Ratio = 0.1) Significant <i>M. pneumoniae</i> antibody fall indicating past infection
456	134	(Seroconversion) Significant <i>M. pneumoniae</i> antibody fall indicating recent past infection

It is unknown whether IgG antibody cross-reactivity may occur with other organisms that cause similar symptomatology. It is recommended that assays to detect other agents or antibodies to other agents always be performed in conjunction with this assay.

The *M. pneumoniae* antibody levels obtained from the assay are an aid to diagnosis only. In most cases, a positive antibody result will provide laboratory support of *M. pneumoniae* infection. However, specific IgM may persist for several months after initial infection or be absent during early infection or reinfection. Each physician must interpret these results in light of the patient's history, physical findings, and other diagnostic procedures.

LIMITATIONS

The state of present-day technology does not provide a recommended reference standard. Because of the current inconsistencies in various test methodologies, physicians and laboratories must rely on a combination of test methods, results and clinical symptoms when making a diagnosis of *Mycoplasma pneumoniae* infection. This test is not intended to replace culture, and should not be used as the sole basis for diagnosis.

False positive results may occur with sera from patients with other *Mycoplasma* infections, pancreatitis, bacterial meningitis and other acute inflammatory disease. Cross-reactivity of this assay with antibodies to the above disease states has not been determined. Epidemiology of case, symptoms and other laboratory tests can help in differentiating these conditions from *Mycoplasma pneumoniae*.

Icteric, lipemic, hemolyzed or heat inactivated sera may cause erroneous results and should be avoided.

A negative antibody result does not rule out *Mycoplasma pneumoniae* infection. False negative results may occur when samples are drawn too early after onset. Production of detectable antibody levels may be delayed. Some patients may never generate detectable antibody levels. Patients with symptoms suggestive of *Mycoplasma pneumoniae* infection with negative test results should be retested in 4-6 weeks using paired sera analysis.

Mycoplasma pneumoniae infection can have a long incubation period, thus elevated antibody titers in the acute specimen are common, and reinfection may occur. Therefore, seroconversion (negative to positive) is unusual.

A positive single serum result only indicates prior exposure to *Mycoplasma pneumoniae*. The antibody level in a single specimen does not have significance for disease severity. The presence or absence of antibody cannot be used to determine the success or failure of antibiotic therapy.

Screening of the general population should not be performed. Testing should only be performed when clinical symptoms are present or exposure is suspected.


The results of ELISA immunoassays performed on serum from immunocompromised patients must be interpreted with caution.

EXPECTED RESULTS

It is reported that the percentage of pneumonias caused by *M. pneumoniae* is 10-33% in the general population, 35-74% in children (5-19 years old), 27-52% in college students, 8-54% in military recruits and 7-17% in civilian adults⁷.

An increase of IgG relative to IgM antibodies occurs with time after onset of illness. Also, adults respond with higher IgG antibody ratios than do children². IgM titers are significant in a high percentage of patients at admission¹. Seventy-five normal sera from asymptomatic blood donors were tested and the reported IgG activities (U/mL) are shown in Figure 1.

Figure 1: Normal Sera

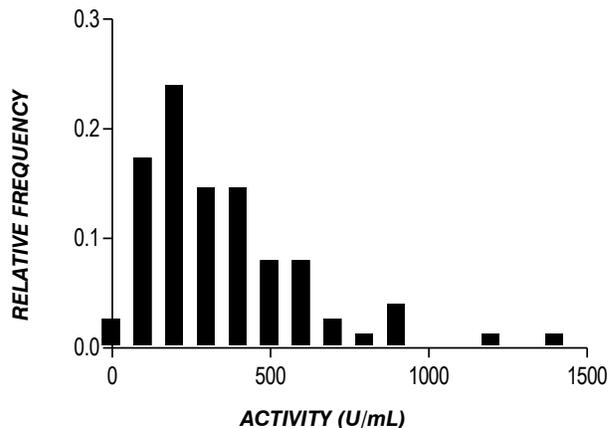

PERFORMANCE CHARACTERISTICS

Reference results (CF or IAHA method) are classified as: 1) greater than a four-fold titer increase, 2) single value above 1:1024 titer, 3) falling titer greater than four-fold, or 4) no significant change. Paired samples were not selected by the sites, but were frozen and retrospectively evaluated.

Note: The majority of samples are from reference laboratories that may receive selected samples. Since assay performance depends on the prevalence of disease in a population, users may not see the same performance in their laboratory.

Sensitivity

Table 4 compares reference method results to ImmunoWELL IgG results, not taking into account ImmunoWELL IgM test results. Combining the CF and IAHA rise, fall and greater than or equal to 1024 titer results as significant positives, the relative sensitivity is 81% (67-90%). The relative specificity is 100% (66-100%).

**Table 4: Relative Performance (Only ImmunoWELL IgG Results)
CF and IAHA Combined**

ImmunoWELL IgG Ratio Results		<u>Rise</u>	<u>Fall</u>	<u>1024 Titer</u>	<u>No Change</u>	<u>Total</u>
ImmunoWELL IgG Ratio Results	Agree	34	6	2	0	42
	Disagree	2	4	4	9	19
	Total	36	10	6	9	61

Using the same pairs evaluated in Table 4, pairs showing an ImmunoWELL IgM positive result are excluded from IgG consideration. The relative performance of ImmunoWELL IgG to CF and IAHA results is shown in Table 5. There is 75% (43-95%) agreement with traditional serology testing for positive pairs and 100% (66-100%) agreement for negative pairs.

Table 5: Relative Performance (Without IgM Positives)

ImmunoWELL IgG Ratio Results (without IgM positive pairs)		CF and IAHA Combined				<u>Total</u>
		<u>Rise</u>	<u>Fall</u>	<u>1024 Titer</u>	<u>No Change</u>	
ImmunoWELL IgG Ratio Results (without IgM positive pairs)	Agree	7	1	0	8	16
	Disagree	2	1	0	0	3
	Total	9	2	0	8	19

Overall relative performance following both ImmunoWELL IgM and IgG package insert guidelines is shown in Table 6. The sensitivity is 96% (87-100%) and specificity is 89% (52-100%).

Table 6: Relative Performance (IgM and IgG Results)

ImmunoWELL IgM and IgG Ratio Results		CF and IAHA Combined				<u>Total</u>
		<u>Rise</u>	<u>Fall</u>	<u>1024 Titer</u>	<u>No Change</u>	
ImmunoWELL IgM and IgG Ratio Results	Agree	35	9	6	8	58
	Disagree	1	1	0	1	3
	Total	36	10	6	9	61

Performance of standard serology methods using both ImmunoWELL IgM and IgG results shows a relative sensitivity of 95% (58/61) and a relative specificity of 89% (8/9). Since the above studies represent a selected population, no positive or negative predictive values may be calculated.

Note: Please be advised that "relative" refers to the comparison of this assay's results to that of a similar assay. There was not an attempt to correlate the assay's results with disease presence or absence. No judgment can be made on the comparison assay's accuracy to predict disease or infection.

Specificity

Forty-five sera collected from asymptomatic blood donors were used to assess specificity. Two separate dilutions to mimic acute and convalescent preparations were made from each sample. The two dilutions (i.e., acute and convalescent) were tested in ImmunoWELL and the ratios were calculated as described in the INTERPRETATION section. In no case was a significant titer rise observed. Therefore the specificity is 100% (92-100%).

Reproducibility

Twenty assay runs, testing samples in duplicate, using common reagents on twenty different days were made at GenBio. The assay's results are shown in Table 7.

Caution: EIA precision may vary between laboratories.


Table 7: Assay Precision

<u>Ratio</u>	<u>Within Run Variation (% CV)</u>	<u>Between Day Variation (% CV)</u>
5.8	11%	29%
2.6	8%	19%
2.1	10%	23%

ASSAY LINEARITY

Triplicate, two-fold serial dilutions of one positive serum were tested in duplicate. The results are shown in Figure 2. The r_2 is 0.92 and the linear regression runs test supports linearity from 200 to 1500 units.

Figure 2: Assay Linearity

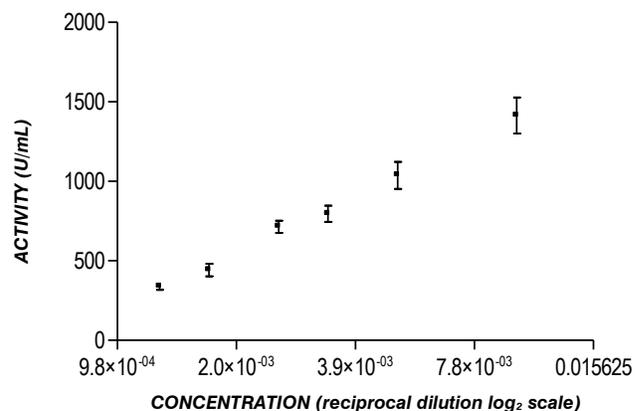

BIBLIOGRAPHY

1. Ali, NH, M Sillis, BE Andrews, PF Jenkins, BDW Harrison. The Clinical Spectrum and Diagnosis of *Mycoplasma pneumoniae* Infections. *Q J Med* 58:227, 241(1986)
2. Foy, HM. *Mycoplasma Pneumoniae*, pp 345-366. In AS Evans and HA Feldman (ed.), *Bacterial Infections of Humans: Epidemiology and Control*. Plenum Publishing, New York (1982)
3. Foy, HM, GE Kenny, MK Cooney, and ID Allen. Long Term Epidemiology of Infections with *Mycoplasma pneumoniae*. *J Infect Dis* 139:681(1979)
4. Cherry, JD, ES Hurwitz, RC Welliver. *Mycoplasma pneumoniae* Infections and Exanthems. *J Pediatr* 87:369(1975)
5. Levy, M and NH Shear. *Mycoplasma pneumoniae* Infections and Steven-Johnson Syndrome: Report of Eight Cases and Review of the Literature. *Clin Pediatr* 30:42(1991)
6. Sillis, M. The Limitations of IgM Assays in the Serological Diagnosis of *Mycoplasma pneumoniae* Infections. *J Med Microbiol* 33:253(1990)
7. Keitel, WA, and RB Couch. Mycoplasmal pneumonia: In the differential all year. *J Resp Dis* June:119(1985)

QUICK REFERENCE PROCEDURE

ImmunoWELL Mycoplasma IgG

- Prepare Wash Buffer from Wash Concentrate.
- Dilute each control and specimen 1:100 in Specimen Diluent.
- Add 100 μ L of Specimen Diluent into the first well as a substrate blank.
- Pipet 100 μ L of the prediluted calibrator, controls and specimens into coated microwells and incubate 60 min at room temperature.
- Aspirate microwells and wash microwells three times with Wash Buffer.
- Pipet 100 μ L of Conjugate into microwells and incubate 30 min at room temperature.
- Aspirate microwells and wash microwells three times with Wash Buffer.
- Prepare fresh Color Developer.
- Pipet 100 μ L of Color Developer into microwells and incubate 30 min at room temperature
- Pipet 100 μ L of Stop Solution into microwells and read results at 405 nm.

To place an order for ImmunoWELL products, contact your local distributor, or call GenBio directly for the distributor nearest you and for additional product information.

For assistance, please call toll-free 800-288-4368.

ABTS® is a registered trademark of Boehringer Mannheim GmbH



15222-A Avenue of Science
San Diego, CA 92128



EMERGO EUROPE

Molenstraat 15

2513 BH, The Hague

The Netherlands