



CUSTOMER:	P/N: MD903	REV.	APPROVED BY:
6096±50			
REVISIONS DESCRIPTION DATE			
REV.	△		
△			
△			
△			
△			

NOTES:


1. RoHS shown on the carton

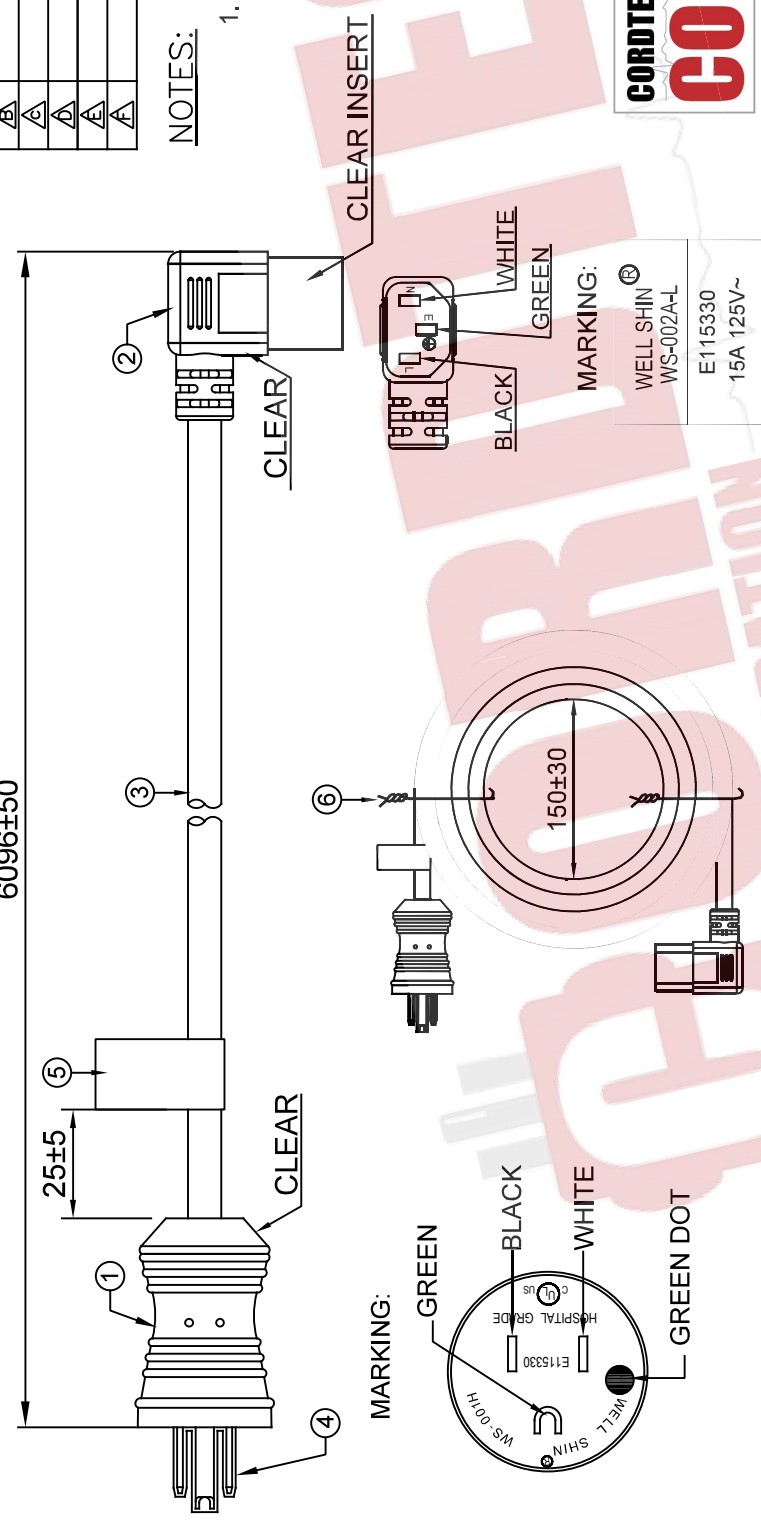

NEMA 5-15P HOSPITAL GRADE CLEAR
IEC-60320-C13 LEFT ANGLE CLEAR

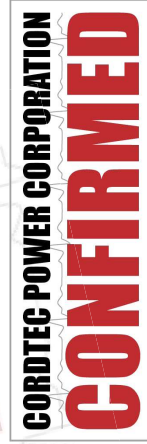

⑤ Hosp. Grade label

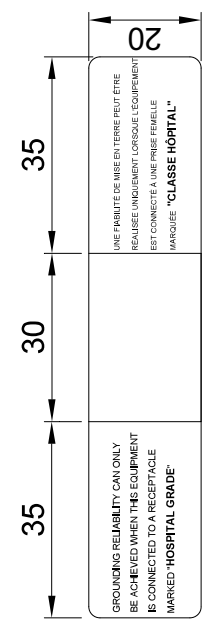

ITEM	DESCRIPTION	COLOR	QTY
⑥	Cable tie	WHITE	2
⑤	Hosp. Grade label	---	1
④	Plastic cap	WHITE (GY-H)	1
③	SJTW 14AWG 3C 105°C APPROVAL :UL,CSA	PANTONE Cool Grey 9C	1
②	WS-002A-L 15 (A) 125(V) APPROVAL :UL,CUL	CLEAR	1
①	WS-001H 15 (A) 125(V) APPROVAL :UL,CUL	CLEAR	1

SIGNATURE	
SAFETY ENGINEER:	
MANAGER BY:	
CHECKED BY:	
DRAWN BY:	



AC Connectors of Cordtec Power Corp
 Main: 1-414-434-2920 Fax: 1-414-323-8386 Text: 1-414-323-3240
 Email: Info@CordtecPower.com
 Website: CordtecPower.com/ ACWORKS.com

