


LINE2design, Inc. Manual Track Stair Chair Track Stair Chair - Yellow
Item # 70007-Y

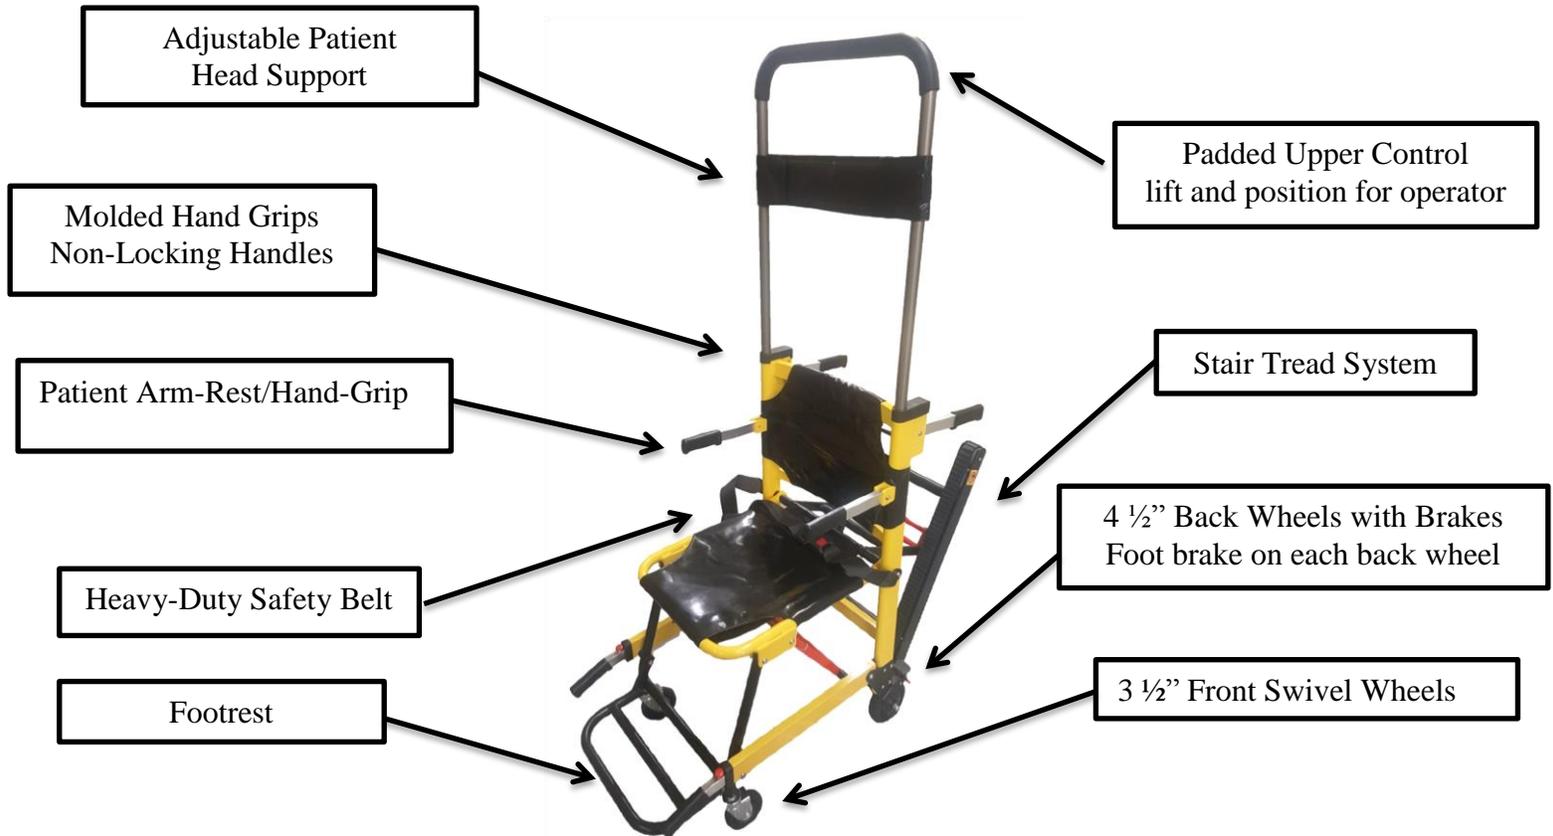

The handles in front of the Manual Track Stair Chair extend for easy transportation.

Push the red button to release the front handles.

Make sure the handles are fully extended, 14.25" and locked into position prior to use.

Specifications & Features
LINE2design Manual Track Stair Chair

Model #	70007-Y
Height:	64"
Width:	21. 1/2 "
Length:	49"
Weight:	40 lbs
Max. Load:	400 lbs

- Molded Hand Grips
- Heavy-duty seat restraint for patient safety
- 4 1/2 " Rear wheels for smoother transportation
- 3 1/2 " Front swivel wheels
- Adjustable head support
- Two rear wheel foot brakes
- Easy set-up
- Folds compactly for efficient storage
- Manual Track Stair Chair Tread System for controlled transportation down stairs
- Bright yellow for high visibility



Non-locking handles lift up to transport patient
 Handles fold down for storage

Track angle with 3 position adjustment
 To transport a patient: Push red bar towards chair, then pull up to extend the Track out until it locks into place.
 When storing the chair: Push Red bar towards chair and push all the way down until Track locks into place.
Always make sure Track is locked in place



Push in bar towards chair to raise or lower the upper handle
Always make sure upper handle is in position prior to use

Easy to adjust Patient Head Support



The handles in front of the Manual Track Stair Chair extend for easy transportation. Push down on red button to extend or retract.
Make sure the front handles are fully extended and locked into place before use.
Handle Length: 14.25"



**LINE2design, Inc. Manual Track Stair Chair Track Stair Chair - Yellow
Item # 70007-Y**



Rear Wheel Brakes
(both wheels)

To apply brakes:
Push down on red lever

To release brakes:
Push down on grey lever



Foot-rest for patient stability



3 1/2" Front Swivel Wheels

Patient Arm-Rest/Hand-Grips





**LINE2design, Inc. Manual Track Stair Chair Track Stair Chair - Yellow
Item # 70007-Y**

CLEANING AND STORING

- Clean the Manual Track Stair Chair with a clean cloth or soft brush and warm soapy water
- Rinse with warm water and air dry completely
- Do NOT clean with products containing bleach or phenol
- A stiff bristled brush can be used if necessary
- Always clean the chair before storing
- Make sure the chair is completely dry before storing
- Make sure there are no rocks or debris in the track before storing
- Make sure the chair is NOT damaged and working properly before storing
- Store in a clean and dry area
- Do Not Lubricate Manual Track Stair Chair System or any other part of the track system.
- Lubricants on the belts or track can cause the chair to perform unpredictably, resulting in injury to the patient and/or operators.
- If track or belts pick up oil or grease during use, clean the track and belts with a mild all-purpose cleaner before using the chair again.
- DO NOT lubricate the track on the Manual Track Stair Chair.

LINE2design, Inc.

1500 Crafton Avenue, Building 128
Mentone, CA 92359
909-798-1829

www.LINE2design.com
www.LINE2EMS.com

INSTRUCTIONS

LINE2design, Inc. MANUAL TRACK STAIR CHAIR-70007Y

Please keep these instructions for future reference. Store with the Stair Chair for reference and/or new users.

SETUP

- Remove all packaging materials before use
- NEVER modify the chair to fit in storage area/compartment



To Unfold Manual Track Stair Chair

1. Stand behind the chair
2. Apply wheel locks on both rear wheels
3. Pull the backrest and extension handle away from each other
4. Pull up on the seat to make sure that it is locked in the unfolded position
5. If the chair does not fold then the chair is locked

To Fold the Manual Track Stair Chair

1. Apply the wheel locks on both rear wheels
2. Buckle the restraint straps
3. Stand at the side of the chair and pull up on the red lock bar at the rear of the chair
4. Tip the chair forward
5. Fold the seat up to the backrest until the front legs lock into the clips on the bottom of the seat tube

NEVER
Use the Manual Track Stair Chair
with suspected cervical, spinal or
fracture injuries.

NEVER
Leave a patient unattended while in
the Manual Track Stair Chair.

LINE2design, Inc.

1500 Crafton Avenue, Building 128
Mentone, CA 92359
909-798-1829

www.LINE2design.com
www.LINE2EMS.com



LINE2design Manual Track Stair Chair Instructions

Always keep these instructions for future reference. Store with the Stair Chair for reference and/or new users.

TRANSPORTING PATIENTS

- Using the chair to move up stairs requires a minimum of two trained operators working together.
- Use additional help as needed to control the chair.
- LINE2design recommends that the two operators face each other when transporting a patient on stairs and that a third trained person, “spot” for the head-end operator.
- Follow your local protocols when using the Manual Track Stair Chair.
- Remove any water, ice, snow, or debris from the stairs before using the stair chair.
- Remove any water, ice, snow, or debris from the track system and belts before using the chair on stairs.
- Verify that the track system is locked in the open position before using the chair on stairs.

TRANSPORTING PATIENT DOWN STAIRS

1. Always transport a patient on the Manual Track Stair Chair with a minimum of two operators.
2. Using a third person as a helper/spotter is highly recommended.
3. Apply and adjust the patient head-rest to fit directly behind the patients head.
4. Buckle seat-belt and make sure the patient is secure before moving the chair.
5. Roll the chair to the stairs and align it with the edge of the first step.
6. Foot-end operator: Push the release buttons to extend the foot end lift handles and extend the handles until they lock into place.
7. Head-end operator: Use one hand to push the red bar in and pull up, use the other hand to pull up and fully extend the handle. Release the handle and make sure that the handle is locked on both sides in the fully extended position.
8. Push forward the red track release bar against the back of the chair. Relax your grip on the release bar and forcefully pull the Manual Track Stair Chair system to a fully extended position until both sides lock securely. Always make sure that both sides of the Track Stair Chair tread system are locked by trying to fold it back up.
9. Operators face each other while descending stairs.
10. Head-end Operator: Tilt the chair back just far enough to allow the tread system to contact the floor.
11. Both operators: Glide down the stairs until the treads are level across the edges of two or three steps.
 - Head-end Operator: Apply slight downward pressure on the extendable upper control handle while the
 - Foot-end Operator applies slight upward pressure on the foot end lift handles to keep the chair from rocking forward as it glides down the stairs.
12. Foot-end Operator: When the track reaches the last step, release the front handles.
13. Head-end Operator: Allow the chair to tip forward until all four wheels are on the ground. Roll the chair.



LINE2design Manual Track Stair Chair Instructions

TRANSPORTING PATIENT UP STAIRS

1. Using the chair to move up stairs requires a minimum of two trained operators working together.
2. Use additional help as needed to control the chair.
3. LINE2design recommends that the two operators face each other when transporting a patient on stairs and that a third trained person, “spot” for the head-end operator.
4. Follow your local protocols for using stair chairs.
5. Remove any water, ice, snow, or debris from the stairs before using the chair.
6. Remove any water, ice, snow, or debris from the track system and belts before using the stair chair on stairs.
7. Verify that the track system is locked in the open position before using the chair on stairs.
8. Both Operators: Roll the chair backward near the bottom of the stairs and engage the wheel locks.
9. Open the track system and verify that it is locked.
10. Operators raise the lift bar and/or extend the foot-end lift handles to the desired positions and verify that all handles are locked into place.
11. If using a third person: Stand above the head-end operator with a hand on the operator’s back to help steady and guide him/her throughout the ascent.
12. Head-end Operator: Disengage the wheel locks.
13. Both Operators: Together, tilt the chair back until the top of the track belts touch the edge of the lowest step of the stairway.
14. Head-End Operator: Make sure the track system is aligned with the stairs and start the belts moving in the proper direction to ascend the stairs.
15. Both Operators: Together, guide the chair to climb the stairway. The tracks should engage two or three steps. This establishes the glide angle.



If either operator needs to pause or rest while descending or ascending the stairs, tilt the chair forward just enough to allow the rear wheels to rest on the tread of the stair. To continue down the stairs from the resting position, the Head-end Operator will exert slight downward pressure on the upper control handle while the Foot-end Operator provides slight upward pressure to tilt the chair back and activate the Manual Track Stair Chair system.



OPERATION GUIDELINES
LINE2design, Inc. MANUAL TRACK STAIR CHAIR-70007Y

Please keep these instructions for future reference. Store with the Stair Chair for reference and/or new users.

- Only operate the LINE2design Manual Track Stair Chair as outlined in the instructions.
- Operator trainees need to:
 - Read and understand this manual.
 - Be trained on the use of the chair.
 - Practice with the chair before using it with a patient.
 - NEVER use the chair with untrained operators.
- Operators using the chair need: a working knowledge of emergency patient-handling procedures, and the ability to assist the patient.
- Always use two trained personnel when operating the Manual Track Stair Chair. A third person as a helper/spotter is recommended.
- Only use the wheel locks during patient transfer in and out of the chair.
- Always use all restraint straps to secure the patient in the Manual Track Stair Chair prior to use. An unrestrained person may fall and be injured.
- Do not attempt to transport patient loads greater than what you can safely lift.
- Always advise the patient before you move the chair, ascend or descend stairs.
- Always stay with the patient, and keep control of the chair at all times.
- To avoid tipping, do not apply a wheel lock when the Manual Track Stair Chair is in use or when moving.
- Always insure that the tracking system is locked before transporting a patient.
- Condensation, water, ice, or debris on the track system of the Manual Track Stair Chair can cause unpredictable performance that may result in sudden change of the weight that the operators must support.
- Avoid getting dirt or other debris inside the tracks.
- The Manual Track Stair Chair may not work properly on all stair surfaces and in all weather conditions. You may encounter varying degrees of resistance. Water, ice or debris on the stairs can affect the operator's footing and proper operation of the Manual Track Stair Chair.
- Always make sure the path is clear or use an alternate route.
- DO NOT modify the Manual Track Stair Chair; only use the chair as built and assembled by LINE2design.
- Before and after each use ensure the Manual Track Stair Chair is working properly and in good condition.

LINE2design, Inc.

1500 Crafton Avenue, Building 128
Mentone, CA 92359
909-798-1829

www.LINE2design.com
www.LINE2EMS.com