# **Safe**Basics™







# **TECHNICAL DATA SHEET**

## **FEATURES & BENEFITS**

- Non-woven spunbond outer layer provides maximum protection against fluid penetration.
- Soft, strong, ultrasonically sealed earloops attached to outside of mask prevent pulling and irritation and allow easy removal with less risk of self-contamination.
- o Shingle pleat design prevents fluid pooling and cross-contamination.
- o High-quality media ensures optimal filtration and breathability.
- Adjustable, enclosed nosepiece forms a strong seal to provide customized protection and comfort.

### RECOMMENDED USE

 Procedure masks are intended to be worn by personnel during medical procedures to protect both the patient and the operating personnel from transfer of microorganisms, body fluids and particulate material transfer. Latex free.

## PRODUCT DETAILS

Product Name: Medicom SafeBasics™

**Procedure Earloop Face Mask** 

Product Type: Single-use, non-sterile, three-layer construction

Earloop: Polyester and spandex
Nosepiece: Plastic-covered iron
Colour: See Appendix 1

Quantity per Inner Carton: 50 Country of Origin: China


ITEM	COLOUR	DIMENSIONS
	Blue	175 (+/- 5 mm)
2151		90,5 (+/- 5 mm)




DETAILED MASK DIM	ENSIONS		
Length of Earloop	165 mm		
Pleat Depth			
Length of Nose-piece	105 mm		



ASTM F2100 - LEVEL 3 BARRIER PROTECTION								
PERFORMANCE FACTORS	TEST METHODS	RESULT						
Bacterial filtration efficiency (BFE)	ASTM F2101	≥ 98%						
Sub-micron particulate efficiency at 0.1µm (PFE) /	ASTM F2299	≥ 98%						
Resistant to penetration by synthetic blood	ASTM F1862	@ 160 mm Hg						
Differential Pressure (ΔP)	EN 14683	< 6.0 mm H <sub>2</sub> O/cm <sup>2</sup>						
Flame Spread	16 CF 1610	Class 1						

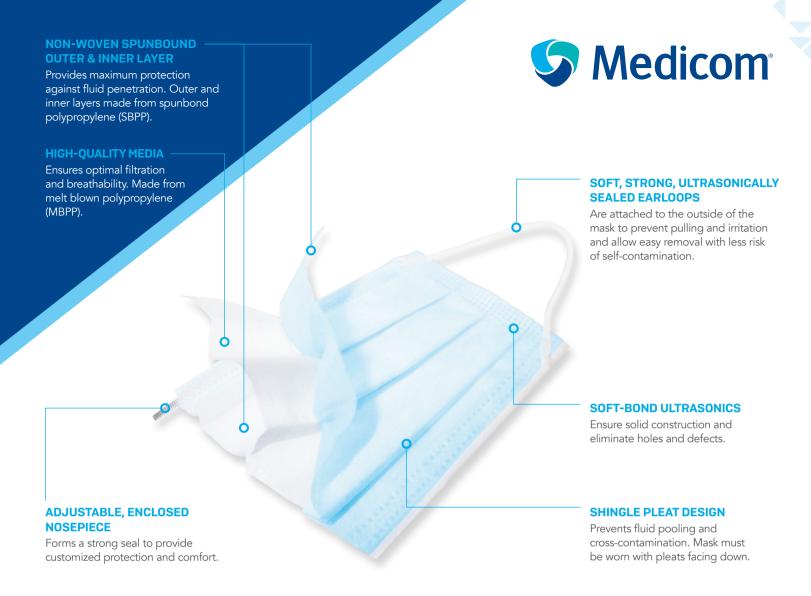

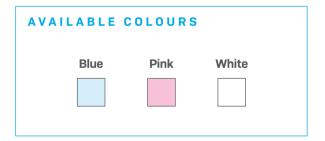

### **CERTIFICATION & STANDARDS**

ISO 13485 certified manufacturer. Class 1 Medical Device.

Health Canada registered medical device manufacturer.

### STORAGE CONDITIONS

These masks should be disposed of after each use. Store in a cool, dry place. Avoid excessive heat (40 °C or 104 °F).





## **DONNING INSTRUCTIONS**

- o Fan to open pleats.
- o Shape before applying to ensure a better fit.
- o Pull earloops over each ear.
- With two fingers on either side of your nose, firmly shape around your nose and across your cheeks, concentrating on the bridge of your nose, to secure the seal.
- Pinch the nosepiece and make sure the base of the mask sits comfortably below your chin.

### **DOFFING INSTRUCTIONS**

- o Pull the earloops off your ears.
- Pull the mask away from your face, taking care not to touch its outer surface.
- Still holding only the earloops and taking care not to touch outer surface, dispose of mask in a clinical waste bin.
- o Always wash your hands thoroughly after removing a mask.



Appendix 1 (List of items)										
Item Code	Description	Packaging Information	Color	Specific Attribute	Treatment	Marketed in USA as	Marketed in Canada as			
2150	Medicom Safebasics Procedure Earloop Face Masks	50 Masks/Box, 10 Boxes/Case, 500 Masks/Case	White	Plastic Covered Iron Nose-piece, Flat Knitted Earloop, Regular Earloop Length	Non-Sterile	Medical Device Class 2	Medical Device Class 1			
2151	Medicom Safebasics Procedure Earloop Face Masks	50 Masks/Box, 10 Boxes/Case, 500 Masks/Case	Blue	Plastic Covered Iron Nose-piece, Flat Knitted Earloop, Regular Earloop Length	Non-Sterile	Medical Device Class 2	Medical Device Class 1			
2152	Medicom Safebasics Procedure Earloop Face Masks	50 Masks/Box, 10 Boxes/Case, 500 Masks/Case	Pink	Plastic Covered Iron Nose-piece, Flat Knitted Earloop, Regular Earloop Length	Non-Sterile	Medical Device Class 2	Medical Device Class 1			

AMD Medicom Inc. | 2555 Chemin de l'Aviation, Montreal, Quebec, Canada H9P 2Z2

APP1 06.03-41EN\_1M Date: 04-Feb-2022 Page 1 / 1