


GP-20/21 Underhook

Applicable models: GP-20 (GP-12K/20K/22K/30K/40K/30KS)
GP-21 (GP-60K/100K/102K/100KS)


The GP-20/21 is the underhook for the GP series balance for measuring density.

Assembling


(1) Remove the underhook cover.

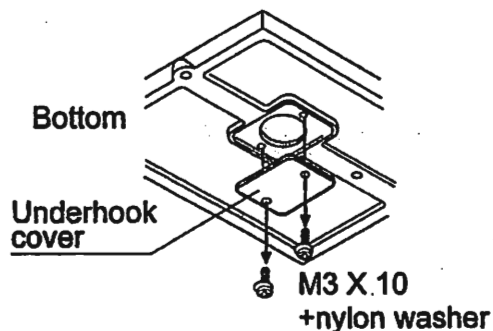

(2) Fasten the underhook to the GP sensor unit gently.

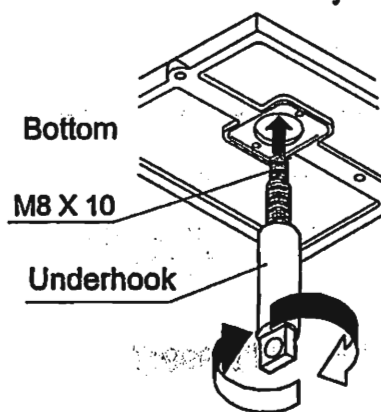


(3) Screw the guide to the bottom of the GP gently.
Make sure that the underhook does not touch the underhook guide.

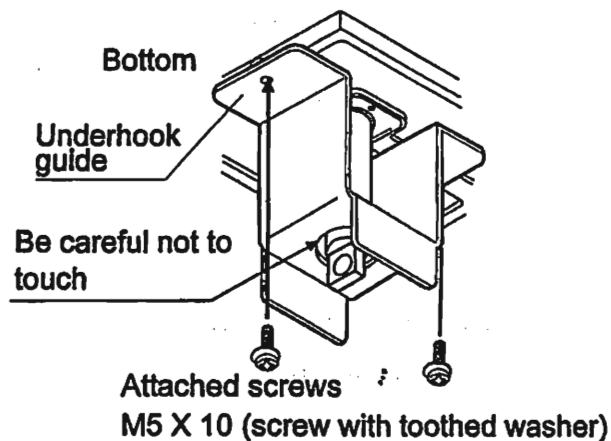

(4) Place the GP balance on a weighing table with a hole cut in it.

(5) Hang a lightweight weighing harness through this hole.

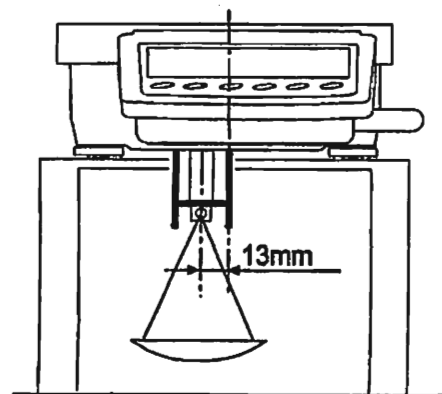

AND


An Example of Underhook Weighing

A weight of metal immersed in a liquid decreases by the weight of the liquid it displaces (Archimedes' Principle). Therefore you can obtain the volume and the density.

- (1) Place the material on the pan.

Find the weight A of the material in air. $A=10000.0g$

- (2) Press the **RE-ZERO** key.

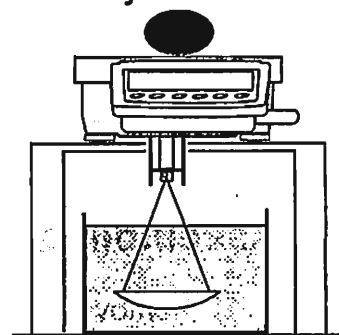

$A=10000.0g$

- (3) Lower the material into water at 10 °C.


Find the absolute weight B of the material in water. $B=466.1g$

- (4) Find the water density C from following table. $C=466.2cm^3$

0 °C	0.99984 g/cm ³
4	0.99997
10	0.99970
15	0.99910
20	0.99820
25	0.99704
30	0.99565 Reference

$$\frac{466.1g}{0.99970g/cm^3} = 466.2cm^3$$

$C=466.2cm^3$

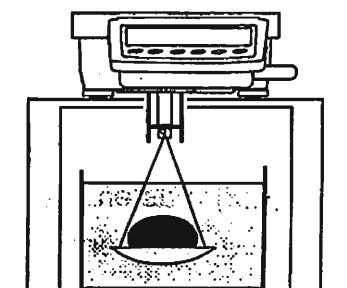

$B=|-466.1g|$
 $=466.1g$

- (5) The density is 21.45 g/cm³. This material is most likely platinum.

$$\frac{10000.0g}{466.2g/cm^3} \approx 21.45g/cm^3$$

NOTE: For measuring density, refer to "13. DENSITY MEASUREMENT" of the GP series instruction manual.