

www.abstraxtech.com | info@abstraxlabs.com | 15550 Rockfield Blvd, Suite B120 | Irvine, CA 92618


	C	Certificate of Analysis			
	Name: Matrix: Lot #: Product #:		Manufac Expiratio Overall F		
Test	Specific	cation		Resu	ult
Appearance					
rith ASTM E 542 and NIST Proced ometers and temperature probes are ording to master documents that as y for each lot manufactured.	erance requirements of ASTM E 288 a ure NBSIR 74-461. Balances are calib e calibrated before first use and recalil ssure manufacture according to valida	rated regularly with weig brated regularly with a th ated methods. Batch reco	thts certified t hermometer to	raceable to the NIS raceable to NIST sta t raw material trace	T national ma andards. All pr ability and pro
with ASTM E 542 and NIST Proced ometers and temperature probes an ording to master documents that as by for each lot manufactured. Specific Gravity @ 25 °C	ure NBSIR 74-461. Balances are calible calibrated before first use and recalibesure manufacture according to validate specifical spe	rated regularly with weig brated regularly with a th ated methods. Batch reco	thts certified t hermometer to	raceable to the NIS raceable to NIST sta t raw material trace Resi	T national mas andards. All pr ability and pro
with ASTM E 542 and NIST Proced ometers and temperature probes an cording to master documents that as ry for each lot manufactured.	ure NBSIR 74-461. Balances are calib e calibrated before first use and recalib ssure manufacture according to valida	rated regularly with weig brated regularly with a th ated methods. Batch reco	thts certified t hermometer to	raceable to the NIS raceable to NIST sta t raw material trace	T national mas andards. All pr ability and pro
with ASTM E 542 and NIST Proced ometers and temperature probes an ording to master documents that as my for each lot manufactured. Specific Gravity @ 25 °C Gas Chromatograph	ure NBSIR 74-461. Balances are calible calibrated before first use and recalibesure manufacture according to validate specifical spe	rated regularly with weig brated regularly with a th ated methods. Batch reco	thts certified t hermometer to	raceable to the NIS raceable to NIST sta t raw material trace Resi	T national mas andards. All pr ability and pro
with ASTM E 542 and NIST Proced nometers and temperature probes are cording to master documents that as ry for each lot manufactured. Specific Gravity @ 25 °C	ure NBSIR 74-461. Balances are calible calibrated before first use and recalibesure manufacture according to validate specifical spe	rated regularly with weig brated regularly with a th sted methods. Batch reco cation	thts certified t hermometer to	raceable to the NIS raceable to NIST sta t raw material trace Resi	T national mas andards. All pr ability and pro

Methylene Chloride

Pentane

Ethanol

Ethyl Acetate

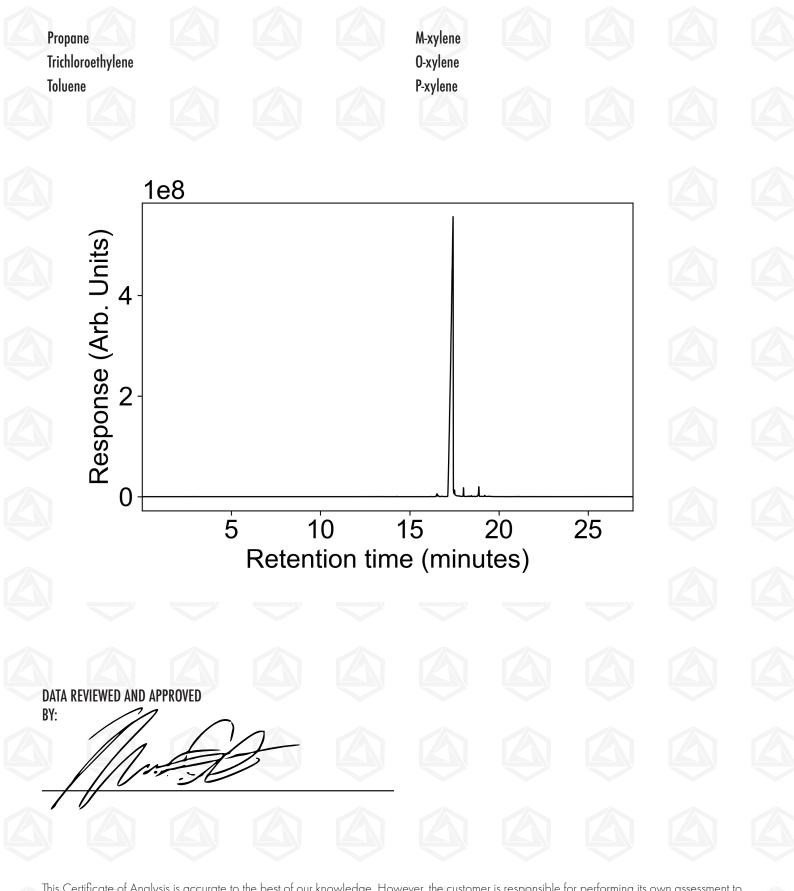

This Certificate of Analysis is accurate to the best of our knowledge. However, the customer is responsible for performing its own assessment to ensure that the material is suitable for its intended applications, including compliance with all pertinent legal requirements. The expected shelf life is calculated from the original manufacture date and is based on unopened containers stored under proper conditions. Once containers have been opened, maintaining minimal headspace and storing under appropriate conditions will aid in preserving the product's integrity.